

Standard Name 109 of 118

↑

19106/190293D-A

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 22-Dec-23 Time: 10:28:08

Batch Name 1 of 1

↑

4070004IR-01 117956 EXP2400024 GRAPHITE

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal


Date: 12-Feb-24 Time: 13:19:05

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
DKF19106 24070004IR-01 117956 EXP2400024 GRAPHITE	D65 10 Deg	0.85	0.08	0.32	0.60	-0.42	0.19	0.76		Warn	too light	too dull	too red
DKF19106 24070004IR-01 117956 EXP2400024 GRAPHITE	F11 10 Deg	0.87	0.37	0.42	0.63	-0.69	0.26	0.97	0.33	Pass	too light	too dull	too red

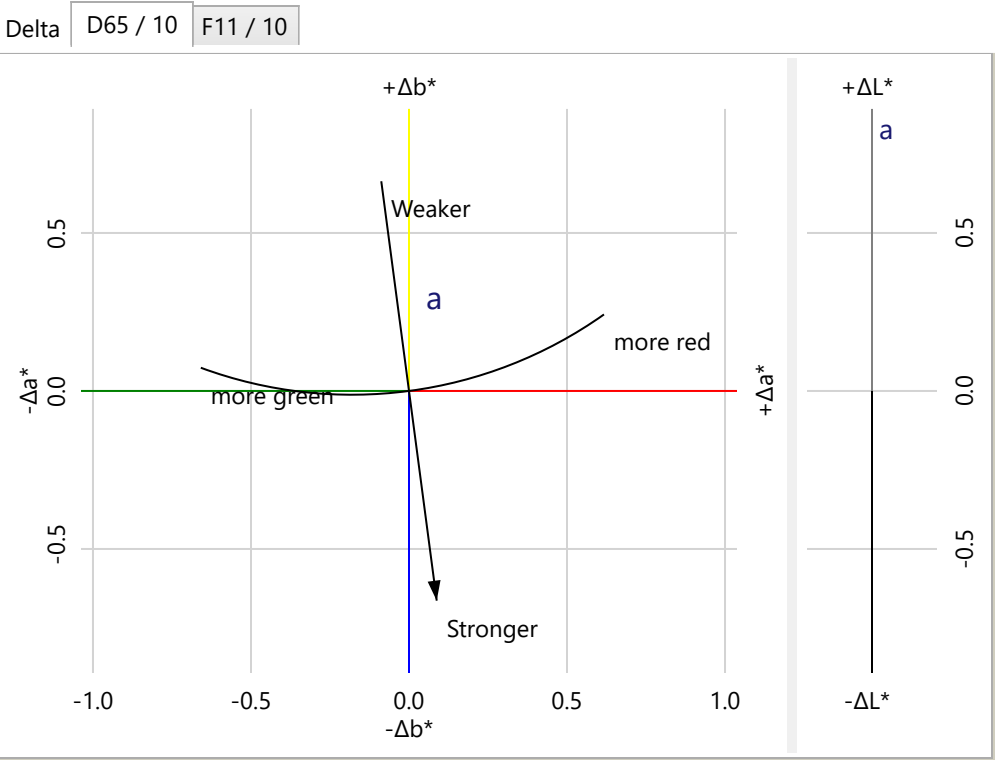

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form