

Standard Name    467   of   474

↑

18157/200331M-C

↓

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup:%R LAV   SCI UV Cal

Date: 01-Aug-23                      Time: 00:54:11

Batch Name                      2   of   2

↑

2218265 5366657 85365 DOM2300838 ROVER

↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV   SCI UV Cal


Date: 03-Aug-23                      Time: 11:44:46

CMC DE Pass/Fail Tolerance:      1.00

I:c Ratio: (   2.00   1.00 )

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments		
R2218265 5366657 85365 DOM2300838 ROVER	D65 10 Deg	-1.25	0.12	0.37	-0.62	0.40	-0.11	0.74		Pass	too dark	too bright	too red
R2218265 5366657 85365 DOM2300838 ROVER	F11 10 Deg	-1.27	0.22	0.34	-0.62	0.34	-0.31	0.77	0.09	Warn	too dark	too bright	too red
R2218265 5366657 85365 DOM2300838 ROVER	A 10 Deg	-1.22	0.15	0.39	-0.60	0.41	0.05	0.73	0.09	Pass	too dark	too bright	too yellow

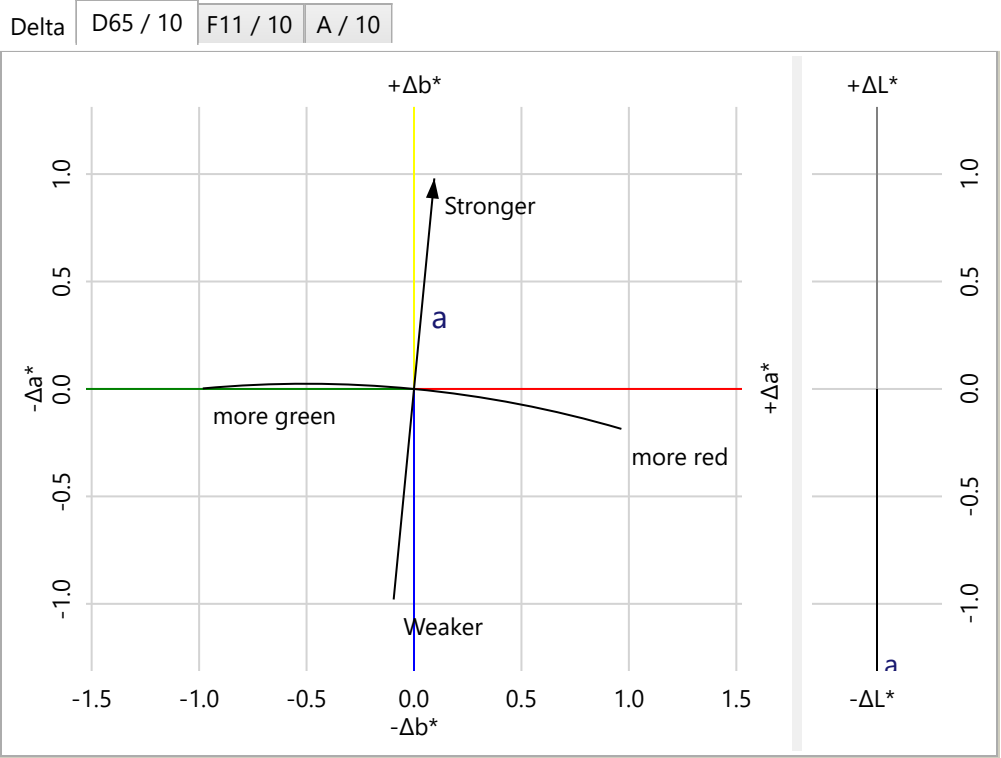

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form