

Standard Name 30 of 76

↑

19106/230152M-B

↓

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup:%R LAV SCI UV Cal

Date: 13-Mar-23 Time: 10:45:23

Batch Name 5 of 5

↑

R2213455 24050171IR-01 118987 EXP2400010

↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal


Date: 07-Feb-24 Time: 11:25:51

CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color	Comments	
R2213455 24050171IR-01 118987 EXP2400010	D65 10 Deg	-0.61	0.07	0.54	-0.30	0.20	-0.57	0.67		Warn	too dark	too bright	too yellow
R2213455 24050171IR-01 118987 EXP2400010	F11 10 Deg	-0.56	0.10	0.64	-0.27	0.20	-0.68	0.76	0.12	Pass	too dark	too bright	too yellow

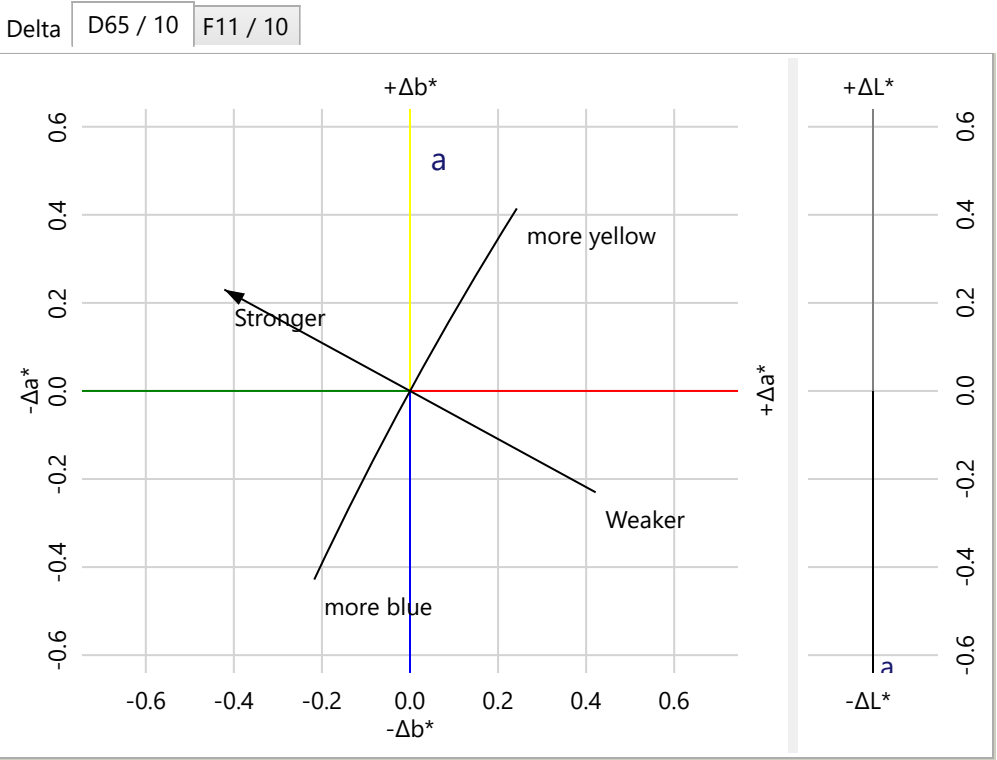

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form