

Standard Name38 of 63

↑

17109/210497S-B

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV SCI UV Cal

Date: 30-Dec-22Time: 08:20:02

Batch Name3 of 3

↑

2 4501932443 104924 EXP2300888 TRUE RED

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV SCI UV Cal


Date: 21-Dec-23Time: 14:59:30

CMC DE Pass/Fail Tolerance:0.80

I:c Ratio: ( 2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/F	Color	Comments	
HJY18402 4501932443 104924 EXP2300888 TRUE RED	D65 10 Deg	0.19	-0.76	-1.15	0.10	-0.42	-0.43	0.61		Warn	too light	too dull	too blue
HJY18402 4501932443 104924 EXP2300888 TRUE RED	F11 10 Deg	0.09	-0.57	-1.31	0.04	-0.42	-0.53	0.67	0.32	Pass	too light	too dull	too blue

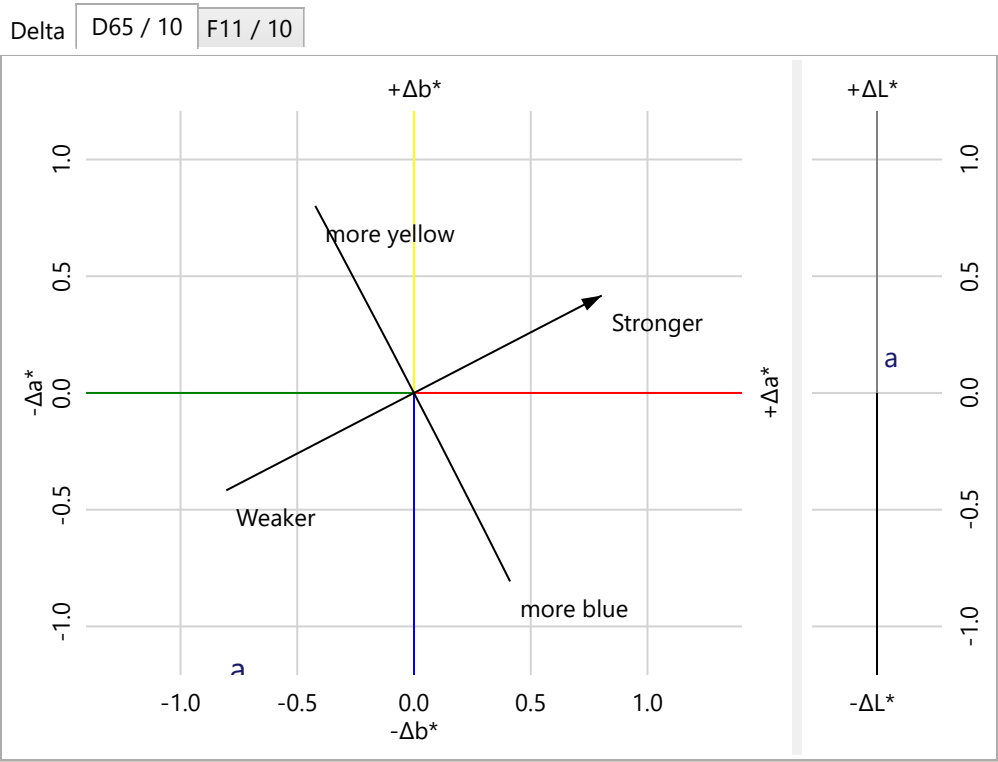

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form