

Standard Name    484   of   509

↑

19106/230098L-B

↓

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup:%R LAV   SCI UV Cal

Date: 13-Mar-23                      Time: 10:39:22

Batch Name                      1       of       3

↑

3120113IC-01 83437 EXP2300602 SUNDANCE

↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV   SCI UV Cal


Date: 07-Aug-23                      Time: 11:22:22

CMC DE Pass/Fail Tolerance:       1.00

I:c Ratio: (   2.00   1.00 )

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments			
DKF19106 23120113IC-01 83437 EXP2300602 SUNDANCE	D65 10 Deg	-0.15	-0.33	-0.90	-0.05	-0.56	0.46	0.72		Pass	too dark	too dull	too blue	
DKF19106 23120113IC-01 83437 EXP2300602 SUNDANCE	F11 10 Deg	-0.22	-0.35	-1.06	-0.08	-0.65	0.41	0.77	0.18	Warn	too dark	too dull	too green	
DKF19106 23120113IC-01 83437 EXP2300602 SUNDANCE	A 10 Deg	-0.24	-0.50	-1.03	-0.08	-0.71	0.44	0.84	0.22	Warn	too dark	too dull	too green	

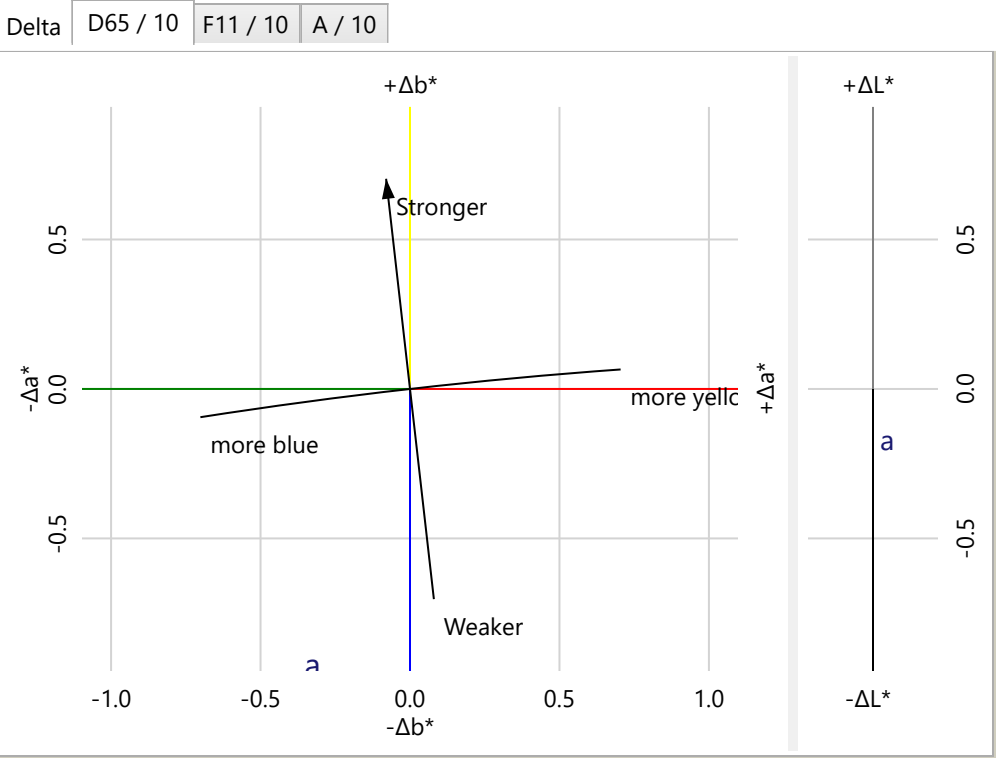

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form