

VENDOR NAME

▼

▼

TECHNICIAN

Standard Name

41 of 41



A0TB Bright Red CONST FW14



Hue Preference:

red (yellowish)

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup: %R LAV SCI UV Cal

Batch Name

1 of 1



I-00663 108187 DOM2301392 A0



New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Date: 13-Dec-23

Time: 15:54:33

Instrument Setup: %R LAV SCI UV Cal


CMC DE Pass/Fail Tolerance: 0.80

I:c Ratio: (2.00 1.00)

Delta CMC

D65 / 10

F11 / 10

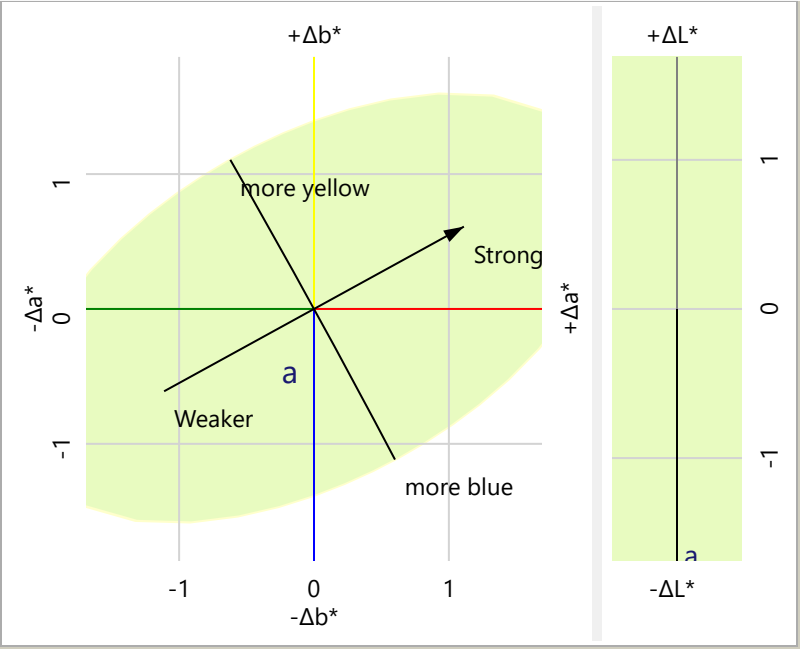

Single/All

Zoom In

Zoom Out

CMC Plot

Print Form

Store All Bats

Batch Name		III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	Status	Metamerism	Color Comments		
60044210	231111-SS24-FI-00663 108187 DOM2301392 A0	D65 10 Deg	-1.61	-0.19	-0.41	-0.73	-0.12	-0.17	0.76	Pass		darker	too dull	more blue
60044210	231111-SS24-FI-00663 108187 DOM2301392 A0	F11 10 Deg	-2.22	-1.72	-1.65	-0.95	-0.78	-0.25	1.25	Fail	2.04	darker	too dull	more blue