

VENDOR NAME

TECHNICIAN

Standard Name31 of 41

↑

AESW Silver PebbleS23

↓

Hue Preference: YELLOW/GREENISH

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup: %R LAV SCI UV Cal

Batch Name1 of 1

↑

3 112696 SAM2300226 AESW SI

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat


Date: 13-Dec-23Time: 16:06:59

Instrument Setup: %R LAV SCI UV Cal

CMC DE Pass/Fail Tolerance: 0.80

l:c Ratio: (2.00 1.00)

Delta CMC D65 / 10 F11 / 10

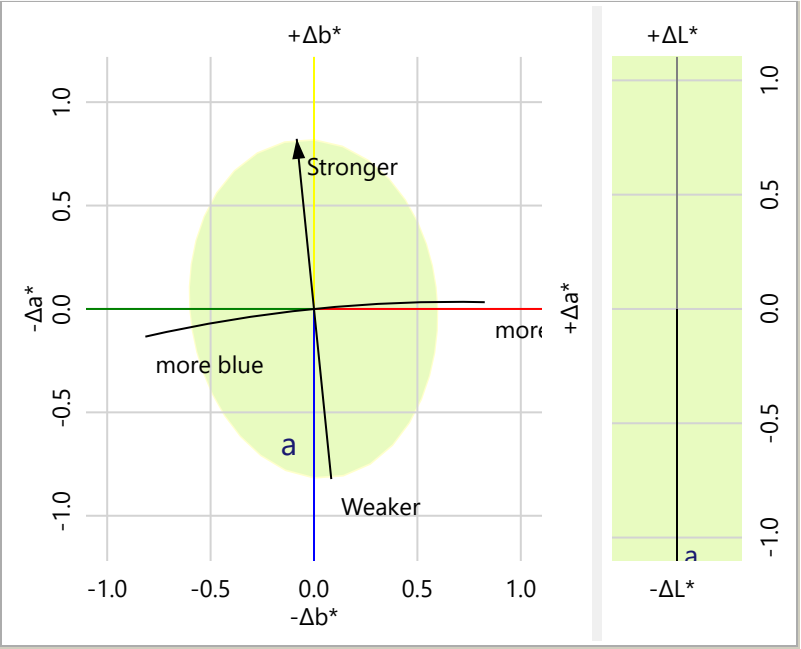

Single/All

Zoom In

Zoom Out

CMC Plot

Print Form

Store All Bats

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	Status	Metamerism	Color Comments		
70005871 POPS2306A/E0063 112696 SAM2300226 AESW SI	D65 / 10 Deg	-1.04	-0.13	-0.62	-0.46	-0.58	0.26	0.78	Pass		darker	too dull	more blue
70005871 POPS2306A/E0063 112696 SAM2300226 AESW SI	F11 / 10 Deg	-1.31	0.72	-0.76	-0.57	-0.84	-0.65	1.21	Fail	0.89	darker	too dull	more yellow