

Standard Name 127 of 127

DataColor TOOLS 2.8.1

S/N NO. 8823242

18157/210974D-C

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal

Date: 14-Dec-22 Time: 10:57:09

Batch Name 1 of 1

027004AA-004 51337 DOM2300049 MAIZE YEL

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------


Instrument Setup: %R LAV SCI UV Cal

Date: 28-Feb-23 Time: 09:41:24

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

Measured by: ▼

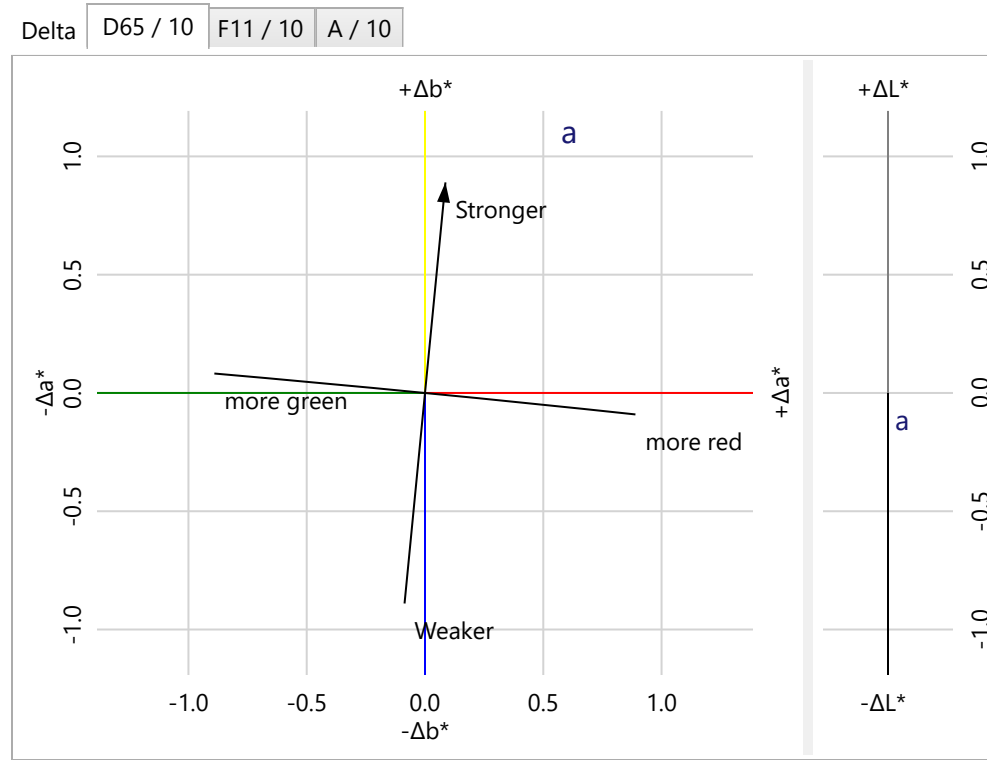

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/F	Color	Comments	
SJS7091 B23027004AA-004 51337 DOM2300049 MAIZE YEL	D65 10 Deg	-0.09	0.61	1.13	-0.03	0.36	-0.27	0.45		Pass	too dark	too bright	too red
SJS7091 B23027004AA-004 51337 DOM2300049 MAIZE YEL	F11 10 Deg	-0.08	0.59	1.12	-0.03	0.34	-0.26	0.43	0.06	Pass	too dark	too bright	too red
SJS7091 B23027004AA-004 51337 DOM2300049 MAIZE YEL	A 10 Deg	-0.01	0.48	1.12	-0.00	0.36	-0.16	0.39	0.23	Pass	too dark	too bright	too red