

Standard Name 87 of 113

↑

18157/191081D-D

↓

Visual Hue Request:

New Std	Retrieve Std	Store Std	List Std	Update Std
---------	--------------	-----------	----------	------------

Instrument Setup:%R LAV SCI UV Cal

Date: 28-Jun-23 Time: 13:24:38

Batch Name 4 of 5

↑

5365133 88322 DOM2300806 ACT RESUBMIT

↓

New Bat	Retrieve Bat	Store Bat	List Bat	Update Bat
---------	--------------	-----------	----------	------------

Instrument Setup: %R LAV SCI UV Cal


Date: 08-Sep-23 Time: 09:31:45

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

Measured by:

Batch Name	III/Obs	DL*	Da*	Db*	DL*/ISL	DC*/cSC	DH*/SH	CMC DE	M.I.	P/E	Color Comments		
HJY20124 5365133 88322 DOM2300806 ACT RESUBMIT	D65 10 Deg	0.31	0.94	0.08	0.17	0.49	-0.52	0.74		Pass	too light	too bright	too blue
HJY20124 5365133 88322 DOM2300806 ACT RESUBMIT	F11 10 Deg	0.38	0.99	0.19	0.20	0.51	-0.57	0.80	0.12	Pass	too light	too bright	too blue
HJY20124 5365133 88322 DOM2300806 ACT RESUBMIT	A 10 Deg	0.42	0.79	0.30	0.22	0.43	-0.32	0.58	0.30	Pass	too light	too bright	too red

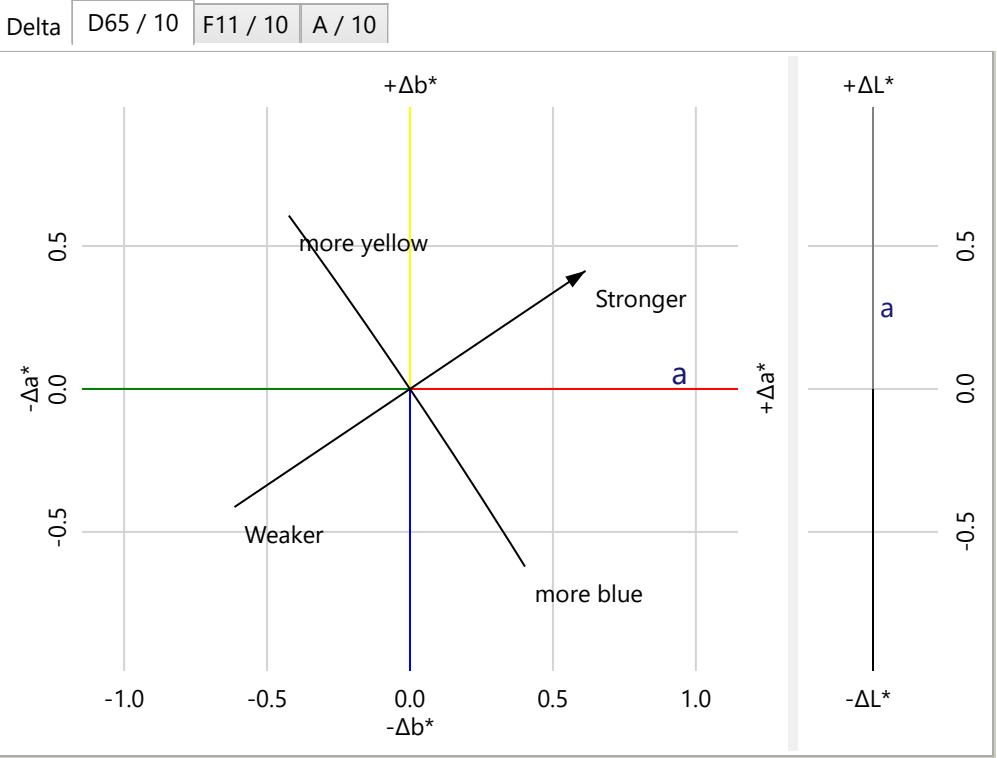

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form