

Standard Name    415   of   415

↑

18157/220766S-A

↓

Visual Hue Request:

New Std

Retrieve Std

Store Std

List Std

Update Std

Instrument Setup:%R LAV   SCI UV Cal

Date: 18-Nov-22                      Time: 14:06:04

Batch Name                      1           of           1

↑

24 4501828921 79729 EXP2300538 SPICY RED

↓

New Bat

Retrieve Bat

Store Bat

List Bat

Update Bat

Instrument Setup: %R LAV   SCI UV Cal


Date: 20-Jul-23                      Time: 15:58:06

CMC DE Pass/Fail Tolerance:        1.00

I:c Ratio: (   2.00   1.00 )

Measured by:

| Batch Name                                     | III/Obs    | DL*  | Da*   | Db*   | DL*/ISL | DC*/cSC | DH*/SH | CMC DE | M.I. | P/E  | Color Comments |          |          |
|--|------------|------|-------|-------|---------|---------|--------|--------|------|------|----------------|----------|----------|
| HJY20124 4501828921 79729 EXP2300538 SPICY RED | D65 10 Deg | 1.11 | -0.14 | -0.42 | 0.54    | -0.10   | -0.20  | 0.59   |      | Pass | too light      | too dull | too blue |
| HJY20124 4501828921 79729 EXP2300538 SPICY RED | F11 10 Deg | 1.19 | -0.15 | -0.19 | 0.55    | -0.08   | -0.06  | 0.56   | 0.17 | Pass | too light      | too dull | too blue |
| HJY20124 4501828921 79729 EXP2300538 SPICY RED | A 10 Deg   | 1.07 | 0.15  | -0.60 | 0.48    | -0.08   | -0.39  | 0.62   | 0.71 | Pass | too light      | too dull | too blue |

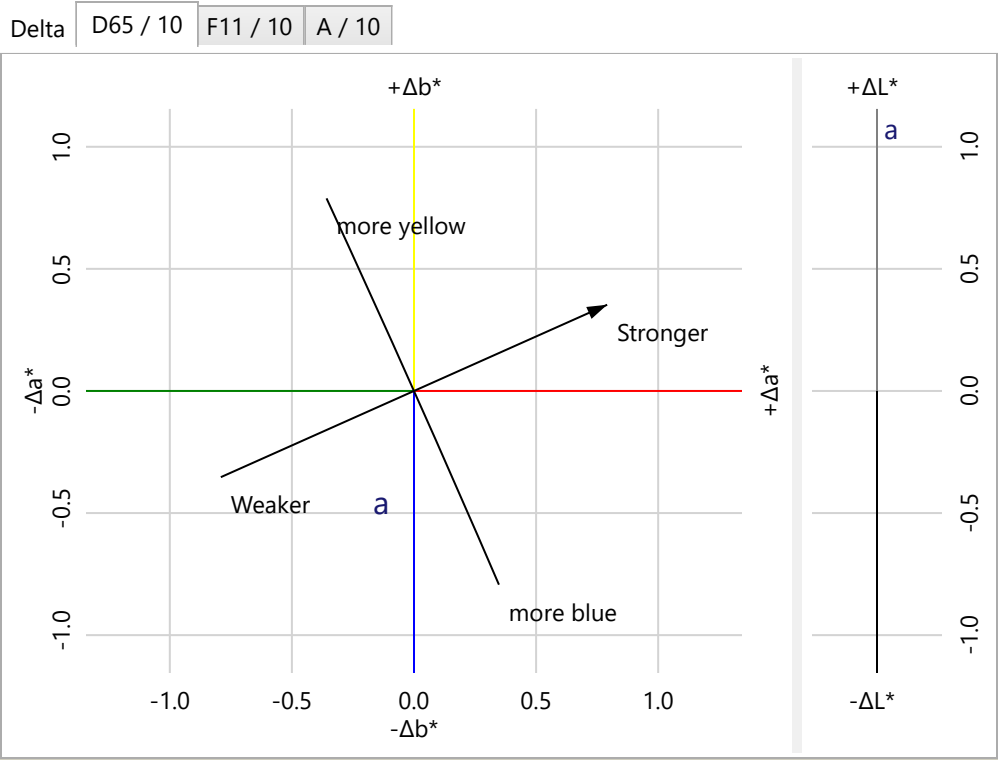

Single/All

CMC Plot

Zoom Out

Zoom In

Print Form