

Standard Name 120 of 127

DataColor TOOLS 2.8.1

S/N NO. 8823242

20124/210280D-D

Visual Hue Request:

| | | | | |
|---------|--------------|-----------|----------|------------|
| New Std | Retrieve Std | Store Std | List Std | Update Std |
|---------|--------------|-----------|----------|------------|

Instrument Setup: %R LAV SCI UV Cal

Date: 11-Oct-22 Time: 15:56:39

Batch Name 1 of 2

↑ 0179-A01ACB 55010 EXP2300146 ESPRESSO ↓

| | | | | |
|---------|--------------|-----------|----------|------------|
| New Bat | Retrieve Bat | Store Bat | List Bat | Update Bat |
|---------|--------------|-----------|----------|------------|


Instrument Setup: %R LAV SCI UV Cal

Date: 27-Feb-23 Time: 08:59:35

CMC DE Pass/Fail Tolerance: 1.00

I:c Ratio: (2.00 1.00)

Measured by: ▼

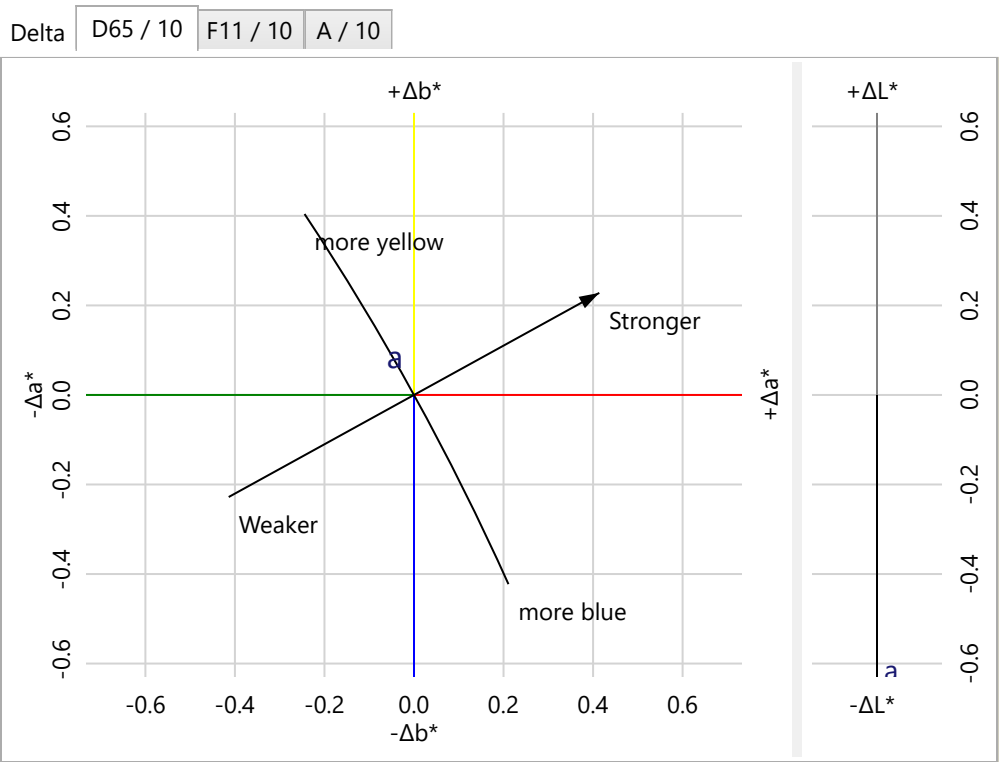

- Single/All
- CMC Plot
- Zoom Out
- Zoom In
- Print Form

| Batch Name | III/Obs | DL* | Da* | Db* | DL*/ISL | DC*/cSC | DH*/SH | CMC DE | M.I. | P/E | Color | Comments |
|--|---------|-------|------|-------|---------|---------|-------------|--------|------|----------|------------|------------|
| HJY20124 LU00179-A01ACB 55010 EXP2300146 ESPRESSO D65 10 Deg | -0.60 | -0.05 | 0.10 | -0.47 | 0.01 | 0.16 | 0.49 | | Pass | too dark | too bright | too yellow |
| HJY20124 LU00179-A01ACB 55010 EXP2300146 ESPRESSO F11 10 Deg | -0.63 | -0.01 | 0.02 | -0.49 | 0.01 | 0.03 | 0.49 | 0.08 | Pass | too dark | too bright | too yellow |
| HJY20124 LU00179-A01ACB 55010 EXP2300146 ESPRESSO A 10 Deg | -0.59 | 0.09 | 0.10 | -0.45 | 0.12 | 0.06 | 0.47 | 0.17 | Pass | too dark | too bright | too yellow |