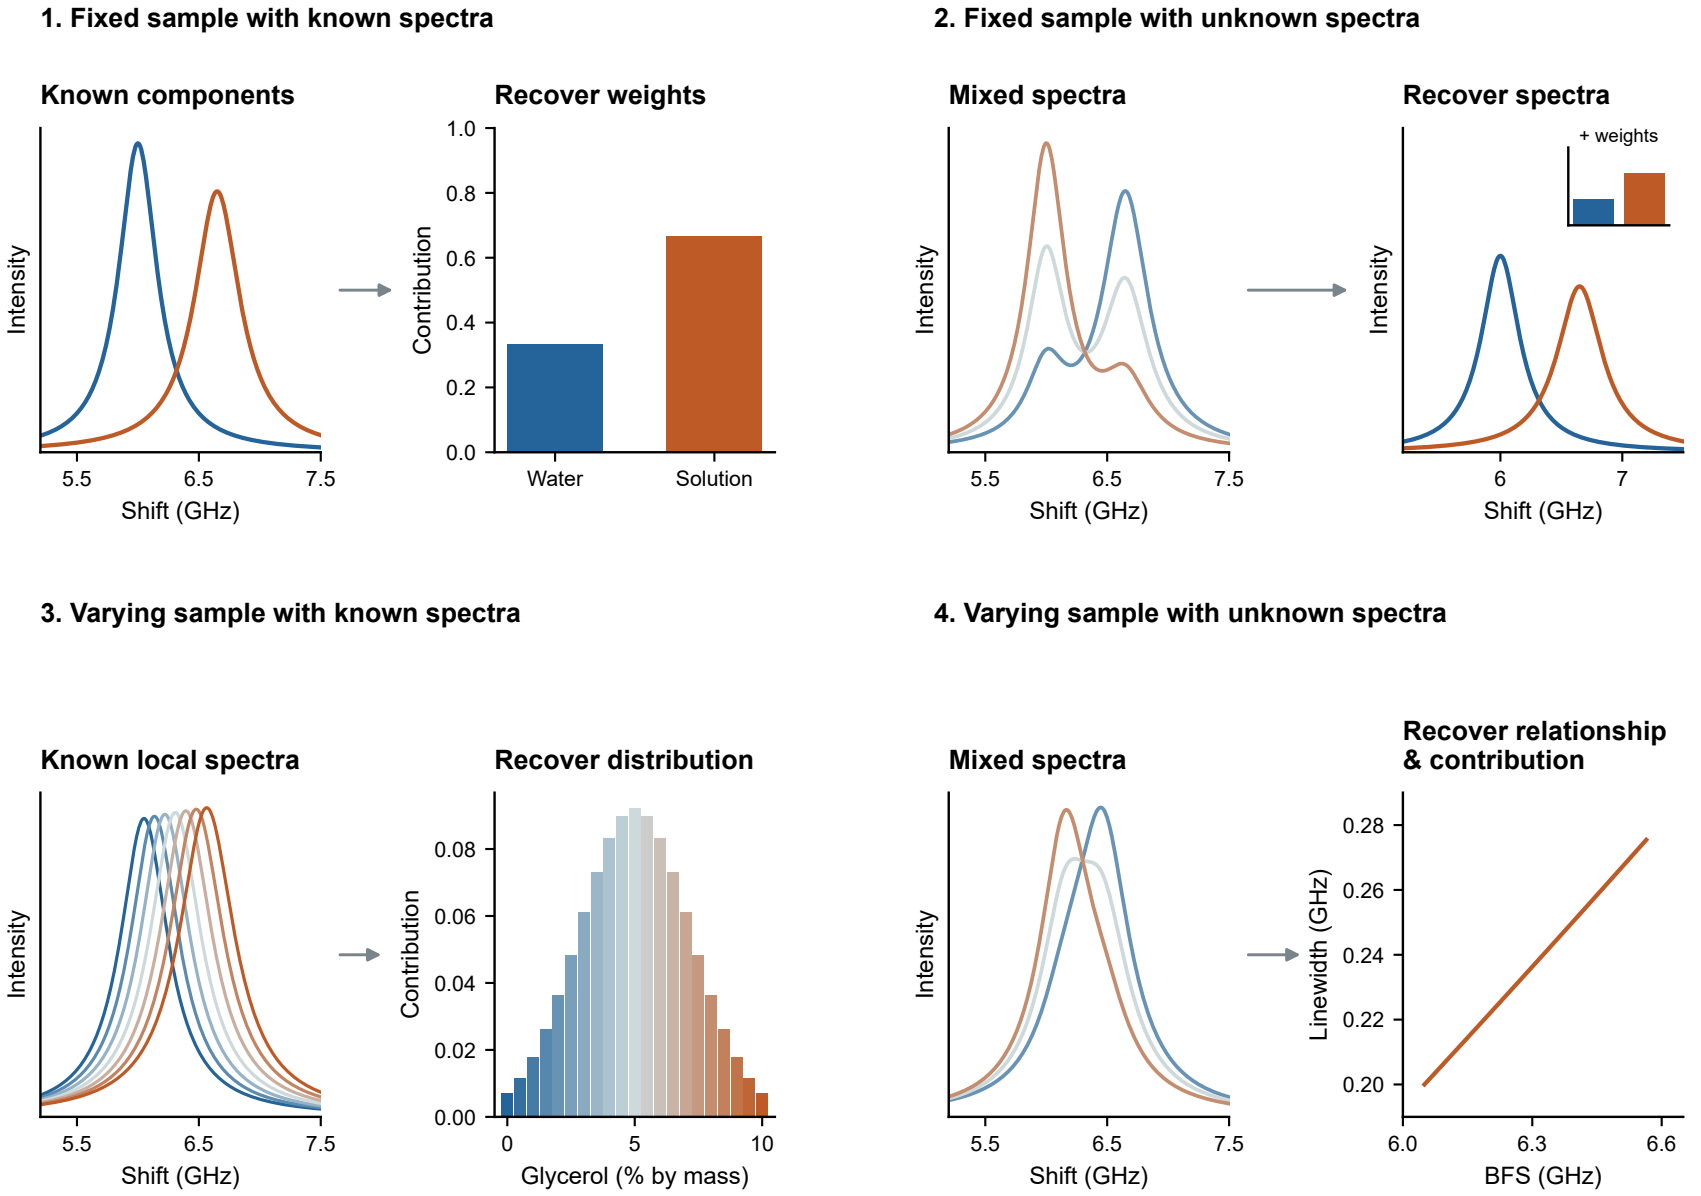

1. Fixed sample with known spectra
Known components
Recover weights
Intensity
5.5
6.5
7.5
Shift (GHz)
Contribution
1.0
0.8
0.6
0.4
0.2
0.0
Water
Solution
2. Fixed sample with unknown spectra
Mixed spectra
Recover spectra
Intensity
5.5
6.5
7.5
Shift (GHz)
+ weights
Intensity
6
7
Shift (GHz)
3. Varying sample with known spectra
Known local spectra
Recover distribution
Intensity
5.5
6.5
7.5
Shift (GHz)
Contribution
0.08
0.06
0.04
0.02
0.00
0
5
10
Glycerol (% by mass)
4. Varying sample with unknown spectra
Mixed spectra
Recover relationship & contribution
Intensity
5.5
6.5
7.5
Shift (GHz)
Linewidth (GHz)
0.28
0.26
0.24
0.22
0.20
6.0
6.3
6.6
BFS (GHz)