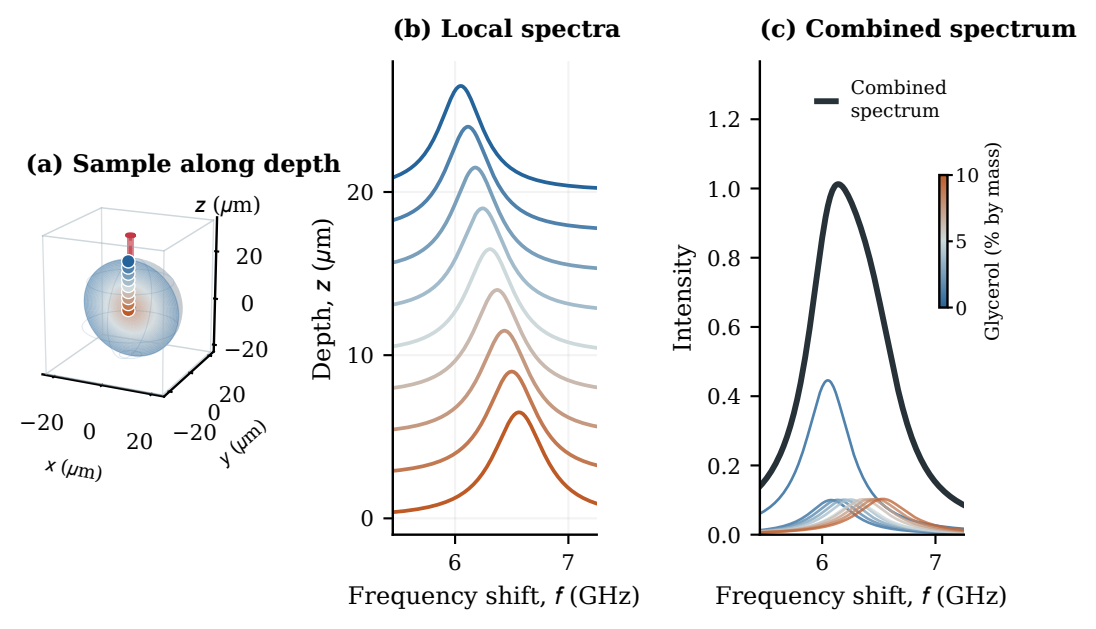

(a) Sample along depth
z (μm)
20
0
−20
−20
0
20
x (μm)
20
0
−20
y (μm)
(b) Local spectra
Depth, z (μm)
20
10
0
6
7
Frequency shift, f (GHz)
(c) Combined spectrum
Combined spectrum
Intensity
1.2
1.0
0.8
0.6
0.4
0.2
0.0
10
5
0
Glycerol (% by mass)
6
7
Frequency shift, f (GHz)