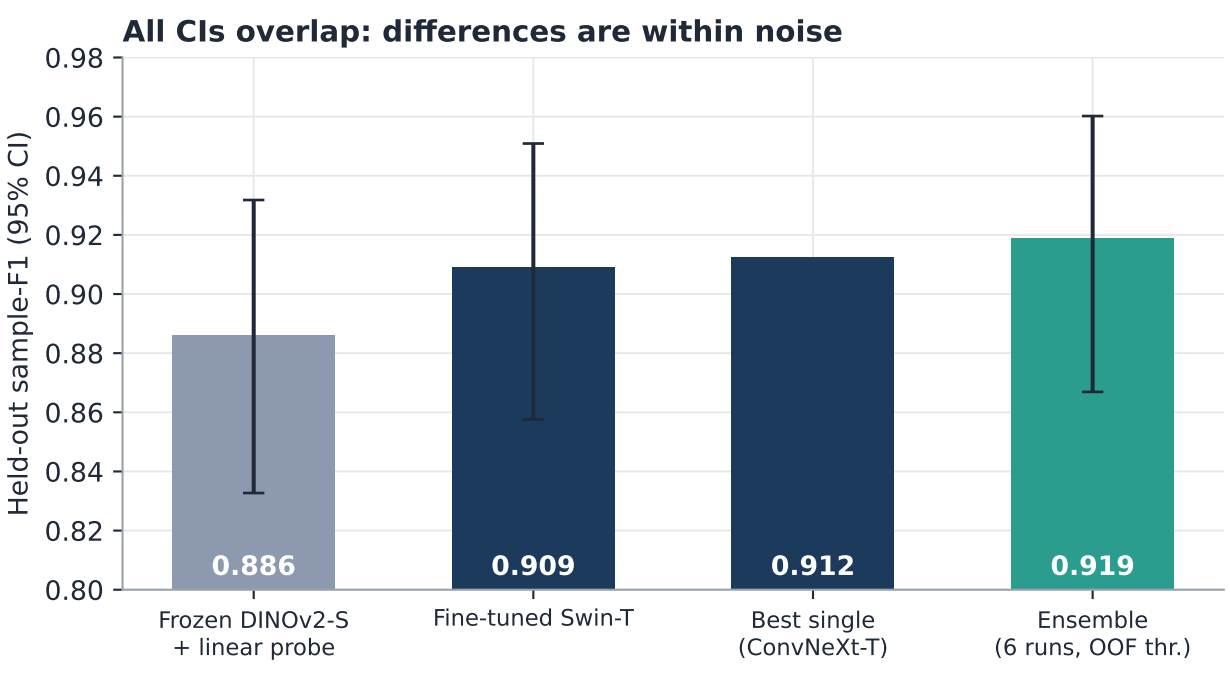
All CIs overlap: differences are within noise
Held-out sample-F1 (95% CI)
0.98
0.96
0.94
0.92
0.90
0.88
0.86
0.84
0.82
0.80
0.886
0.909
0.912
0.919
Frozen DINOv2-S + linear probe
Fine-tuned Swin-T
Best single (ConvNeXt-T)
Ensemble (6 runs, OOF thr.)