
Automated cosine response test bench

Rotating laser source and stationary detector

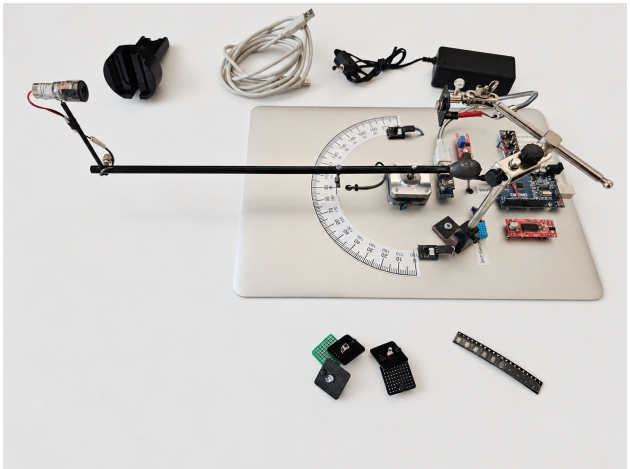


Angular screening

-90 to +90 degrees

Historical analysis:
100 readings per scan
+ constructed endpoint

New firmware:
101 acquired samples

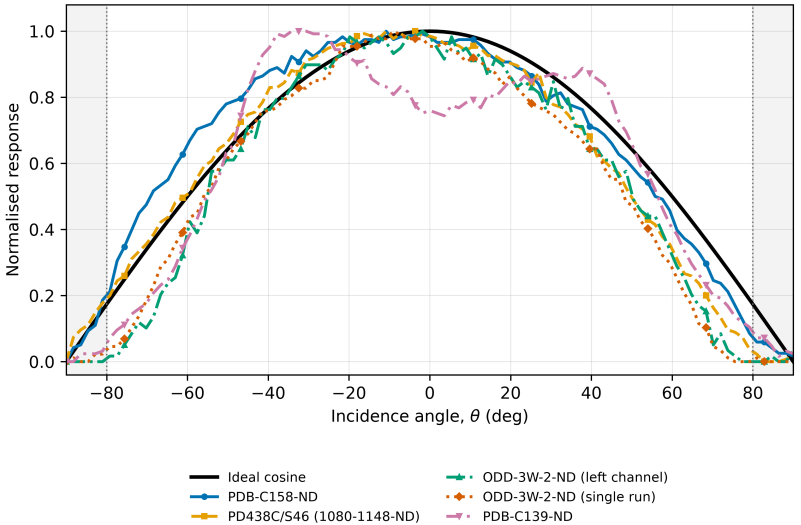

Workbook cohort: PDB-C158 lowest RMSE80 (0.0801); PD438C/S46 lowest MAE80 (0.0635).

Narrow-band package screening; no claim of broadband pyranometer calibration.