



Coupled native Human: unchanged baseline and temporary half-drive intervention
10 s initialization; drive scaled by 0.5 during 60–100 s; existing regulation resumes after 100 s


Inspired volume per completed breath

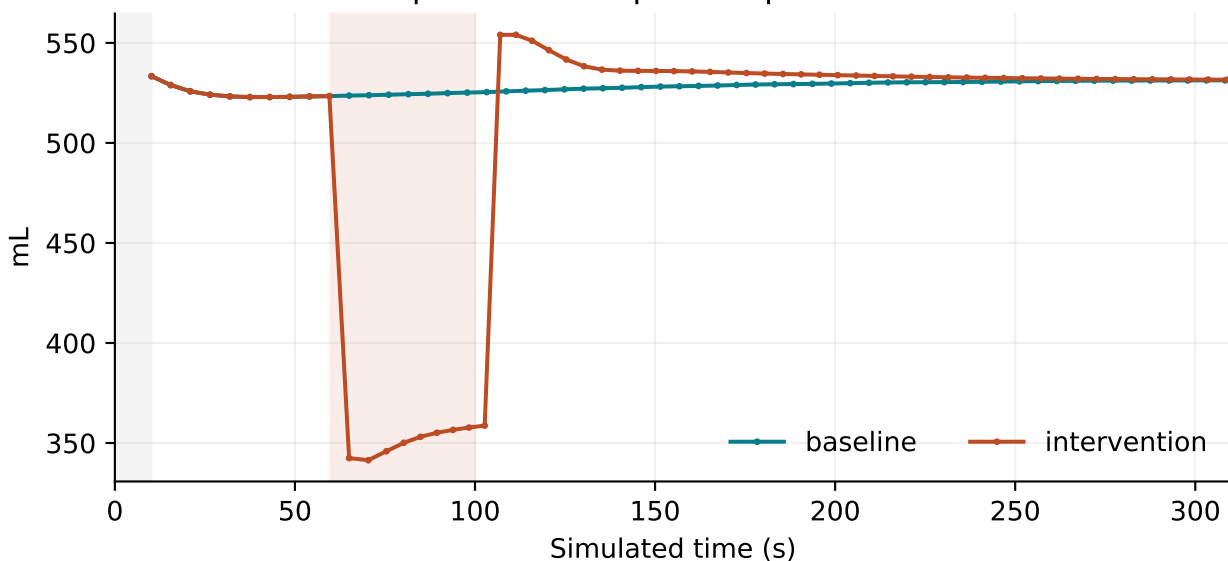


Inspired ventilation, trailing 30 s

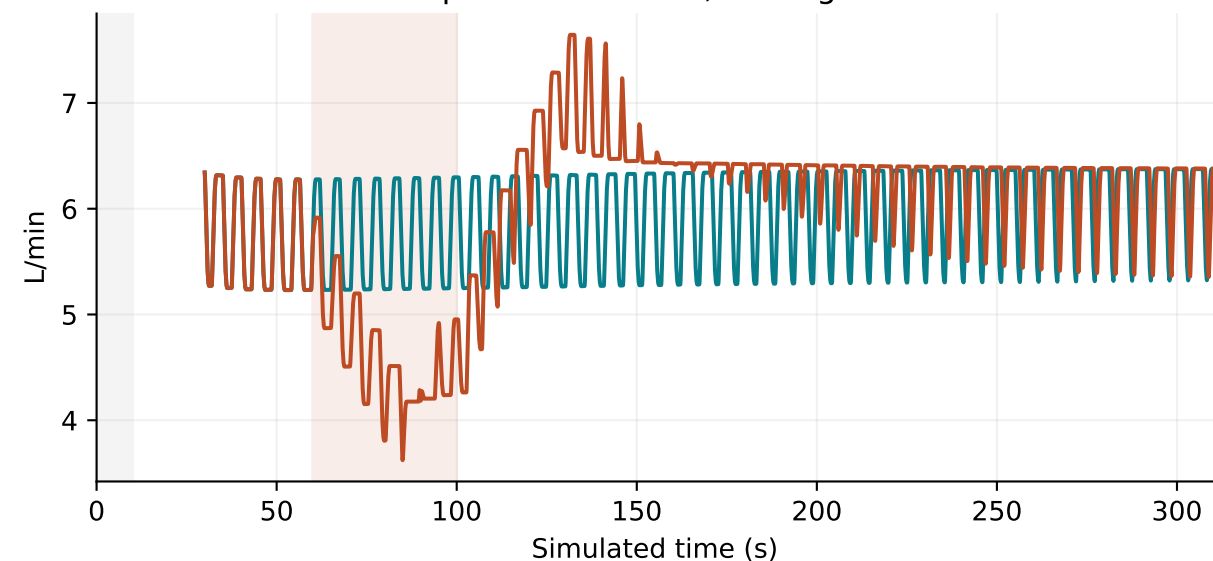


Arterial oxygen partial pressure

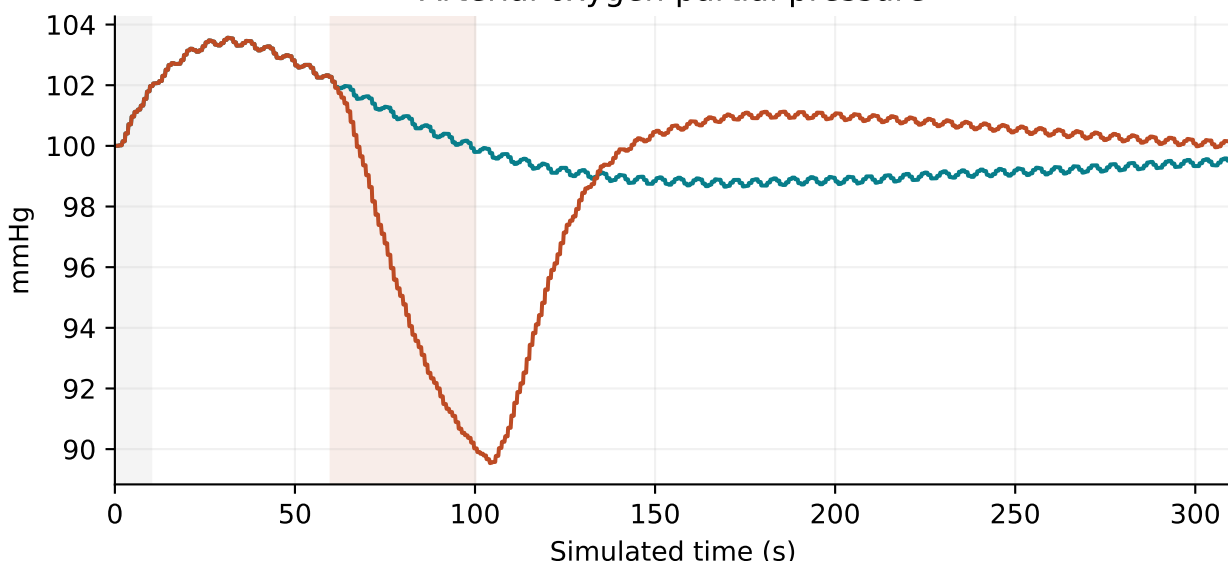

Arterial carbon dioxide partial pressure

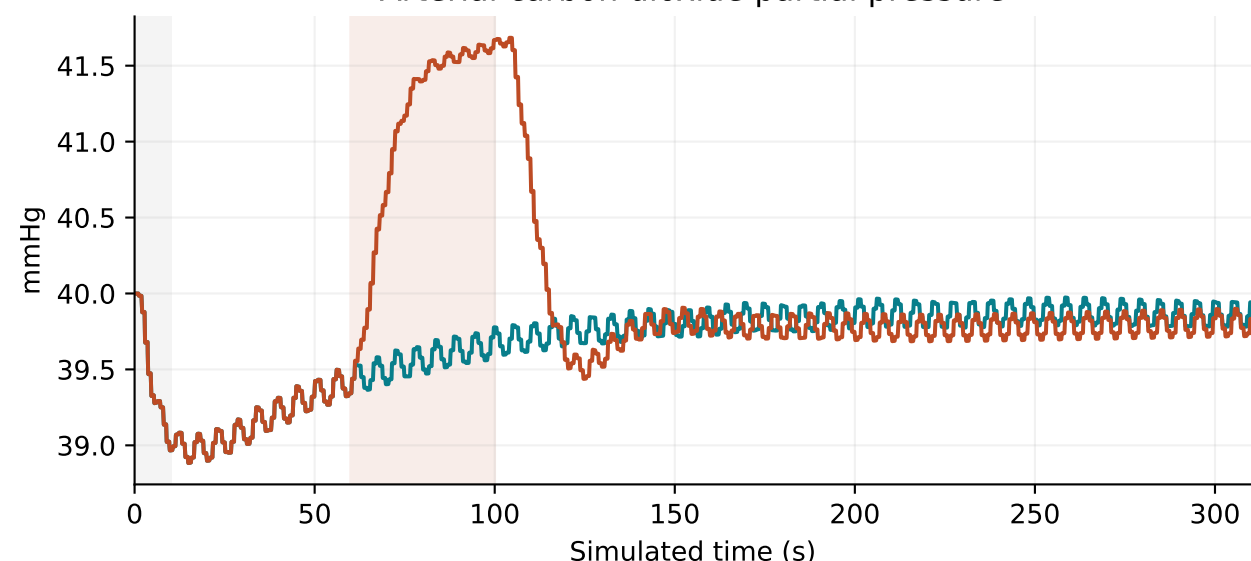

Left-ventricular stroke volume

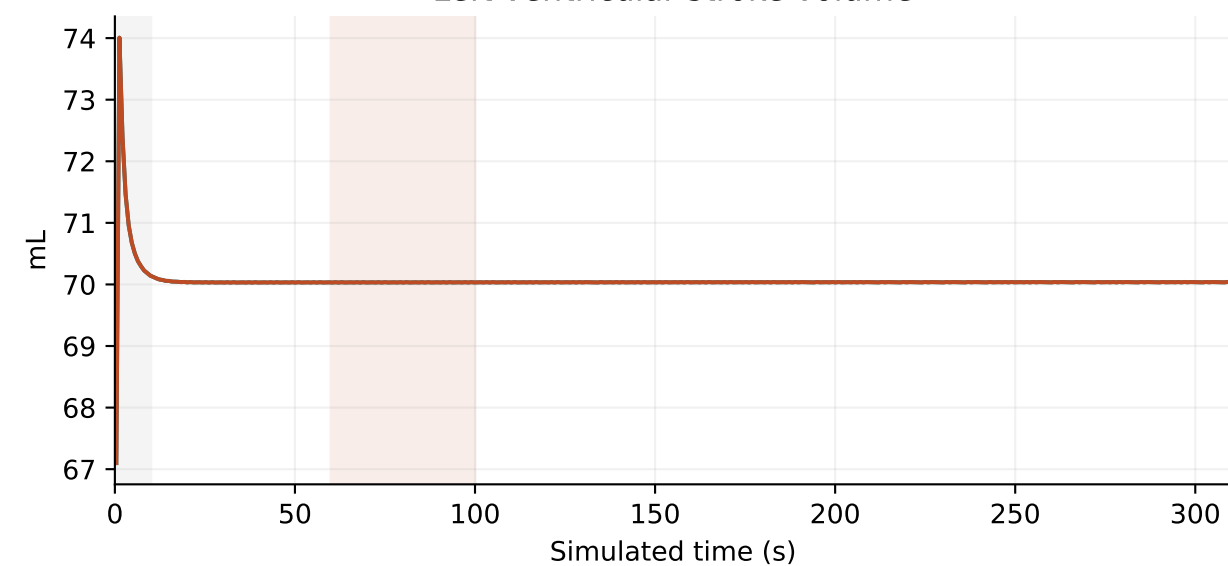

Blood-volume deviation: running maximum

