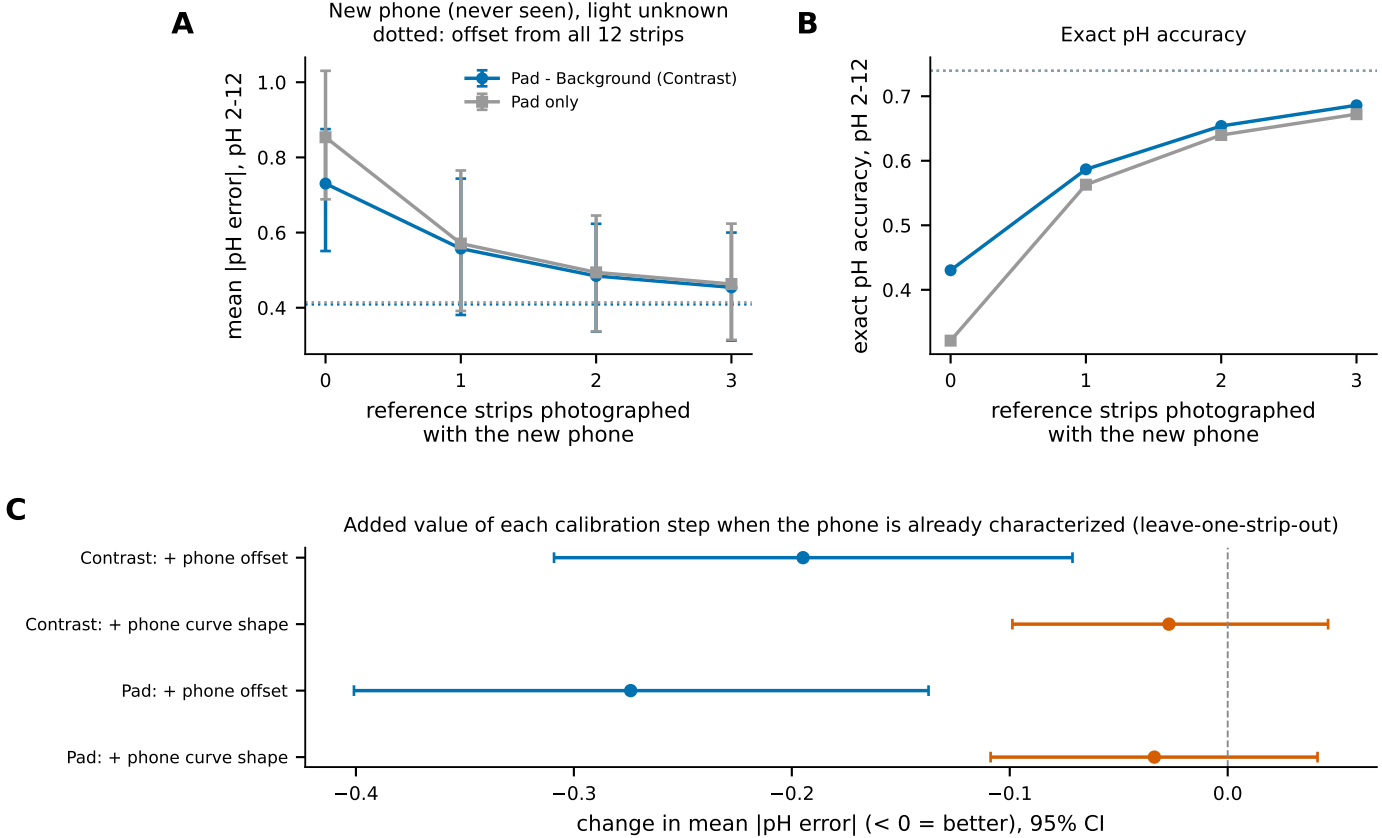
A
New phone (never seen), light unknown
dotted: offset from all 12 strips
Pad - Background (Contrast)
Pad only
mean |pH error|, pH 2-12
1.0
0.8
0.6
0.4
0
1
2
3
reference strips photographed
with the new phone
B
Exact pH accuracy
exact pH accuracy, pH 2-12
0.7
0.6
0.5
0.4
0
1
2
3
reference strips photographed
with the new phone
C
Added value of each calibration step when the phone is already characterized (leave-one-strip-out)
Contrast: + phone offset
Contrast: + phone curve shape
Pad: + phone offset
Pad: + phone curve shape
−0.4
−0.3
−0.2
−0.1
0.0
change in mean |pH error| (< 0 = better), 95% CI