尺寸:100X145mm

材质:105g铜版纸,钉装

IPL Cooling Hair Remover
OB0130

User Manual

Product Name:IPL Cooling Hair Remover
Model:OB0130
Product Dimensions:185.4*63.5*36.5mm
Product Weight:820g
Input Power:48W
Battery/Charging: DC 24V/2A

Precautions:

Please follow the **User Manual** for product assembly and usage.

Before use, carefully read and keep the manual safe.

If you have any questions, please contact online customer service.

Warnings:

Incorrect operation may cause personal injury.

Do not use the product while bathing or showering.

Do not use near bathtubs,washbasins, or other water-filled containers.

Keep the product and power adapter dry to avoid the risk of electric shock.

Do not insert objects into the product to prevent damage.

Do not use near the eyes. Wear protective eyewear to protect your eyes.

When using the device for back treatment, it is recommended to have assistance from another person.

Keep the skin clean and free from oils.

Not suitable for children, pregnant women, or people with certain health conditions.

*Stop using the device immediately if you encounter any discomfort/ pain or injury (burn, discoloration, or scarring) on your skin, and consult your physician before using it again.

Notes:

When using the product, ensure the device adapter matches the voltage.

Do not use near flammable materials.

Avoid direct exposure of strong light to the eyes during operation; wear protective eyewear.

After use, clean the device to prevent malfunctions.

INTENDED USE AND SCOPE OF APPLICATION

1、Intended use: as an adjunctive treatment for the reduction of body hair.

2、the product is expected to be used in medical institutions, clinics, beauty salons, and families, should be in the ambient temperature of 5 ~ 30 °C, relative humidity is not greater than 80%, can not be in the presence of flammable anaesthesia gas mixed with air or with oxygen or nitrous oxide mixed with flammable anaesthesia gas under the circumstances of the equipment; please do not use the product under strong sunlight directly.

3、Applicable people: Adults over 18 years old.

4、Applicable parts: face, limbs, armpits, bikini, body parts.

PRODUCT STRUCTURE DIAGRAM

This product mainly consists of a device, adapter, goggles, and instruction manual. The device contains power supply setting, control setting and induction setting; the treatment head contains reflective focusing device, xenon lamp light sources, light guiding crystals, skin sensing accessory, and ice cooling acessory

The structure diagram of each model is specified below:

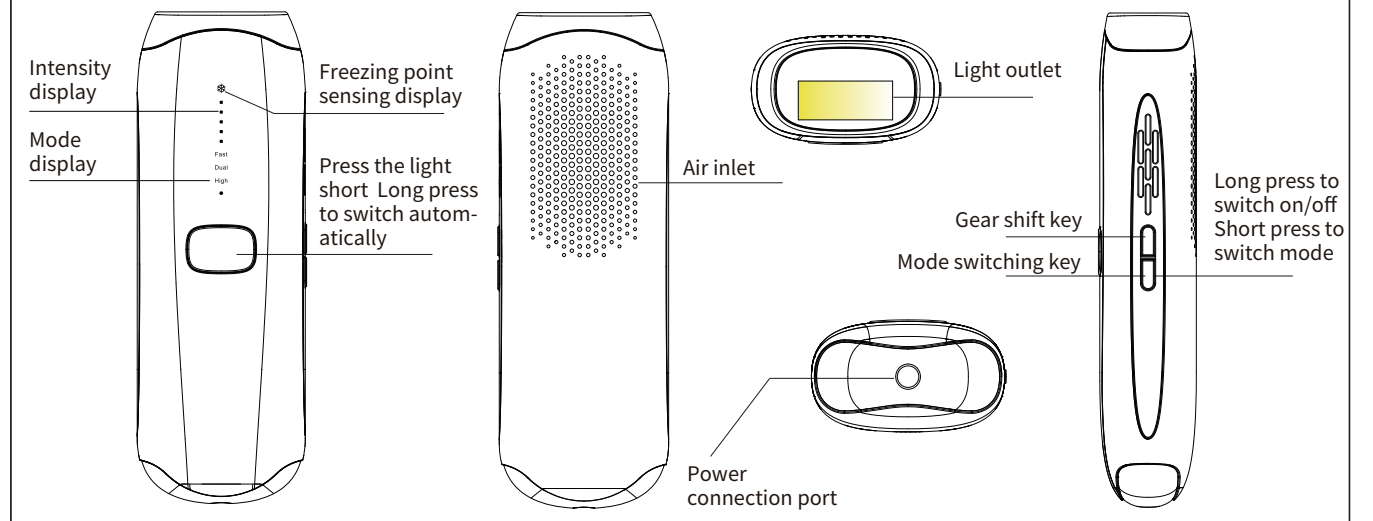
Intensity display
Mode display
Freezing point sensing display
Press the light short Long press to switch automatically
Air inlet
Light outlet
Power connection port
Gear shift key
Mode switching key
Long press to switch on/off Short press to switch mode

This picture is for reference only, the actual object shall prevail.

PRODUCT MAIN PERFORMANCE PARAMETERS

1、Normal working conditions:
-Ambient temperature: 5°C~30°C
-Relative humidity: not more than 80 per cent
-Atmospheric pressure: 86.0kPa~106.0kPa
-Adapter Input: 100-240V~;50/60Hz.
-Adapter output: 24Vdc 2A (T27-B)
-Software Release No.: V1.0

2、Main performance parameters:
-Output wavelength range: 510nm~1200nm
-Pulse parameters:
a. Pulse output mode: single pulse Pulse string
b. For pulse output parameters, see the table below:

Model	Mode	Output method	Pulse width(ms)
T27-B	High	Single pulse	10.0ms, with an allowable error of ±10 per cent
	Fast	Pulse train	Within 1.9s to 4.3s, the allowable error is ±10%.
		Subpulse	0.35ms, with an allowable error of ±10 per cent
	Dual	Pulse train	0.36s with a permissible error of ±10 per cent
		Subpulse	Subpulse 1 0.10ms with an allowable error of ±10 per cent Subpulse 2 10.0ms, with an allowable error of ±10 per cent

c. Pulse energy: within 9J～22J, the allowable error is ±20%;

Model	Mode	Output method	Pulse energy J	Number of subpulses	Subpulse interval
T27-B	High	Single pulse	Within 9.5J～18J, the permitted error is ±20%.	Single pulse	/
	Fast	Pulse train	Within 9J～22J, the allowable error is ±20%.	Five	0.54s～1.06s, allowable error is ±10%.
	Dual	Pulse train	Within 10J～20J, the allowable error is ±20%.	Two	0.35s~4.03 with a permissible error of ±10 per cent

-Accuracy of working data: the error between the actual output value of pulse energy of the therapeutic instrument and the set value should be within ±20%.
-Energy density at the treatment end: 2.3~5.7J/cm², with an allowable error of ±20%.

According to GB 9706.283-2023 risk classification level is divided into: Exemption category

Output spot size:

Model	Exposure area	Tolerances
T27-B	3.9cm²	±0.2cm²

PRODUCT INSTALLATION AND OPERATION INSTRUCTIONS

1、Pre-use inspection

1) Unpacking and checking: take out the main unit and its accessories from the packing box, count the accessories according to the packing list, and save the relevant packing materials for subsequent transport, preservation and reference.

2) Check whether the mainframe and each accessory are intact, check whether there is any mechanical damage, if there is any sign of damage to the function of the equipment, it should not be used, and contact the agent or after-sales service unit in time.

3) If there is a sudden increase in the intensity of the light emitted from the device when it is in use, please switch off the device immediately and contact the manufacturer or local distributor for maintenance.

4) Wear goggles before use, if you do not wear goggles, and long-term use of intense pulsed light therapy device, easy to cause eye vision damage.

2、 Preparation for use



1、Thoroughly clean the skin, ensuring that it is free of hair, cuts, tattoos, spots, completely dry, and free of oily residues (residues of perfumes, lotions, deodorants, sunscreens, etc.).



2、Make sure that there is no dirt residue such as dust and hair in the irradiation port, and that there is no breakage or abnormality. If there is dirt, please be sure to clean up, so as not to cause product failure, deterioration and skin problems.



3、The use of intense pulsed light therapy device before the first skin test, skin test 2 hours later, to confirm the skin condition, if the irradiation site does not appear abnormal (redness, blisters), you can rest assured that the use of this product.

3、Methods of use

1. Use a razor to shave off the hair in the area to be cared for (Figure 1). Note: Do not use the razor in direct contact with the skin, use it together with the foam or shave in the shower. The razor is sharp, please use it carefully to avoid scratching. Do not use depilatory creams for hair removal as the chemicals may trigger adverse skin reactions.



Figure 1

2. Plug the power cord into the power input connector at the end of the product (Figure 2).
3. See the power cord is connected to the product power input connector, then insert the plug into the power outlet (Figure 3).
4. Long press the mainframe side on button to switch on the machine (Figure 4).



Figure 2



Figure 3



Figure 4

5. Adjust the intensity level，function mode, maual or auto mode according to your needs.

6. Wear goggles before treatment to protect your eyes.

7.The light port will be placed in the skin to be treated area and vertically affixed, the treatment instrument sensor light will flash white light, indicating that it has been fully contacted, press the flash button to start the treatment operation, if not flash white light, it means that the light head and the skin is not fully affixed, the instrument will not be light.

8.After the treatment is completed, long press the on/off button to switch off the equipment (do not unplug directly without switching off the equipment to avoid causing damage)



Figure 5



Figure 6



Figure 7



Figure 8

Note: The maximum temperature of the light outlet during use can reach 48°C, there is a slight sense of warmth and tingling sensation, which is a normal symptom when using the equipment.

The semiconductor refrigeration works automatically after the host is switched on, and the surface temperature of the treatment head should be the range of 0°C to 25°C within 1 minute.

4、Presentation of modalities

1、Automatic mode
(for large areas such as arms and legs).

Place the light outlet on the area of the skin to be treated, and fully fit with the skin, at this time, the sensor light of the treatment instrument will flash, indicating that the light head and the skin have been fully contacted. Long press the flash button, immediately begin to move the instrument slowly and evenly on the skin, and skin to maintain the fit, the flash will be issued at certain intervals, at this time, please keep the intense pulsed light therapy instrument to move, in the need for treatment of the region back and forth sliding two times to ensure that the treatment area is evenly covered, to avoid leakage of light.T27-B will be set to the intense pulsed light therapy instrument for the automatic exposure mode, the therapeutic head in contact with human skin, can be exposed, 1 mode Fast contact a continuous flash 5 times, 1 mode Fast contact a continuous flash 5 times. T27-B is set to automatic exposure mode, where the treatment head touches the human skin and can be exposed. Mode 'Fast' contacts once and flashes 5 times in a row, Mode 'Dual' contacts once and flashes 2 times in a row, and Mode 'High' contacts once and flashes once.

Tip: The speed of the skin's movement can be adjusted according to the flash speed for more even coverage. The flash frequency is faster in the 1st gear, slightly slower in the 2nd gear, and the higher the gear the slower the speed of the light.

2.Manual mode
(for finger, lip hair and other small areas).



Place the light outlet on the skin to be treated area, and fully fit the skin, at this time, the treatment instrument sensor light will flash to indicate that the light head and the skin fully fit. Press the flash button briefly to start the treatment. Move the light head to the next piece of skin, wait for the white light of the sensor lamp of the treatment instrument to flash, and then press the flash button, and repeat the above operation in turn.T27-B will set the intense pulsed light therapy instrument to manual exposure mode, the treatment head touches the skin of the human body, and briefly press the exposure button once, can be exposed, the 1 mode Fast contact with a continuous flash of 5 times, the 2 mode Dual contact with a continuous flash of 2 times, the 3 mode High Contact a flash once.
Tip: If at any time during the treatment, your skin starts to feel overheated, simply pause for a few seconds to allow the outlet to re-cool before proceeding.

[Tips on the use of intense pulse light therapy instrument]



1.due to the intense pulsed light therapy instrument continuous flash will continue to accumulate heat, in order to make the effect continue to be effective, it is recommended that in the process of use if you feel that the skin is overheated, you can temporarily replace the use of another area, wait for the skin to cool down and then carry out the treatment.



2.the use of intense pulsed light therapy device, the lamp head should be tightly pressed against the skin, so that it is in full contact with the hair follicle, to ensure that the hair follicle absorbs a high level of energy, to achieve a more effective therapeutic effect.

5、Usage suggestions

Weeks 1-2 , use 3 times a week;
Weeks 3-5, use twice a week;
After 5 weeks, use every half month or once a month.

Note: Please use it several times according to the growth of hairs, too coarse and hard hairs can increase the gear and frequency appropriately on the basis of this, the specific situation varies from person to person.

[Post-treatment precautions]
1. It is recommended to avoid touching water within 6 hours after the treatment operation, after which moisturising water can be used to moisturise the irradiated area.
2. Do not use perfume, masks and cosmetics containing scrub beads after skin treatment.
3. Please avoid UV exposure within 24 hours after the treatment operation, if necessary, please apply sunscreen.
4. Artificial tanning skin during treatment procedures is prohibited.
5. Please consult your doctor if you need plastic surgery after the treatment (only the treated area).
6. If there is any discomfort, please consult your surgeon.
7. Pregnant women can not use

PRODUCT CARE AND MAINTENANCE

1、Product cleaning and maintenance

In order to ensure that the product achieves the best results and the longest service life, please clean the product before and after each treatment to avoid the accumulation of hair and dust over time, if you do not clean it properly, the product will not get its proper effect.

1. Before starting to clean, the unit must be switched off and unplugged to allow the machine to cool down.

2. With a soft, clean and dry cloth dipped in alcohol (concentration of not more than 95%) to wipe, clean the light outlet mirror and the body (not regularly clean the head will appear black spot situation).

3. Store the equipment in a dry and dust-free environment at -10°C-55°C. Do not wash the product and accessories under the tap or in the dishwasher.

Note: Do not use steel wool abrasive cleaners (toothpaste, etc.) or caustic liquids (petrol, oil, acetone, etc.) to clean the product.

This product is intended for personal use, please do not share this product with others. If the product must be used by more than one person, please clean and sterilise the light outlet before use. Failure to do so may cause cross-contamination.

WARRANTY

1. The warranty period is one year from the day purchased by the consumer.
2. Division of warranty responsibilities
If the product is under warranty, the company will replace the new product for you after checking the non-human factors. Other faults caused by abnormal use or force majeure are not covered by the warranty.

CONTACT US

MALAYSIA Healthy World Lifestyle Sdn. Bhd
No. 22 Jalan Anggerik Mokara 31/47,
Kota Kemuning, 40460 Shah Alam,
Selangor Darul Ehsan, Malaysia
Tel: +603-5121 4286
Fax: +603-5121 4386

SINGAPORE
OGAWA Health Care Pte Ltd
27 Tampines Industrial Avenue 5,
T5@Tampines Singapore 528623
Tel: +065-6846 8588
Fax: +065-6846 7677

IPL Cooling Hair Remover
OB0130

使用说明书

产品名称:IPL Cooling Hair Remover
产品型号:OB0130
产品尺寸:185.4*63.5*36.5mm
产品重量:820g
输入功率:48W
电池/充电: DC 24V/2A

注意事项：

1. 请遵循《使用说明书》进行产品装配和使用。
2. 使用前，请仔细阅读并妥善保管说明书。
3. 如有疑问，请联系在线客服。

警告：

错误操作可能导致人身受伤。

禁止在洗澡或淋浴时使用。

请勿在浴缸、沐浴盆、洗脸盆等盛水器具附近使用。

请保持产品和电源适配器干燥，避免触电。

请勿将物体插入产品，避免损坏。

请勿在眼睛周围使用，佩戴防护眼镜可保护眼睛。

使用背部治疗时，建议有他人帮助。

若有长发，使用前请剃发，以避免不适。

保持皮肤干净且无油脂。

不适用于儿童、孕妇或有某些健康问题的人群。

如果在使用过程中感到不适/疼痛，或皮肤出现烧伤、变色或疤痕，请立即停止使用，并在再次使用前咨询医生。

注意：

使用时，请确保设备适配器匹配电压。

请勿在易燃物品附近使用。

操作时，避免强光直射眼睛，佩戴防护眼镜。

若设备损坏，必须由专业人员更换电源适配器。

使用后请清洁设备，避免故障。

预期用途和适用范围

1、 预期用途：用于减少身体毛发的辅助治疗。
2、该产品预期使用的地点为医疗机构、诊所、美容院、及家庭，应在环境温度5~30°C、相对湿度不大于80%，不能在有与空气混合的易燃麻醉气或与氧或氧化亚氮混合的易燃麻醉气情况下使用的设备；避免强光直射下使用本设备。
3、 适用人群：仅适用于年龄大于18周岁。
4.适用部位：脸部、四肢、腋下、比基尼、身体部位。

产品结构图

本产品主要由主机、适配器、护目镜、说明书组成。主机含有电源装置、控制装置、感应装置；治疗头含有反射聚光器件、氙灯光源、导光晶体、皮肤感应装置、皮肤制冷装置。

各型号结构图具体如下：

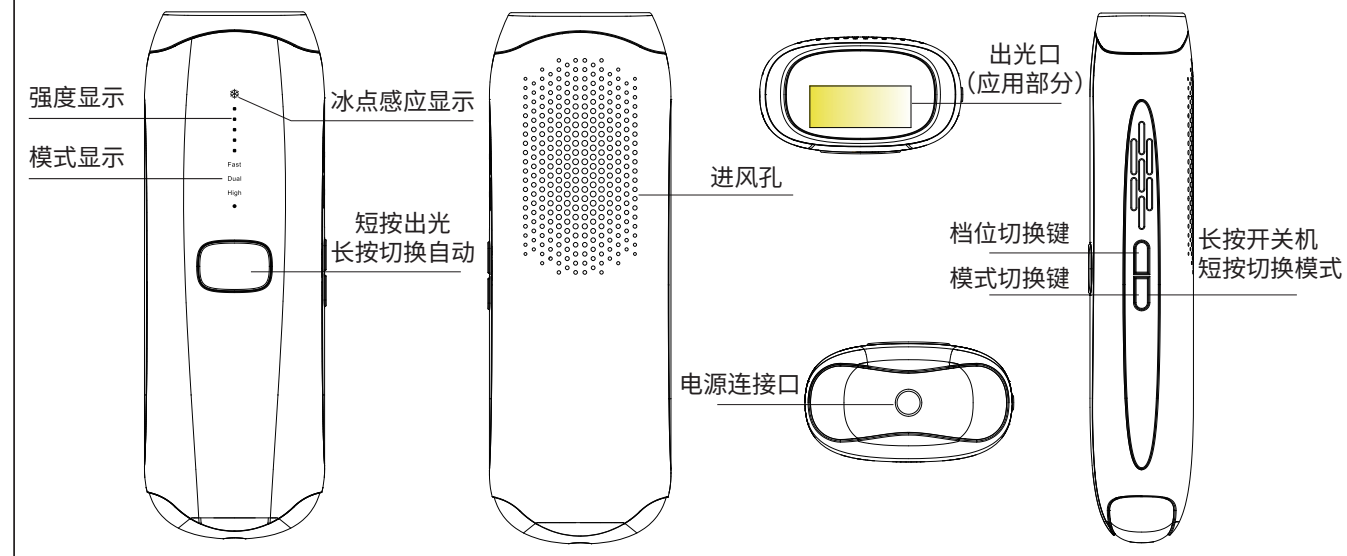

此图仅供参考，具体以实物为准。

产品主要性能参数

一、正常工作条件
-环境温度：5°C~30°C
-相对湿度：不大于80%
-大气压力：86.0kPa~106.0kPa
-由适配器型号（QL048-2402000C）供电输入：100-240Vac，50/60Hz，1.2A输出：DC24V，2.0A，48.0W；由适配器型号（FX48C-240200C）供电输入：100-240Vac，50/60Hz，1.0A输出：DC24V，2.0A，48.0W
-软件发布版本号：V1.0
二、主要性能参数：
-输出光波长范围：510nm~1200nm
-脉冲参数：
a、脉冲输出方式：单脉冲 脉冲串
b、脉冲输出参数，见下表：

型号	模式	输出方式	脉冲宽度ms
T27-B	High	单脉冲	10.0ms，允许误差为±10%
	Fast	脉冲串	1.9s～4.3s内，允许误差为±10%
		子脉冲	0.35ms，允许误差为±10%
	Dual	脉冲串	0.36s，允许误差为±10%
		子脉冲	子脉冲1 0.10ms，允许误差为±10% 子脉冲2 10.0ms，允许误差为±10%

c、脉冲能量：9J～22J内，允许误差为±20%；

型号	模式	输出方式	脉冲能量J	子脉冲个数	子脉冲时间间隔
T27-B	High	单脉冲	9.5J～18J内，允许误差为±20%	单脉冲	/
	Fast	脉冲串	9J～22J内，允许误差为±20%	五个	0.54s～1.06s内允许误差为±10%
	Dual	脉冲串	10J～20J内，允许误差为±20%	两个	0.35s~4.03s允许误差为±10%

-工作数据的准确性：治疗仪的脉冲能量实际输出值与设值的误差应在±20%范围内
-治疗端面的能量密度：2.3~5.7J/cm²,允许误差为±20%。

按GB 9706.283-2023风险分类等级划分为：豁免类

输出光斑尺寸：

型号	照射面积	允差
T27-B	3.9cm²	±0.2cm²

产品安装和操作说明

一、使用前检查
1)开箱检查：从包装盒内取出主机及其附件，按装箱清单清点附件，保存好相关包装材料以备后续运输、保存和查阅用。
2)检查主机和各附件是否完好，检查是否有任何机械性损坏，如有设备功能有损坏的迹象，则不得使用，并及时与代理商或售后服务单位联系。
3）使用时若设备出光强度突然增大，请立即关闭设备,并联系制造商或当地经销商进行维修。
4）使用前先佩戴护目镜，若未佩戴护目镜，且长期使用强脉冲光治疗仪，易造成眼睛视力受损。
二、使用前准备



1、彻底清洁皮肤，保证皮肤没有毛发、没有伤口破损、纹身、斑点、完全干燥，没有油性物质残留（香水、乳液、 香体液和防晒霜等残留物）。



2、确认照射口没有灰尘和毛发等污垢残留，没有破损或异常。如果有污垢请务必清扫干净，以免造成产品故障，劣化以及肌肤问题。



3、使用强脉冲光治疗仪前请先进行皮肤测试，皮肤测试2小时后，确认肌肤状况，如果照射部位没有出现异常（发红、水泡），则可以放心使用本产品。

三、使用方法

1、用剃毛刀将需要护理部位的毛发剃掉(图一)。
注：刮刀请勿直接接触皮肤，配合泡沫一起使用或者在洗澡的时候刮毛。刮刀锋利，请小心使用，避免刮伤。请勿使用除毛膏进行毛发去除，因为化学物质可能会引发皮肤的不良反应。

图一

2、将电源线插入产品尾部的电源输入接口（图二）。
3、见电源线连接到产品电源输入接口后，将插头插入到电源插座（图三）。
4、长按主机侧边开机键开机（图四）。



图二



图三



图四

5、根据自己的需要调节好强度，模式和手自动模式。
6、治疗操作前佩戴护目镜，保护眼睛。
7、将出光口置于皮肤待处理区域并垂直贴合，治疗仪感应灯会闪烁白灯，表明已充分接触，按下闪光键，开始治疗操作，若未闪烁白灯，则表示灯头与皮肤没有完全贴合，仪器不会出光。

8、治疗完成后，长按开关机键关闭设备（切勿不关机直接拔下插头，以免造成损害）

图五



图六



图七

图八

注意:使用时出光口最高温度可达48°C，有轻微的温热感及刺痛感，属于使用设备时产生的正常症状 。
主机开机后半导体制冷自动工作，1分钟内治疗头的表面温度应在0°C～25°C范围内。

四、模式介绍



1、自动模式（适用于手臂、腿等大面积部位）。将出光口置于皮肤待处理区域，与皮肤充分贴合，此时治疗仪感应灯会闪烁，说明灯头与皮肤已充分接触。长按闪光按键，立即开始在皮肤上缓慢匀速移动仪器，与皮肤保持贴合状态，闪光会按一定的间隔时间发出，此时请保持强脉冲光治疗仪移动，在需要治疗的区域来回滑动两遍，以确保治疗区域被均匀覆盖，避免漏打光。T27-B将强脉冲光治疗仪设定为自动曝光模式，治疗头接触人体皮肤，即可曝光，1模式Fast接触一次连闪5次，2模式Dual接触一次连闪2次，3模式High接触一次闪一次。
提示:皮肤的移动速度可根据闪速进行调整，以便覆盖范围更均匀，在第1档闪光频率更快，在2档闪光频率稍慢，档位越高出光速度越慢。



2、手动模式（适用于手指、唇毛等小面积部位）。将出光口置于皮肤待处理区域，与皮肤充分贴合，此时治疗仪感应灯会闪烁说明灯头与皮肤充分贴合。短按闪光按键即可开始治疗。将灯头移到下一块皮肤，等待治疗仪感应灯白色灯闪烁，然后再按下闪光按键，依次重复上述操作。T27-B将强脉冲光治疗仪设定为手动曝光模式，治疗头接触人体皮肤，短按1次曝光键，即可曝光，1模式Fast接触一次连闪5次，2模式Dual接触一次连闪2次，3模式High接触一次闪一次。
提示:在治疗过程中的任何时候，如果你的皮肤开始感到过热，只需暂停几秒钟，让出光口重新冷却，再进行治疗。
【强脉冲光治疗仪使用小贴士】



1、由于强脉冲光治疗仪连续闪光会不断积累热量，为了让效果持续有效，建议在使用过程中如果感觉皮肤过热，可暂时更换到另外区域使用，等待皮肤冷却后再进行治疗。



2、使用强脉冲光治疗仪时，灯头要紧压皮肤，使其与毛囊充分接触，保证毛囊吸收到高的能量，达到更有效的治疗效果。

五、使用周期
第1-2周 ，每周使用3次；第3-5周，每周使用两次；5周以后，每半个月或一个月使用一次。
注：请根据毛发的生长情况来进行多次使用，过于粗硬的毛发可在此基础上适当的增加档位和频率，具体情况因人而异。

【治疗后的注意事项】
1、建议治疗操作后6小时内避免碰水，之后可使用保湿水对照射部位进行保湿。
2、肌肤治疗后请勿使用香水、面膜及含有磨砂珠的化妆品。
3、治疗操作后24小时内，请避免紫外线暴晒，如果必要，请涂防晒用品。
4、不允许在治疗操作期间进行人造美黑肌肤。
5、如需要在治疗后进行整形手术（仅指治疗区域）请咨询医生。
6、如有不适，请咨询外科医生。
7、孕妇不能使用

产品维护和保养

一、产品清洁和保养
为了确保产品达到最佳效果和最长使用寿命，请在每次治疗前后清洁本产品，避免长期积累毛发及灰尘，如果您没有正常清洁，本产品会得不到其应有的效果。
1、在开始清洁之前，必须关掉设备并拔下电源，让机器冷却。
2、用柔软、干净及干燥的布沾酒精（浓度不超过95%）擦拭、清洁出光口镜面及机身（不定期机头清理会出现黑点情况）。
3、将设备储存在-10°C-55°C干燥无尘环境中。切勿在水龙头和洗碗机中清洗本产品及配件。
注意：不要使用钢丝球研磨性清洁剂（牙膏等）或腐蚀性液体（汽油、机油、丙酮等）来清洁产品。
本产品预期为个人使用，请勿他人共用本产品。如必须多人使用本产品时，请对产品的出光口进行清洁消毒再使用。否则可能引起交叉感染。

保修

1、主机：从消费者购买当天算起，保修期限为一年。
2、灯头：由于非人为原因造成，剩余发数超过30% 的灯头故障，可免费维修。
3、保修责任划分
如果产品在保修期内，公司将在检查非人为因素后为您更换新产品。因不正常使用或不可抗力等原因造成的其他故障不在保修范围之内。

联系我们

MALAYSIA Healthy World Lifestyle Sdn. Bhd
No. 22 Jalan Anggerik Mokara 31/47,
Kota Kemuning, 40460 Shah Alam,
Selangor Darul Ehsan, Malaysia
Tel: +603-5121 4286
Fax: +603-5121 4386

SINGAPORE
OGAWA Health Care Pte Ltd
27 Tampines Industrial Avenue 5,
T5@Tampines Singapore 528623
Tel: +065-6846 8588
Fax: +065-6846 7677