




## Certificate of Calibration

Ocean Sonics, Ltd.

Calibration Certificate Number: **C9016**

Test Result: 10 kHz to 100 kHz:  $-173.7 \pm 2.4$   
10 kHz to 200 kHz:  $-172.8 \pm 3.5$

|                      |                           |                        |                            |
|----------------------|---------------------------|------------------------|----------------------------|
| Model Number         | SB35-ETH                  | Projector Manufacturer | Ocean Sonics               |
| Serial Number        | 1411                      | Projector Model        | TH2-SER-4F                 |
| Manufacture Date     | 6-Sep-2018                | Projector Serial       | 2225                       |
| Measurement Date     | 6-Nov-2024                | Measurement Distance   | 1 m                        |
| Certificate Date     | 6-Nov-2024                | Output Level           | 130.7 dB re $\mu$ Pa @ 1 m |
| Sensitivity @ 26 Hz  | -170.5 dB re V / $\mu$ Pa | Tone Burst             | 100.0 $\mu$ s / 300 ms     |
| Case Type            | Titanium                  | Reference Manufacturer | Ocean Sonics               |
| Element Manufacturer | GeoSpectrum               | Reference Model        | RB9-ETH                    |
| Element Model        | M24HF                     | Reference Serial       | 6465                       |
| Element Serial       | F000850                   | Primary Calibration    | 2023-07-04                 |
| Preamp Model         | 04-300435-09              | Preamp Manufacturer    | Ocean Sonics               |
| Calibrated By        | D.Lee                     | Preamp Model           | 04-300451-01               |
| Work Order Number    | W1234                     | Preamp Serial          | Z88                        |
| Test Type            | RX Sensitivity            | Preamp Gain            | 36 dB                      |
| Test Procedure       | Complex RMS               | ADC Manufacturer       | Ocean Sonics               |
| Test Location        | Tank #3, 1 m              | ADC Model Number       | 04-300427-01               |
| Water Temperature    | 16 °C                     | ADC Serial Number      | Z87                        |

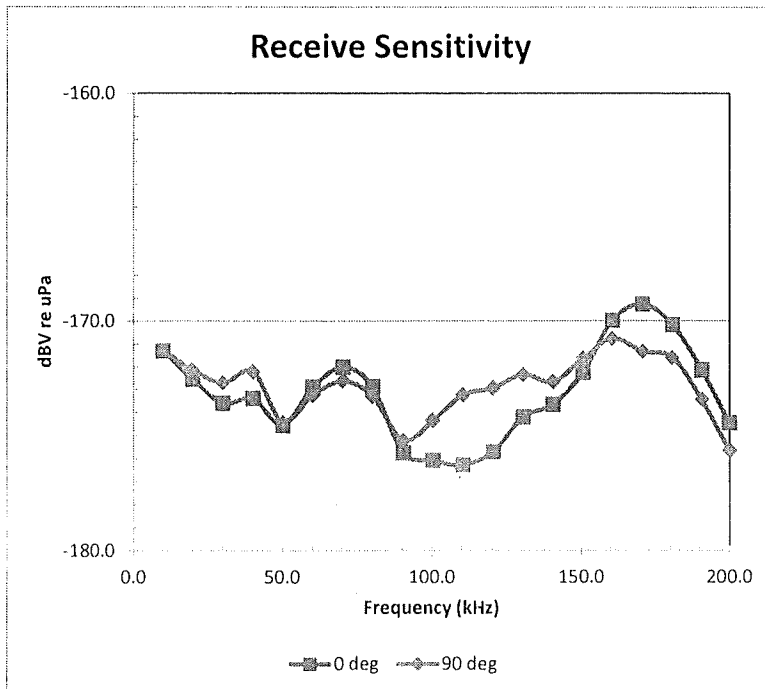

| Frequency<br>kHz | Sensitivity [dBV re $\mu$ Pa] |        |
|------------------|-------------------------------|--------|
|                  | 0 deg                         | 90 deg |
| 10.0             | -171.3                        | -171.3 |
| 20.1             | -172.5                        | -172.1 |
| 30.1             | -173.6                        | -172.7 |
| 40.2             | -173.4                        | -172.2 |
| 50.2             | -174.6                        | -174.4 |
| 60.2             | -172.9                        | -173.2 |
| 70.3             | -172.0                        | -172.6 |
| 80.3             | -172.9                        | -173.3 |
| 90.4             | -175.8                        | -175.2 |
| 100.4            | -176.1                        | -174.3 |
| 110.4            | -176.3                        | -173.2 |
| 120.5            | -175.7                        | -172.9 |
| 130.5            | -174.2                        | -172.3 |
| 140.5            | -173.7                        | -172.7 |
| 150.6            | -172.3                        | -171.6 |
| 160.6            | -170.0                        | -170.8 |
| 170.7            | -169.3                        | -171.3 |
| 180.7            | -170.2                        | -171.6 |
| 190.7            | -172.2                        | -173.4 |
| 200.0            | -174.5                        | -175.7 |

| # | Quantity | Part                                                                                                                                                                                        | Issue | Type   | Resolution |
|---|----------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------|--------|------------|
| 4 | 1 ea     | SB35-ETH - icListen HF - Ethernet,<br>3500m Depth Rating, 10 Hz - 200<br>kHz. Includes case, test cable and<br>power adapter, with 256 GB<br>memory. Country/Origin: Canada<br>SN(s): 1250; |       | Repair |            |

-----  
US Shipments

If you need to inform the ECCN code please use the following:

- \* The ECCN code for deep hydrophones (more than 1000m) is 6A001.a.2.a.6
- \* The ECCN code for our 200m and 900m (less than 1000m) hydrophones is EAR99

-----  
General Shipping Instructions for the Return of **RMA#757** to Ocean Sonics:

1. \*\*Please, when shipping the goods back to Canada use the HS code 901590 for the accessories and HS code 901580 for the hydrophones.. State clearly on the airway bill, customs declaration form and commercial invoice, "NOT FOR SALE! Canadian Goods Returning for Repair. Value is for Customs Purposes Only." and the RMA #757.

Important: If you are shipping more than 2 hydrophones, declare when filling your air way bill: Ion lithium battery contained in equipment (UN3481, PI 967, section II).

Some courier companies have this drop-down option. If there is you must choose it. If there is not, you have to write this statement in the comment section of after the description of the goods.

Outside the box place two UN3481 labels, one in each opposite side, and with a marker, write near the label: 'PI 967 - II'

2. Print and add the RMA document to the box with the returning unit.

3. When filling the airway and the Commercial Invoice for the return please add the following:  
NOTIFY:

PF Collins

251 E White Hills Rd #100, St. John's, NL A1A 5X7

Canada

Email: import@pfcollins.com , Phone: +1 709 726 7596

NOTE: If the courier company has the option, you can use the Broker Select Option (BSO). This way our broker will be notified upon arrival in Canada.

4. Guideline for valuation of returned equipment: The value for cross border shipment is used for transport insurance and customs value. It should represent the replacement cost of the equipment (to same standard equipment). We suggest 100% of the equipment value.

5. By sending the RMA I acknowledge that the item(s)listed herein are returned without having been advanced in value or improved in condition by any process of manufacture or other means. I acknowledge that all repairs are subject to the Ocean Sonics Terms and Conditions.