F10E | Batch isolation reveals four independent S/O failures

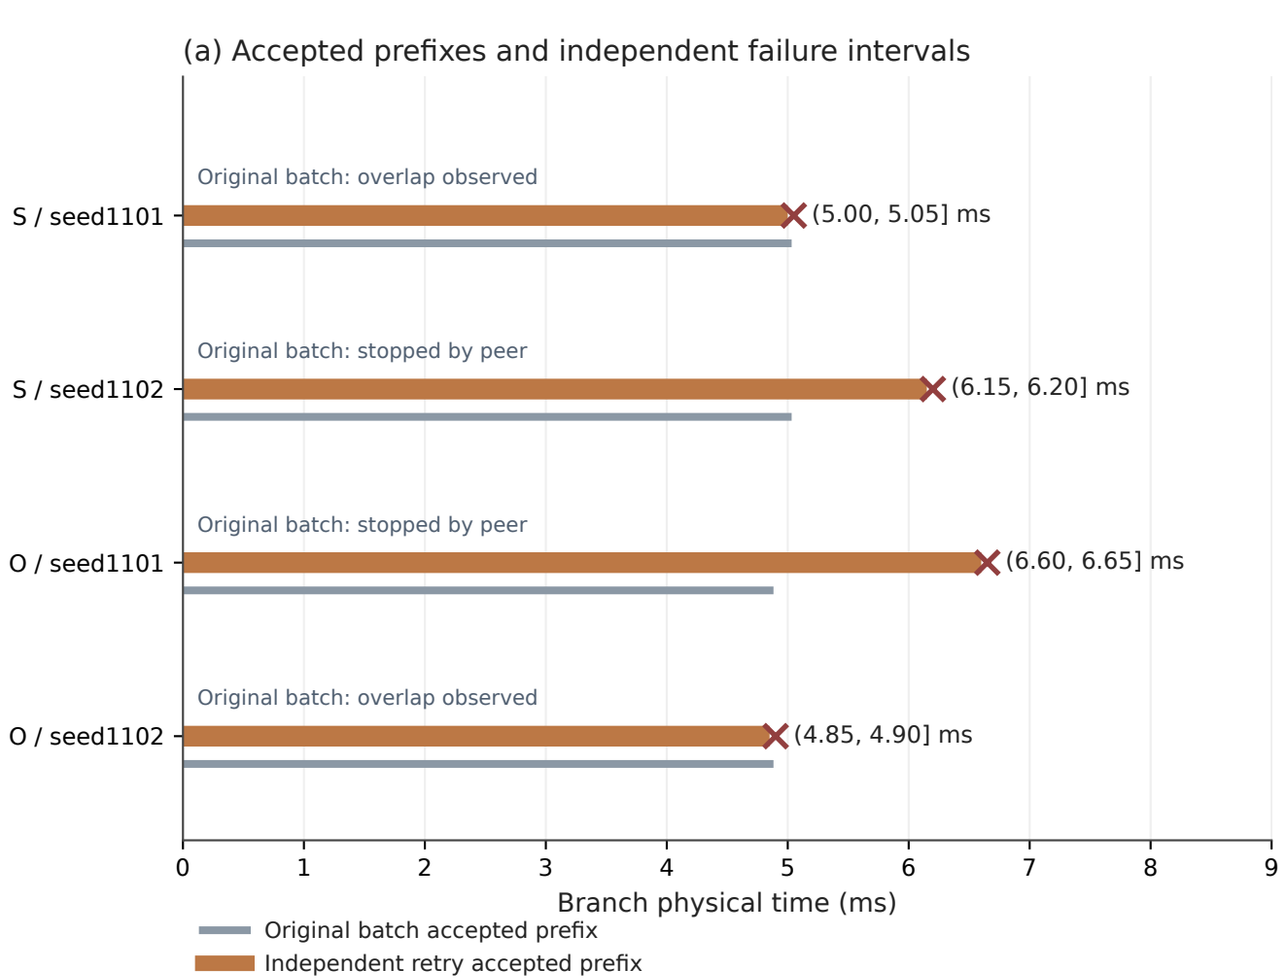

(b) Original 10 µs / 12-round outcomes
Failure times in ms

	Preparation	OFF	S	O
seed1101	PASS	PASS	FAIL (5.00, 5.05]	FAIL (6.60, 6.65]
seed1102	PASS	PASS	FAIL (6.15, 6.20]	FAIL 4.900 ms
seed1103	FAIL (9.45, 9.50]	Not run	Not run	Not run
seed1104	FAIL 2.240 ms	Not run	Not run	Not run

Recovered complete trajectories: 0
Complete OFF/S/O seed families: 0 / 4

Intervals are verified 50-µs brackets; 2.240 and 4.900 ms are step-resolved diagnostics. All four retry prefixes match the original batch.