

F10M | Confirmed apparatus geometry

a Centered PDMS channel and three 7 mm ceramic faces

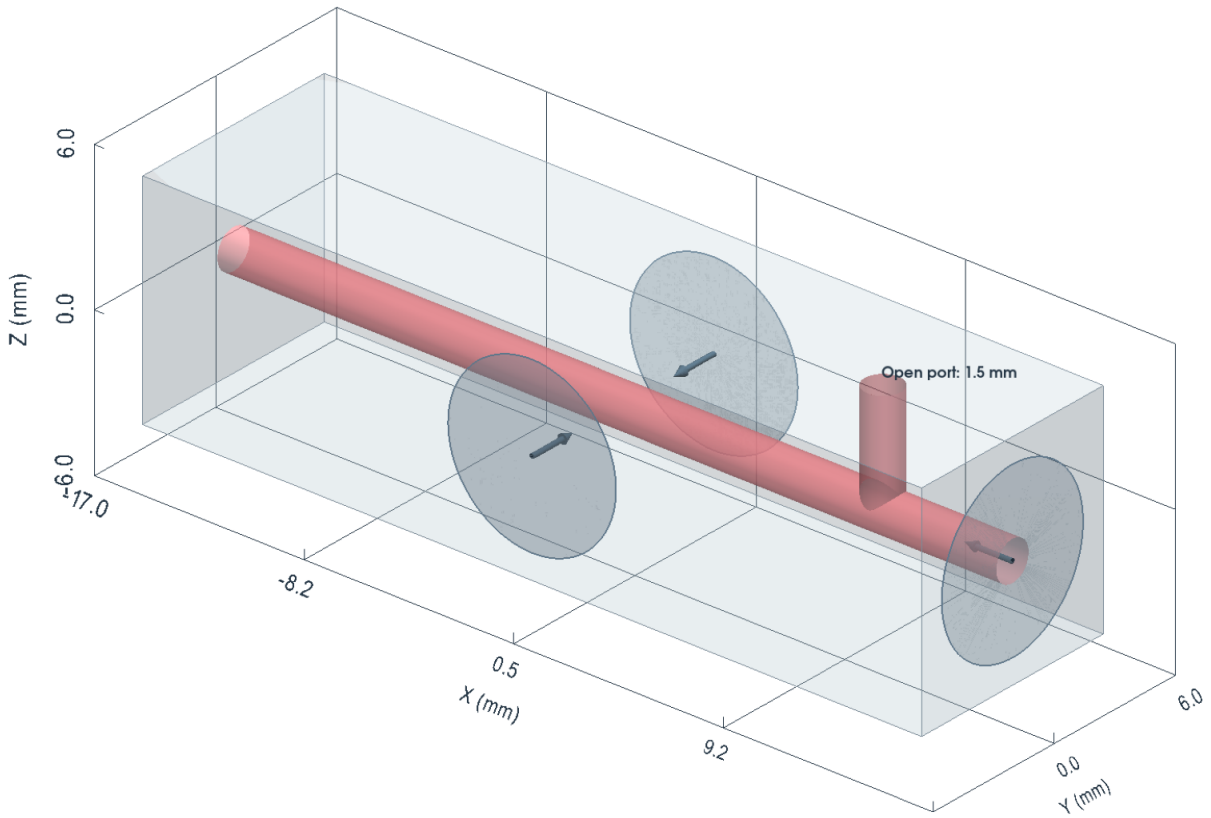

b XY orthographic projection

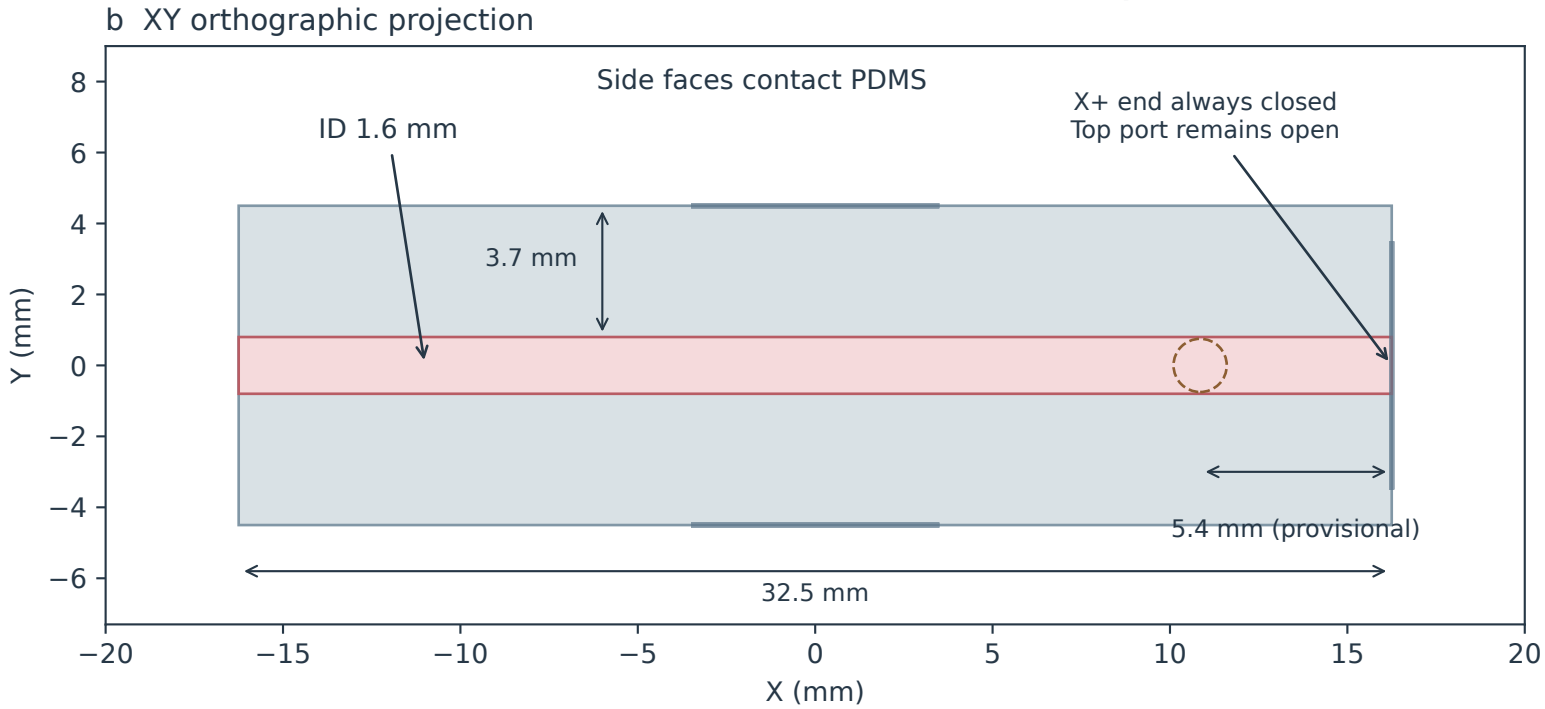

PDMS: 32.5 × 9 × 9 mm. Centered through-channel: ID 1.6 mm. No independent thin tube wall.
True dimensional ratios; translucent display only. Normals point inward. Top port: ID 1.5 mm, open; X+ end: closed. 5.4 mm reference and lateral centering are provisional.