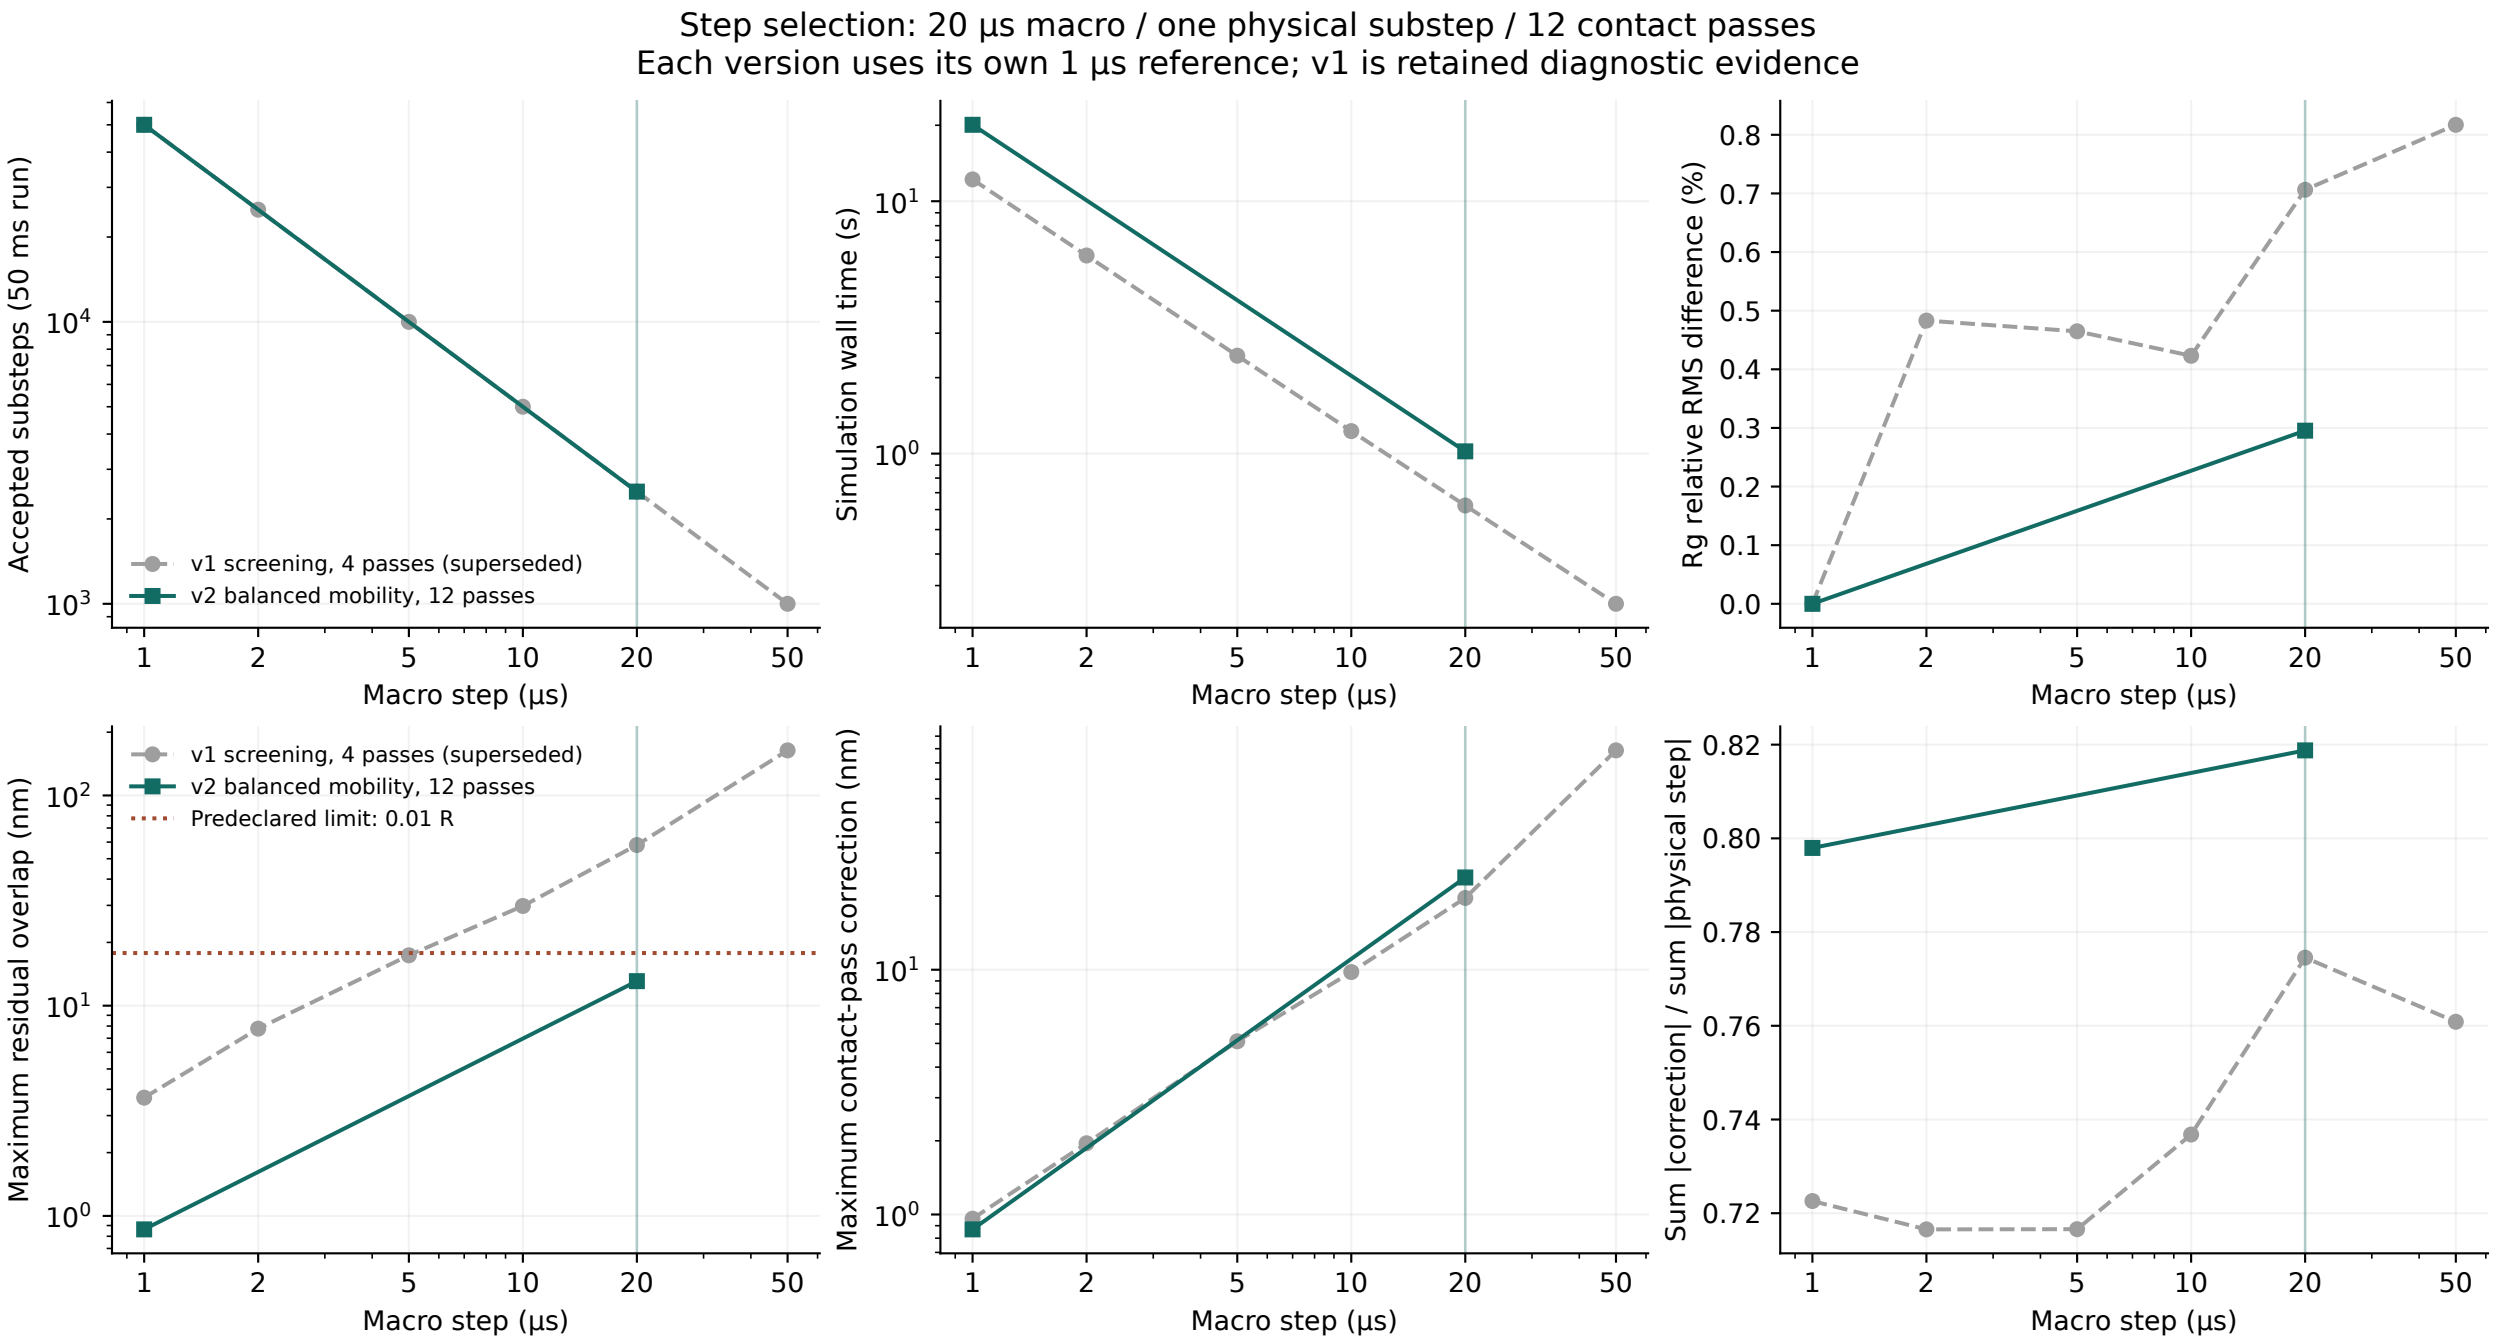
Step selection: 20 µs macro / one physical substep / 12 contact passes
Each version uses its own 1 µs reference; v1 is retained diagnostic evidence
Accepted substeps (50 ms run)
Simulation wall time (s)
Rg relative RMS difference (%)
Maximum residual overlap (nm)
Maximum contact-pass correction (nm)
Sum |correction| / sum |physical step|
Macro step (µs)
v1 screening, 4 passes (superseded)
v2 balanced mobility, 12 passes
Predeclared limit: 0.01 R