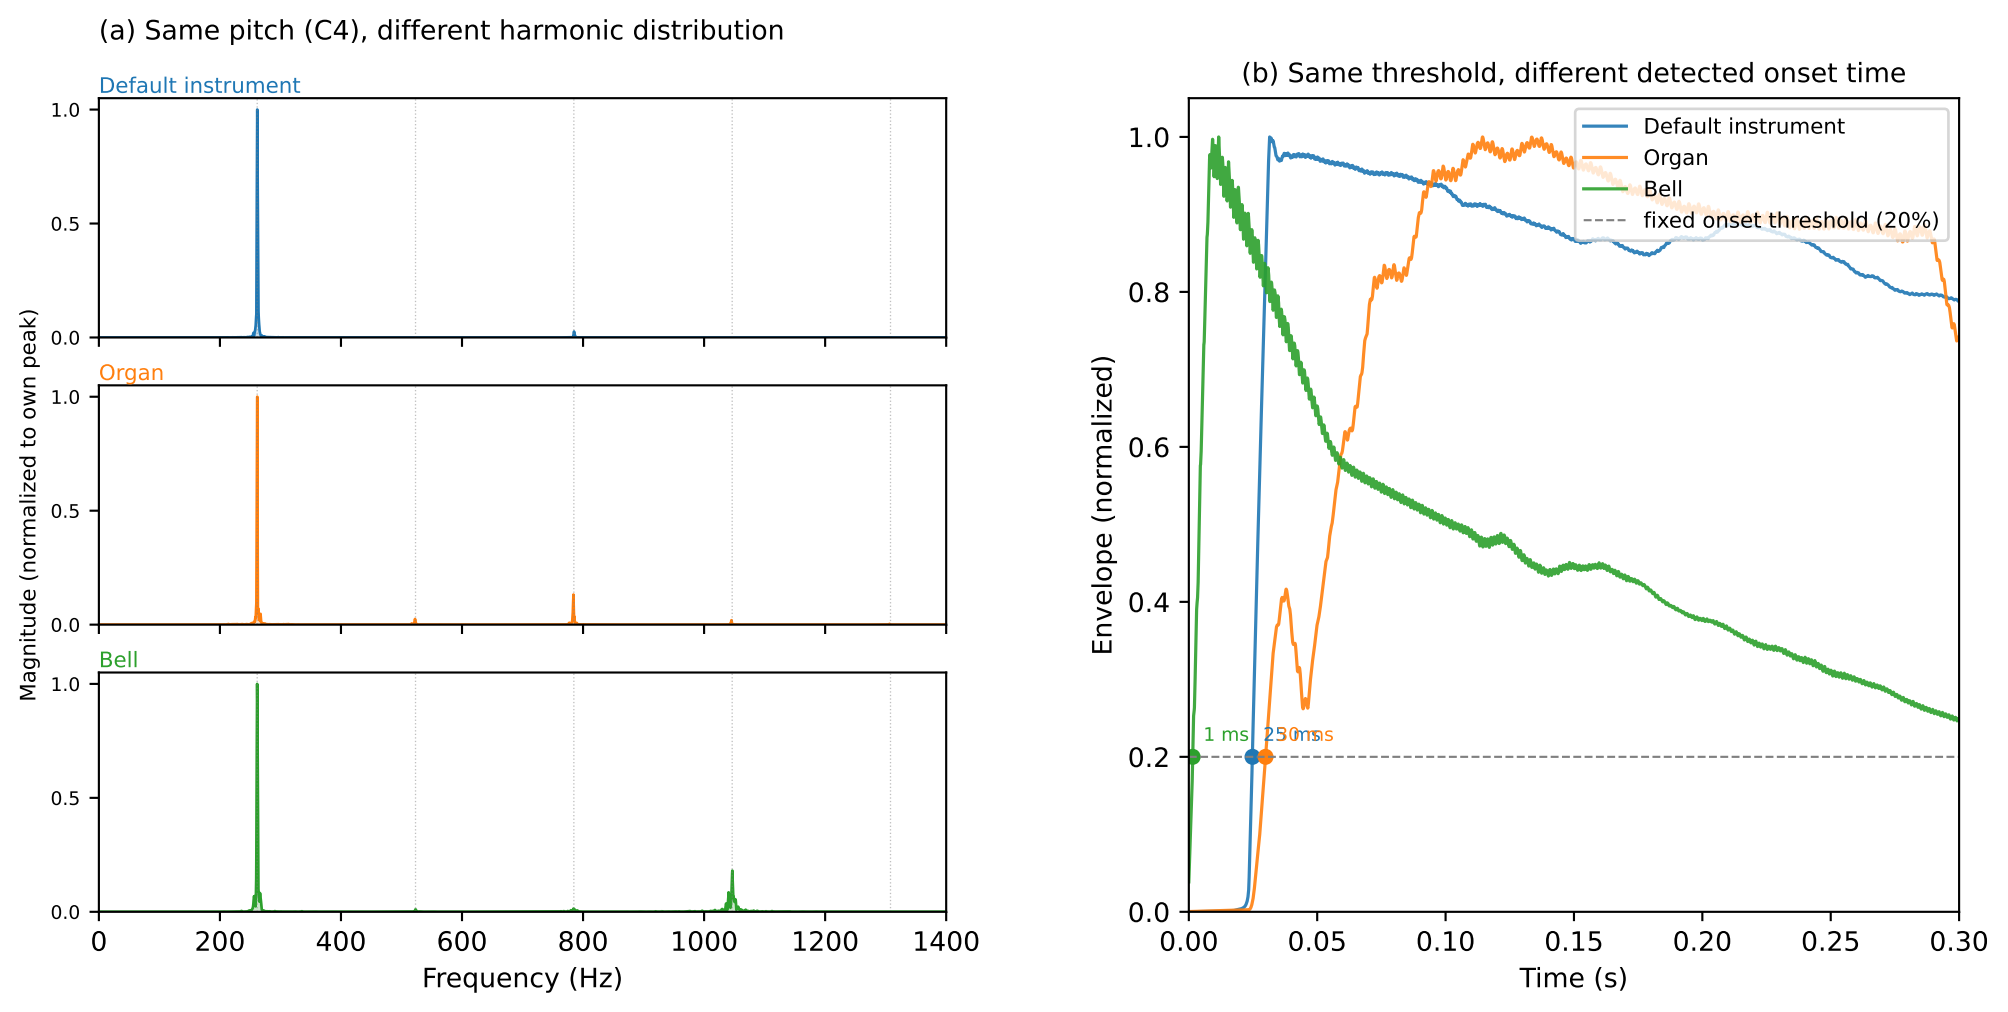

(a) Same pitch (C4), different harmonic distribution
Default instrument
Organ
Bell
Magnitude (normalized to own peak)
Frequency (Hz)
(b) Same threshold, different detected onset time
Default instrument
Organ
Bell
fixed onset threshold (20%)
1 ms
250 ms
Envelope (normalized)
Time (s)