



# Parallel probes 9373/170 and 9373/340 agree across the thesis band — validation for using their mean as the canonical IN reference


(a) Parallel-probe FFT amplitudes

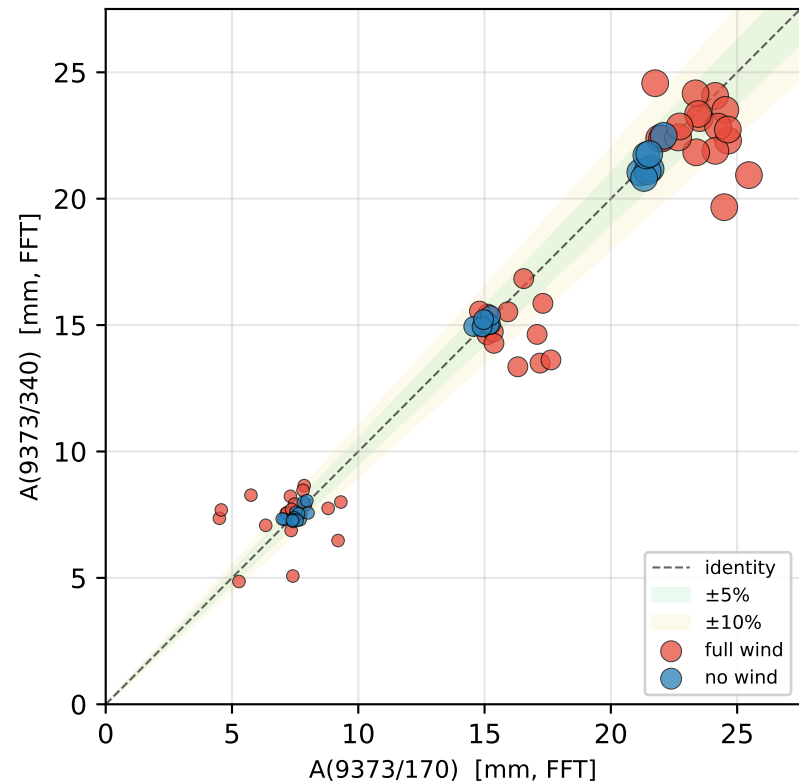

(b) Disagreement vs input amplitude

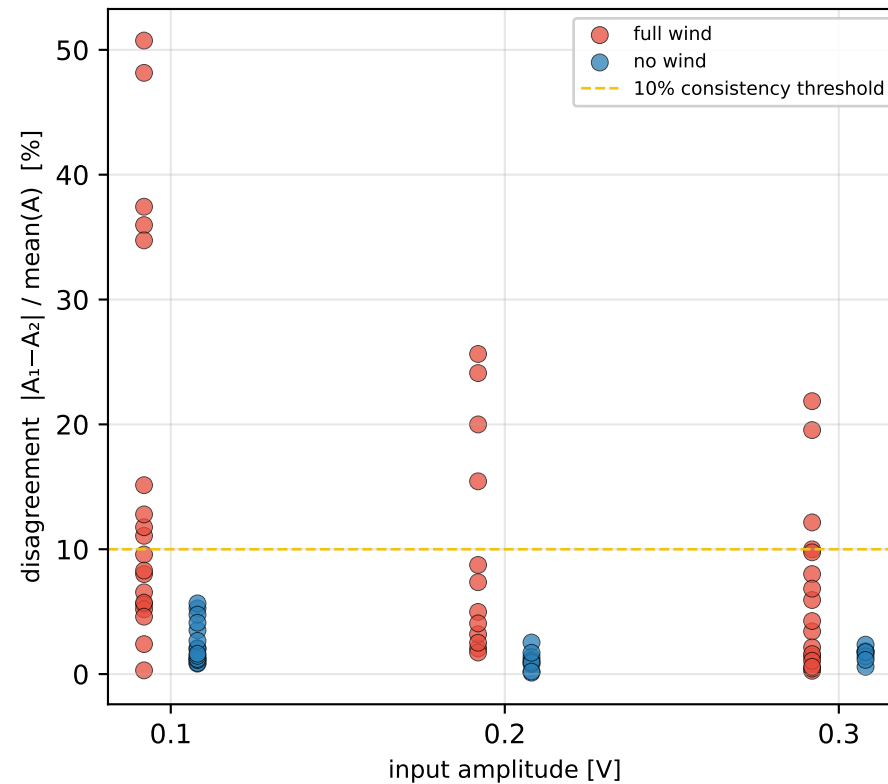

(c) Mean disagreement per (freq, amp, wind)

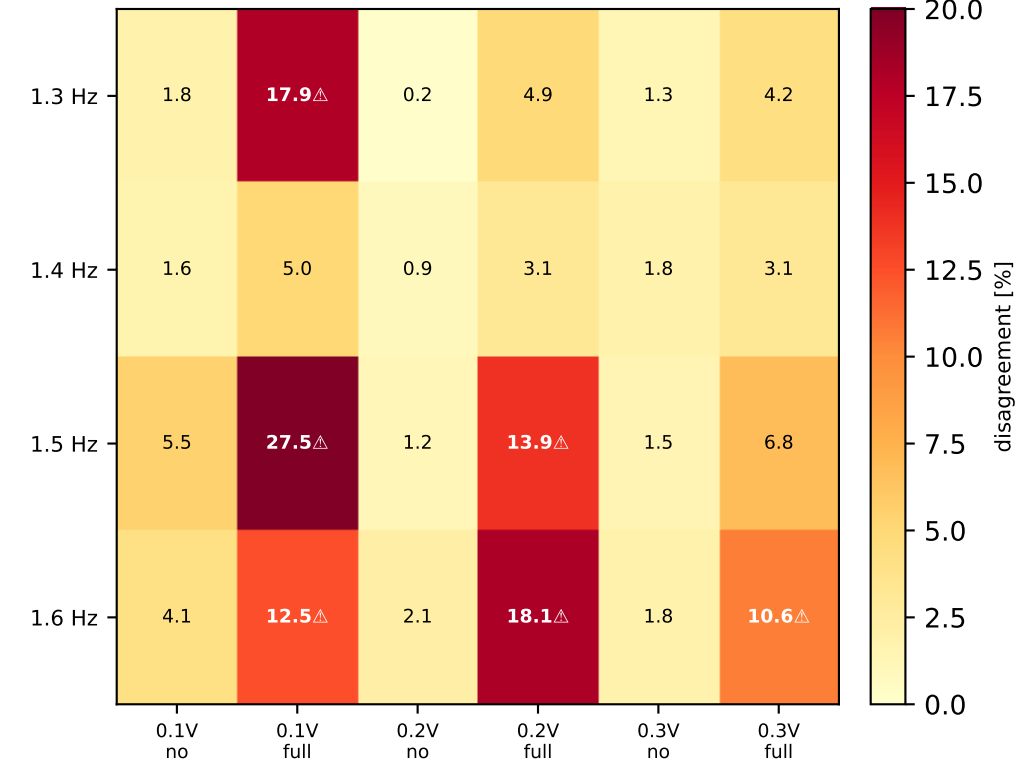

Scope: 78 quality-ok full-panel wave runs, 1.3–1.6 Hz, cond4 lowrange. 62/78 (79%) consistent at 10% threshold. Disagreement is concentrated in 0.1 V fullwind — the low-SNR regime where wind contamination affects each probe differently.