



ENVIRONMENTAL MONITORING REPORT

Report Type: DAILY

Generated: 4/6/2026, 1:12:42 PM

1. Executive Summary

This report presents environmental monitoring data collected from EBA System over period of 4/6/2026 to 4/6/2026. A total of 20 data points were recorded and analysed. During this period, the average temperature was 24.4°C, with a maximum of 29.4°C and a minimum of 0.0°C. Relative humidity averaged 50.8%. CO2 levels averaged 287 ppm.

Data Overview

Total Records: 20

Date Range: 4/6/2026 to 4/6/2026

Parameters: Temperature,
Humidity, CO2, Soil Moisture,
Water Level

2. Detailed Sensor Data

Timestamp	Temp (°C)	Humidity (%)	CO2 (ppm)	Soil (%)	Water (%)
4/6/2026, 12:14:58 PM	0.0°C	0.0%	0	0	0
4/6/2026, 12:16:54 PM	0.0°C	0.0%	0	0	0
4/6/2026, 12:17:11 PM	27.3°C	69.4%	390	0	0
4/6/2026, 12:20:51 PM	28.1°C	61.9%	380	0	0
4/6/2026, 12:22:14 PM	28.5°C	60.8%	370	0	0
4/6/2026, 12:27:10 PM	28.7°C	60.9%	360	0	0
4/6/2026, 12:27:14 PM	28.7°C	60.9%	360	0	0
4/6/2026, 12:32:10 PM	29.1°C	59.8%	350	0	0
4/6/2026, 12:32:14 PM	29.1°C	59.8%	350	0	0
4/6/2026, 12:37:10 PM	29.3°C	57.8%	340	0	0
4/6/2026, 12:37:14 PM	29.3°C	57.8%	340	0	0
4/6/2026, 12:42:10 PM	29.4°C	58.6%	330	0	0
4/6/2026, 12:42:14 PM	29.4°C	58.6%	330	0	0
4/6/2026, 12:47:14 PM	29.1°C	58.2%	320	0	0
4/6/2026, 12:52:14 PM	28.7°C	58.4%	310	0	0
4/6/2026, 12:54:22 PM	0.0°C	0.0%	0	0	0
4/6/2026, 12:57:14 PM	28.9°C	58.7%	300	0	0
4/6/2026, 1:02:14 PM	28.8°C	56.9%	300	0	0
4/6/2026, 1:07:14 PM	28.4°C	58.5%	300	0	0
4/6/2026, 1:12:14 PM	28.1°C	59.2%	300	0	0

3. Statistical Analysis

This section provides statistical analysis of all monitored environmental parameters. For Temperature, values ranged from 27.3 to 29.4 °C, with an average of 28.8 °C and a standard deviation of 0.5 °C. For Humidity, values ranged from 56.9 to 69.4 %, with an average of 59.8 % and a standard deviation of 2.7 %. For CO2, values ranged from 300.0 to 390.0 ppm, with an average of 337.1 ppm and a standard deviation of 28.4 ppm.

Temperature Analysis

Min: 27.3°C Max: 29.4°C Avg: 28.8°C Std Dev: 0.5°C

Humidity Analysis

Min: 56.9% Max: 69.4% Avg: 59.8% Std Dev: 2.7%

CO2 Analysis

Min: 300.0ppm Max: 390.0ppm Avg: 337.1ppm Std Dev: 28.4ppm

4. Data Visualizations

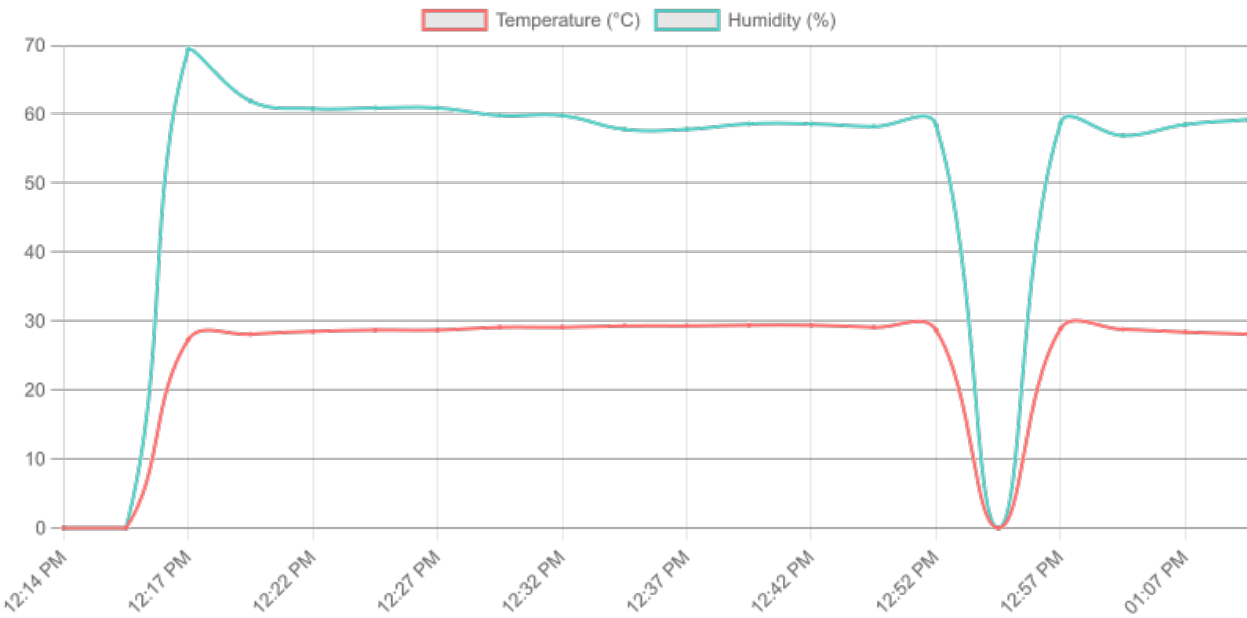


Figure 1: Time series analysis

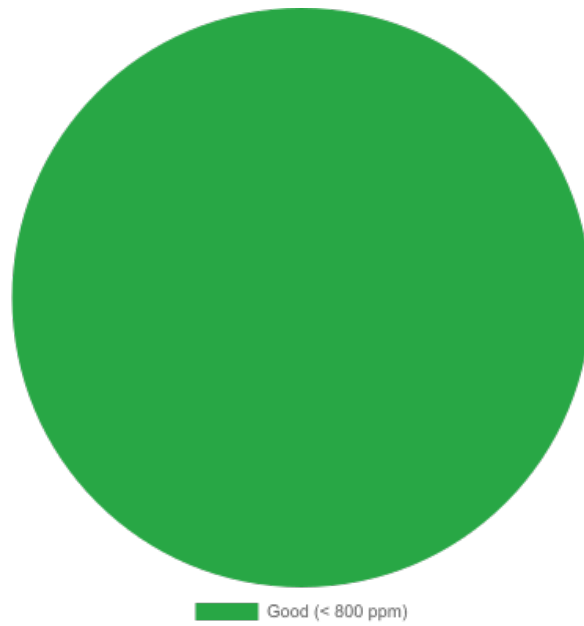


Figure 2: CO2 Level Distribution

5. Recommendations

Based on collected data, the following actions are recommended:

- Temperature levels are within optimal range. Continue regular monitoring.
- Humidity levels are within optimal range. Continue regular monitoring.
- CO2 levels are within acceptable ranges. Continue regular monitoring.