Kera


A closer look at hemoglobin

Kera explores a simpler first check for caregivers:
an experimental estimate from a fingernail photo.

Experimental research prototype

A scan stays on your device

Capture a photo. Mark the nail, skin and white reference. Get an estimate.

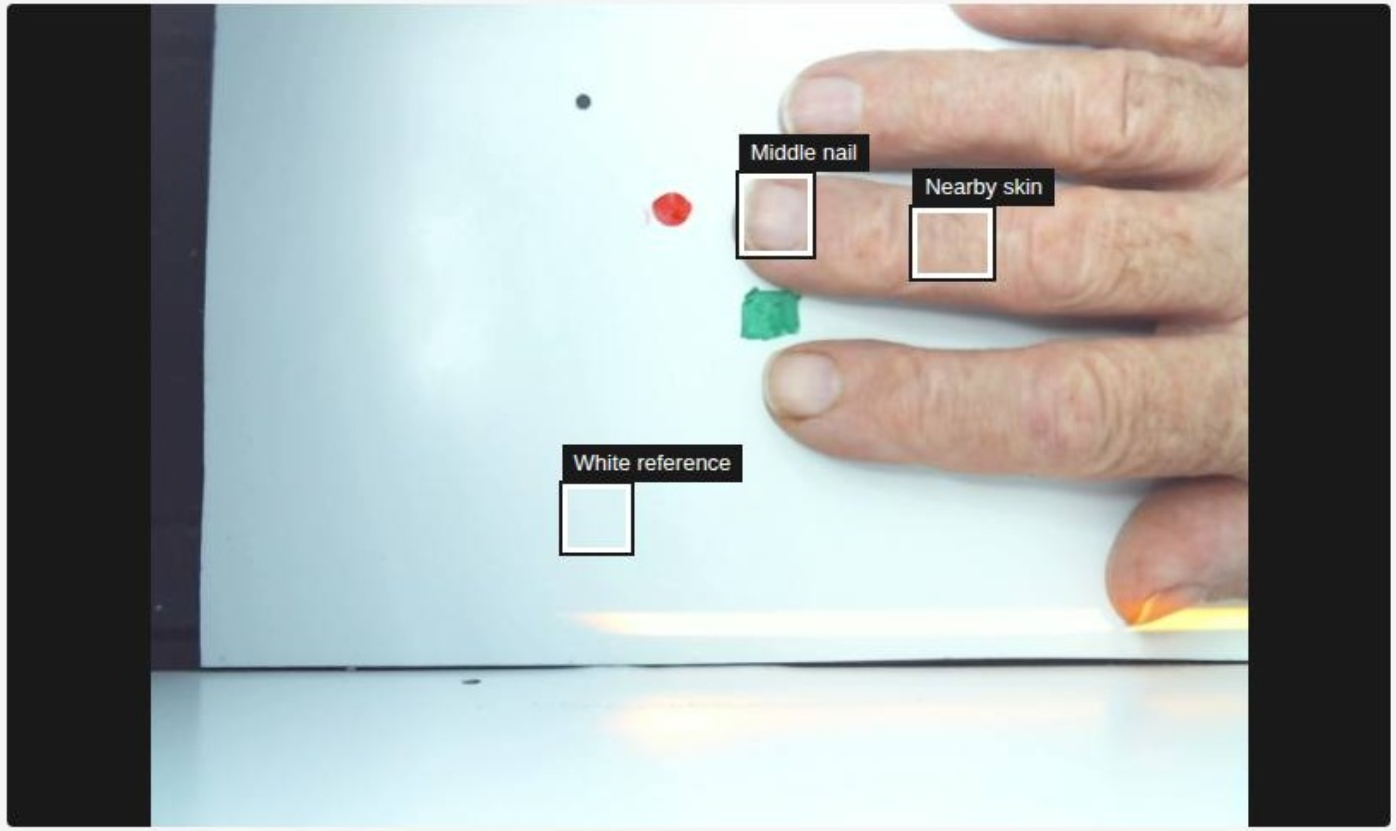

Your estimate.

126.4 g/L

Estimated hemoglobin

An experimental reading from your photo. This does not diagnose or rule out anemia.

Low hemoglobin can be overestimated. Confirm any health concern with a clinician and a blood test.

Take another photo ↗


Adjust regions

Demonstration uses a study image. Webcam performance remains unvalidated.

Model performance

15.96 g/L

Mean absolute error
on 50 held-out patients

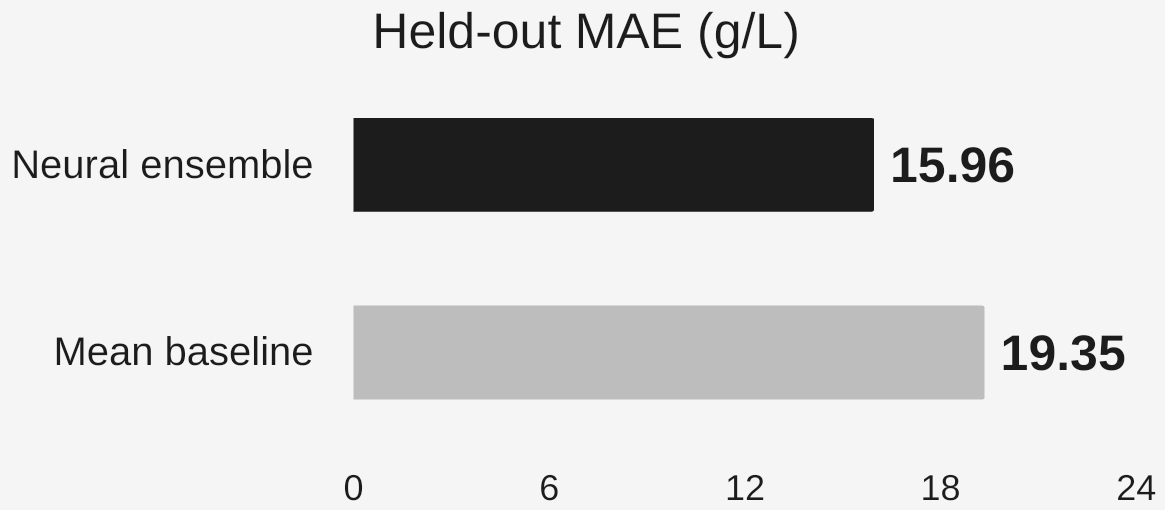

250 study patients
200 for training, 50 held out

Low hemoglobin remains the hard case

The model overestimated Hb by 16.26 g/L on average
in the 11 test patients below 120 g/L.

Kera

The next step: Kera Dock validation

Seeking a care or clinical research partner to pair Kera Dock scans with laboratory hemoglobin results.

Measure camera transfer and repeatability.
Validate across the intended older-adult population.