


IEC 61010-1			
Clause	Requirement — Test	Result — Remark	Verdict

6	TABLE: Protection against electric shock - Block diagram of system Form A.5		P
---	--	--	---

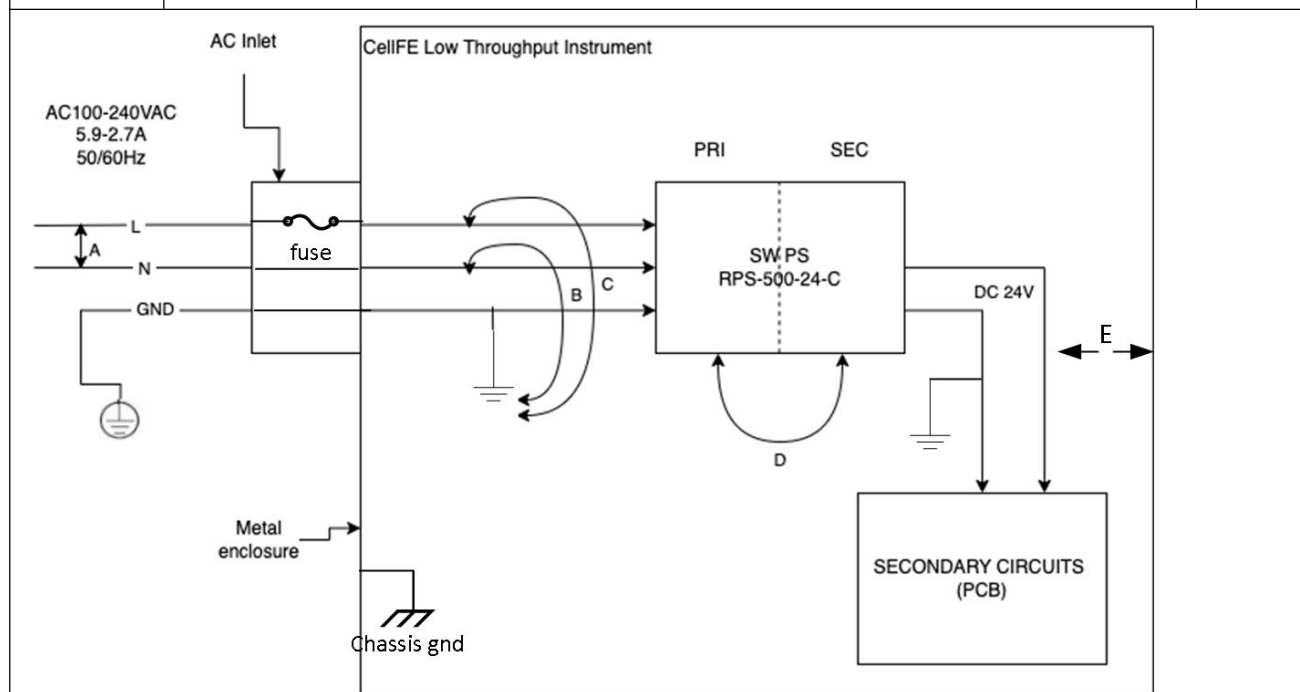

Pollution degree :2

Overvoltage category: II

Location or description	Insulation type (NOTE 1)	Maximum working voltage (NOTE 2)	CREEPAGE Distance (NOTE 3)				CLEARANCE (NOTE 3) mm	Test voltage (NOTE 2) V	Comments
			PWB mm	CTI	Other mm	CTI			
A	BI	240Vrms	1.5	≥100	3.0	>100	1.5		Line to Neutral before fuse
B and C	BI	240Vrms	1.5	≥100	3.0	>100	1.5		Line neutral to GND
D	RI or DI	240Vrms+24Vdc	3.0	≥100	6.0	>100	3.0		Part of power supply
E	BI	24Vdc	0.04	≥100	1.25	≥100	0.5		Secondary to chassis

NOTE 1 – Type of insulation:

BI = BASIC INSULATION

DI = DOUBLE INSULATION

PI = PROTECTIVE IMPEDANCE

RI = Reinforced INSULATION peak SI = Supplementary INSULATION

NOTE 2 - Types of voltage

Peak impulse test voltage (pulse)

r.m.s.

d.c.

NOTE 3 - INSTALLATION CATEGORIES

(OVERVOLTAGE CATEGORIES)

or POLLUTION DEGREES which differ from these should be shown under "Comments".