

Company:	Gener8 LLC.	Engineer/Technician:	Toufik Belahdar 
Project #:	G105581614	CB Mentor:	Kathy Ma 
		Reviewer:	Mike Brousseau 
Models:	TBD	Date:	10/31/2023
Product Name:	CellFE Infinity MTx	Sample Condition:	Production
Standard(s):	IEC 61010-1:2010Ed.3+A1 Safety Requirements for Electrical Equipment for Measurement, Control, And Laboratory Use Part 1: General Requirements UL 61010-1:2012Ed.3 Electrical Equipment For Measurement, Control, And Laboratory Use - Part 1: General Requirements CSA C22.2#61010-1:2004Ed.2+G1 Safety Requirements for Electrical Equipment for Measurement, Control, And Laboratory Use Part 1: General Requirements (R2009) IEC 61010-2-081:2019 Ed.3 Safety Requirements for Electrical Equipment for Measurement, Control, and Laboratory Use – Part 2-081: Particular Requirements for Automatic and Semi-automatic Laboratory Equipment for Analysis and Other Purposes UL 61010-2-081:2019 Ed.3 Safety Requirements for Electrical Equipment for Measurement, Control, and Laboratory Use - Part 2-081: Particular Requirements for Automatic and Semi-Automatic Laboratory Equipment for Analysis and other Purposes CSA C22.2#61010-2-081:2019 Ed.3 Safety Requirements for Electrical Equipment for Measurement, Control, and Laboratory Use - Part 2-081: Particular Requirements for Automatic and Semi-Automatic Laboratory Equipment for Analysis and other Purposes		

Scope of Project:

cETLus/CB certification and report for CellFE Infinity MTx – Safety

Quote No:

Qu-01390131-0

Evaluation Period:

October 02, 2023 – Oct 31, 2023

Evaluation Summary:

Description and intended use of product:

CellFE's Infinity Platform is designed to deliver a wide range of payloads into any cell type, even with the most complex editing protocols needed to develop increasingly advanced cell therapies. This technology effectively delivers mRNA, CRISPR, Cas9 protein, and plasmid DNA and consists of the following two components:

CellFE's Infinity MTx™ platform is a microfluidic transfection methodology that offers a novel way to transfect cells rapidly and simply. The platform successfully delivers a wide range of payloads into any cell type, even with the most complex editing protocols needed to develop increasingly advanced cell therapies. This technology has demonstrated effective delivery of mRNA, CRISPR Cas9 protein, and plasmid DNA while maintaining pre-transfection proliferation rates, cellular phenotypes, and cell subset ratios.

The Infinity Microfluidic Processing Assembly (MPA) is a single use device wherein the transfection process occurs. The MPA contains sterilized membranes and an actuating lid that allows for aseptic use of the Infinity MTx platform outside of a biosafety cabinet. When the Infinity MTx platform directs the flow of cells through microfluidic channels, they pass under a single chevron ridge. This change in channel size leads to rapid cellular compression causing a fleeting loss of intracellular fluid and a subsequent decrease in cell size. Upon re-expansion, within milliseconds, the target payload is actively transported into the cell. This is known as VECT. The MPA is designed to process 8 separate channels of 25-100 uL and up to 2 million cells.

Equipment Ratings:

100-240VAC, 5.9-2.7A, 50/60Hz

Testing:

Refer to IEC 61010-1 TDP in EPF

Deliverables:

105581614MPK-001A (Letter report)

Draft IEC 61010-1 Report shared

Deliverable	☐ Listing	☐ LPC	☐ NC Rpt	☐ CB	☒ TRF	☒ Letter	☐ Data Only
-------------	----------------------------------	------------------------------	---------------------------------	-----------------------------	---	--	------------------------------------

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
4	TESTS		TBD
4.4	Testing in SINGLE FAULT CONDITIONS		TBD
4.4.1	Fault tests	(see Form A.1)	TBD
4.4.2	Application of SINGLE FAULT CONDITIONS		TBD
4.4.2.1	SINGLE FAULT CONDITIONS not covered by 4.4.2.2 to 4.4.2.14	(see Form A.1)	TBD
4.4.2.2	PROTECTIVE IMPEDANCE		N/A
4.4.2.3	PROTECTIVE CONDUCTOR	(see Form A.6)	N/A
4.4.2.4	Equipment or parts for short-term or intermittent operation	Continuous operation	N/A
4.4.2.5	Motors	Fan is only accessible motor	—
	– stopped while fully energized		N/A
	– prevented from starting		N/A
	– one phase interrupted (multi-phase)	DC Motor only	N/A
4.4.2.6	Capacitors		N/A
4.4.2.7	MAINS transformers		N/A
4.4.2.7.2	Short circuit	(see Form A.39)	N/A
4.4.2.7.3	Overload	(see Forms A.26B and A.40)	N/A
4.4.2.8	Outputs		N/A
4.4.2.9	Equipment for more than one supply	Only one supply	N/A
4.4.2.10	Cooling	(see Form A.26A)	—
	– air holes closed	Testing required	TBD
	– fans stopped	Testing required	TBD
	– coolant stopped	No coolant	N/A
	– loss of cooling liquid	No cooling liquid	N/A
4.4.2.11	Heating devices	No heating devices	—
	– timer overridden		N/A
	– temperature controller overridden		N/A
4.4.2.12	Insulation between circuits and parts		N/A
4.4.2.13	Interlocks	No interlocks	N/A
4.4.2.14	Voltage selectors	No voltage selectors	N/A
4.4.3	Duration of tests	(see Form A.1)	—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict

4.4.4	Conformity after application of fault conditions	(see Forms A.1, A.6 and A.18)	TBD
-------	--	-------------------------------	-----

5	MARKING AND DOCUMENTATION		F
5.1	Marking	No markings on equipment	F
5.1.1	General		F
	Required equipment markings		—
	– Visible from the exterior; or		F
	– Visible after removing cover or opening door		F
	– Visible after removal from a rack or panel		F
	Not put on parts which can be removed by an operator		F
	Letter symbols (IEC 60027) used		F
	Graphic symbols of Table 1 used		F
5.1.2	Identification		F
	Equipment is identified by:		—
	a) Manufacturer's or supplier's name or trademark	Manufacturer: CellFe	P
	b) Model number, name or other means	No model identification on equipment	F
	Manufacturing location identified		N/A
5.1.3	MAINS supply	No electrical ratings on equipment.	F
	Equipment is marked as follows:		—
	a) Nature of supply:		—
	1) a.c. RATED MAINS frequency or range of frequencies.....:	No electrical ratings on equipment.	—
	2) d.c. with symbol 1.....:		—
	b) RATED supply voltage(s) or range.....:	No electrical ratings on equipment.	—
	c) Max. RATED power (W or VA) or input current.....:	No electrical ratings on equipment.	—
	The marked value not less than 90 % of the maximum value	(see Form A.2)	F
	If more than one voltage range:		—
	Separate values marked; or		N/A
	Values differ by less than 20 %	(see Form A.2)	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	d) OPERATOR-set for different RATED supplyvoltages:	No such construction	—
	Indicates the equipment set voltage		N/A
	PORTABLE EQUIPMENT indication is visible from the exterior	Not portable equipment	N/A
	Changing the setting changes the indication		N/A
	e) Accessory MAINS socket-outlets accepting standard MAINS plugs are marked:	No such construction	N/A
	With the voltage if it is different from the MAINS supply voltage..... :		N/A
	For use only with specific equipment		N/A
	If not marked for specific equipment it is marked with:		N/A
	The maximum RATED current or power; or		N/A
	Symbol 14 with full details in the documentation		N/A
5.1.4	Fuses		P
	OPERATOR replaceable fuse marking (see also 5.4.5)..... :		—
5.1.5	TERMINALS, connections and operating devices	None provided in the equipment	F
5.1.5.1	General		N/A
	Where necessary for safety, indication of purpose of TERMINALS, connectors, controls and indicators marked		N/A
	If insufficient space, symbol 14 used		N/A
	Push-buttons and actuators of emergency stop devices and indicators:		—
	– used only to indicate a warning of danger; or		N/A
	– the need for urgent action		N/A
	– coloured red		N/A
	– coded as specified in IEC 60073		N/A
	Supplementary means of coding provided, if meaning of colour relates (see IEC 60073):		—
	– to safety of persons; or		N/A
	– safety of the environment		N/A
5.1.5.2	TERMINALS	No such terminals	—
	MAINS supply TERMINAL identified		N/A
	Other TERMINAL marking:		—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	a) FUNCTIONAL EARTH TERMINALS marked with symbol 5	No functional earth terminal on equipment	N/A
	b) PROTECTIVE CONDUCTOR TERMINALS:		—
	Symbol 6 is placed close to or on the TERMINAL; or	Symbol 6  provided on equipment	P
	Part of appliance inlet		N/A
	c) TERMINALS of circuits (symbol 7 used)		N/A
	d) HAZARDOUS LIVE TERMINALS supplied from the interior		N/A
	Standard MAINS socket outlet used; or		N/A
	RATINGS marked; or		N/A
	Symbol 14 used		N/A
5.1.6	Switches and circuit-breakers	Equipment incorporates a switch as means of disconnecting	P
	If disconnecting device, off position clearly marked		P
	If push-button used as power supply switch:	No push-button	N/A
	– Symbol 9 and 15 used for on-position	Switch uses symbol 9 for on-position	P
	– Symbol 10 and 16 used for off-position	Switch uses symbol 10 for off-position	P
	– Pair of symbols 9, 15 and 10, 16 close together		N/A
5.1.7	Equipment protected by DOUBLE INSULATION or REINFORCED INSULATION	Basic insulation	N/A
	Protected throughout (symbol 11 used)		N/A
	Only partially protected (symbol 11 not used)		N/A
5.1.8	Field-wiring TERMINAL boxes	No such construction	N/A
	If TERMINAL or ENCLOSURE exceeds 60 °C:	(see Form A.26A)	N/A
	Cable temperature RATING marked.....:		N/A
	Marking visible before and during connection or beside TERMINAL		N/A
5.2	Warning markings		
	Visible when ready for NORMAL USE		
	Are near or on applicable parts		
	Symbols and text correct dimensions and colour:		—

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	a) Symbols min 2,75 mm and text 1,5 mm high and contrasting in colour with background		
	b) Symbols and text moulded, stamped or engraved in material min. 2,0 mm high and		
	0,5 mm depth or raised if not contrasting in colour		
	If necessary marked with symbol 14, or		
	Additional symbols such as symbol 12, 13 or 17 used to indicate the nature of HAZARD		
	Statement to place equipment in a safe state before access by using a tool to HAZARDOUS parts is permitted		
5.3	Durability of markings	Testing required	TBD
	The required markings remain clear and legible in NORMAL USE	(see Form A.3)	TBD
5.4	Documentation		
5.4.1	General		
	Equipment is accompanied by documentation for safety purposes for OPERATOR or RESPONSIBLE BODY	No such document provided with equipment	F
	Safety documentation for service personnel authorized by the manufacturer		
	Documentation necessary for safe operation is provided in printed media or		
	in electronic media if available at any time		
	Documentation includes:		—
	a) Intended use	None provided	F
	b) Technical specification	None provided	F
	c) Name and address of manufacturer or supplier	Provided on page 1 of the IFU (IFU-001 Rev. A) as follows: CellFE Biotech, Inc. 980 Atlantic Avenue, Suite 110 Alameda, CA 94501-1098	P
	d) Information specified in 5.4.2 to 5.4.6	None provided	F
	e) Information to mitigate residual RISK (see also subclause 17)		N/A
	f) Accessories for safe operation of the equipment specified	No such accessories required	N/A
	g) Guidance provided to check correct function of the equipment, if incorrect reading may cause a HAZARD		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	from harmful or corrosive substances of HAZARDOUS live parts		
	h) Instructions for lifting and carrying	No instructions for lifting or carrying	F
	Warning statements and a clear explanation of warning symbols:		—
	– provided in the documentation; or		
	– information is marked on the equipment		
5.4.2	Equipment RATINGS		F
	Documentation includes:		F
	a) Supply voltage or voltage range..... :	Incomplete/insufficient electrical ratings provided in IFU	F
	Frequency or frequency range.....:		F
	Power or current rating.....:		F
	b) Description of all input and output connections in accordance to 6.6.1 a)	None provided	F
	c) RATING of insulation of external circuits in accordance to 6.6.1 b)	No external circuits	N/A
	d) Statement of the range of environmental conditions (refer to 1.4):	None provided	—
	1) indoor or outdoor use,	Indoor use only	P
	2) altitude,	Provided in IFU: “ Up to 300 meters. ”	P
	3) temperature,	Provided in IFU: “ 20°C to 30°C ”	P
	4) relative humidity,	Provided in IFU: “ Up to 80% max relative humidity ”	P
	5) MAINS supply voltage fluctuations,	None provided in IFU	F
	6) OVERVOLTAGE CATEGORY,	None provided in IFU	F
	7) WET LOCATION, if applicable,	None provided in IFU	F
	8) POLLUTION DEGREE of the intended environment	None provided in IFU	F
	e) Degree of ingress protection (IEC 60529)	IP53 as stated under Appendix E of IFU	N/A
	f) If impact rating less than 5 J:		—
	IK code in accordance to IEC 62262 marked; or		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	symbol 14 of Table 1 marked, with		N/A
	RATED energy level and test method stated		N/A
5.4.3	Equipment installation	None provided	F
	Documentation includes instructions for:		—
	a) Assembly, location and mounting requirements		F
	b) Instructions for protective earthing	IFU states that equipment must use properly grounded 3-prong power cord	P
	c) Connections to supply	Provided in IFU	P
	d) PERMANENTLY CONNECTED EQUIPMENT:	Not permanently connected equipment	N/A
	1) Supply wiring requirements		N/A
	2) If external switch or circuit-breaker, requirements and location recommendation		N/A
	e) Ventilation requirements	Provided on page 9 in Chapter 1 of IFU “Do not block - Ensure at least 6” of clearance behind instrument.”	P
	f) Safety characteristics for special external services (e. g. maximum and minimum temperature, pressure, flow of air, cooling liquid)	Provided on page 9 in Chapter 1 of IFU Maximum pressurized air source: 120 psi	P
	g) Instructions relating to sound level	No hazard pertaining to sound level	N/A
5.4.4	Equipment operation	None provided	F
	Instructions for use include:		—
	a) Identification and description of operating controls		F
	b) Positioning for disconnection		F
	c) Instructions for interconnection to accessories or other equipment	Provided in IFU	F
	d) Specification of intermittent operation limits	EUT not intended for intermittent operation	F
	e) Explanation of symbols used	Upon evaluation, no symbols were physically present on the EUT	F
	f) Replacement of consumable materials	Provided in IFU	P

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	g) Cleaning and decontamination	Provided in IFU under Chapter 5, titled "Cleaning and Maintenance"	P
	h) Listing of any poisonous or injurious gases and quantities		F
	i) RISK reduction procedures relating to flammable liquids (see 9.5 c)	No flammable liquids used in equipment	N/A
	j) RISK reduction procedures relating burn from surfaces permitted to exceed limits of 10.1		F
	Additional precautions for IEC 60950 conforming equipment in regard to moistures and liquids		F
	A statement about protection impairment if used in a manner not specified by the manufacturer		F
5.4.5	Equipment maintenance and service	None provided in IFU	F
	Instructions for RESPONSIBLE BODY include:		—
	Instructions sufficient in detail permitting safe maintenance and inspection and continued safety:		—
	Instruction against the use of detachable MAINS supply cord with inadequate RATING	No such instruction found in the IFU	F
	Specific battery type of user replaceable batteries	No replaceable batteries	N/A
	Any manufacturer specified parts		F
	RATING and characteristics of fuses	No such ratings and characteristics of replaceable fuse found in IFU	F
	Instructions include following subjects permitting safe servicing and continued safety:		—
	a) Product specific RISKS may affect service personnel		F
	b) Protective measures for these RISKS		F
	c) Verification of the safe state after repair		F
5.4.6	Integration into systems or effects resulting from special conditions		N/A
	Aspects described in documentation		N/A

6	PROTECTION AGAINST ELECTRIC SHOCK		TBD
6.1	General	(see Forms A.14 and A.15)	TBD
6.1.1	Requirements		TBD
	Protection against electric shock maintained in NORMAL		TBD

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	CONDITION and SINGLE FAULT CONDITION		
	ACCESSIBLE parts not HAZARDOUS LIVE		TBD
	Voltage, current, charge or energy below the limits in NORMAL CONDITION and in SINGLE FAULT CONDITION between:		—
	ACCESSIBLE parts and earth		
	two ACCESSIBLE parts on same piece of the equipment within a distance of 1,8 m		
	Conformity is checked by the determination of 6.2 and 6.3 followed by the tests of 6.4 to 6.11		
6.1.2	Exceptions		
	Following HAZARDOUS LIVE parts may be ACCESSIBLE to an OPERATOR:		—
	a) parts of lamps and lamp sockets after lamp removal		
	b) parts to be replaced by OPERATOR only by the use of tool and warning marking		
	Those parts not HAZARDOUS LIVE 10 s after interruption of supply	(see Form A.5)	
	Capacitance test if charge is received from internal capacitor	(see Forms A.4 and A.5)	
6.2	Determination of ACCESSIBLE parts	(see Form A.4)	TBD
6.2.1	General	Testing required	TBD
	Unless obviously determination of ACCESSIBLE parts as specified in 6.2.2 to 6.2.4		TBD
6.2.2	Examination		TBD
	– with jointed test finger (as specified B.2)		TBD
	– with rigid test finger (as specified B.1) and a force of 10 N		TBD
6.2.3	Openings above parts that are HAZARDOUS LIVE		TBD
	– test pin with length of 100 mm and 4 mm in diameter applied		TBD
6.2.4	Openings for pre-set controls	No pre-set controls in equipment	N/A
	– test pin with length of 100 mm and 3 mm in diameter applied		N/A
6.3	Limit values for ACCESSIBLE parts	Testing required	TBD
6.3.1	Levels in NORMAL CONDITION	(see Form A.5)	TBD

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	a) Voltage limits less than 30 V r.m.s. and 42,4 V peak or 60 V d.c.		TBD
	for WET LOCATIONS voltage limits less than 16 V r.m.s. and 22,6 V peak or 35 V d.c.		TBD
	Voltages are not HAZARDOUS LIVE the levels of:		—
	b) Current less than 0,5 mA r.m.s. for sinusoidal, 0,7 mA peak non-sinusoidal or mixed frequencies or 2 mA d.c. when measured with measuring circuit A.1 or A.2 if less than 100 Hz		TBD
	for WET LOCATIONS measuring circuit A.4 used		N/A
	70 mA r.m.s. when measured with circuit A.3 for higher frequencies		N/A
	c) Levels of capacitive charge or energy less:		—
	1) 45 μ C for voltages up to 15 kV peak or d.c. or line A of Figure 3		N/A
	2) 350 mJ stored energy for voltages above 15 kV peak or d.c.		N/A
6.3.2	Levels in SINGLE FAULT CONDITION	(see Form A.6)	TBD
	a) Voltage limits less than 50 V r.m.s. and 70 V peak or 120 V d.c.	Testing required	TBD
	for WET LOCATIONS voltage limits less than 33 V r.m.s. and 46,7 V peak or 70 V d.c.		TBD
	Voltages are not HAZARDOUS LIVE the levels of:		—
	b) Current less than 3,5 mA r.m.s. for sinusoidal, 5 mA peak non-sinusoidal or mixed frequencies or 15 mA d.c. when measured with measuring circuit A.1 or A.2 if less than 100 Hz		TBD
	for WET LOCATIONS measuring circuit A.4 used		TBD
	500 mA r.m.s. when measured with circuit A.3 for higher frequencies		TBD
	c) Levels of capacitive charge or energy less line B of Figure 3		TBD
6.4	Primary means of protection		P
6.4.1	General		P
	ACCESSIBLE parts prevented from being HAZARDOUS LIVE by one or more of following means:		—
	a) ENCLOSURES or PROTECTIVE BARRIERS (see 6.4.2)	Metal enclosure provided	P
	b) BASIC INSULATION (see 6.4.3)	Basic insulation	P

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) Impedance (see 6.4.4)	No such protection	N/A
6.4.2	ENCLOSURES or PROTECTIVE BARRIERS	(see Forms A.15 and A.16)	
	– meet rigidity requirements of 8.1	Testing required	TBD
	– meet requirements for BASIC INSULATION, if protection is provided by insulation		
	– meet requirements of 6.7 for CREEPAGE and – CLEARANCES between ACCESSIBLE parts and – HAZARDOUS live parts, if protection is provided by – limited access		
6.4.3	BASIC INSULATION	(see Forms A.15 and A.16)	
	– meet CLEARANCE, CREEPAGE DISTANCE and solid insulation requirements of 6.7		
6.4.4	Impedance	(see Forms A.12 and A.15)	
	Impedance used as primary means of protection meets all the following requirements:		—
	a) limits current or voltage to level of 6.3.2	(see Form A.6)	
	b) RATED for maximum WORKING VOLTAGE and the amount of power it will dissipate		
	c) CLEARANCE, CREEPAGE DISTANCE between terminations of the impedance meet requirements of BASIC INSULATION of 6.7	(see Form A.15)	
6.5	Additional means of protection in case of SINGLE FAULT CONDITION		
6.5.1	General		
	ACCESSIBLE parts are prevented from becoming HAZARDOUS live by the primary means of protection and supplemented by one of:		—
	a) PROTECTIVE BONDING (see 6.5.2)		
	b) SUPPLEMENTARY INSULATION (see 6.5.3)		
	c) automatic disconnection of the supply (see 6.5.5)		
	d) current- or voltage-limiting device (see 6.5.6)		
	Alternatively one of the single means of protection is used:		—
	e) REINFORCED INSULATION (see 6.5.3)		
	f) PROTECTIVE IMPEDANCE (see 6.5.4)		
6.5.2	PROTECTIVE BONDING	(see Forms A.7, A.8, A.9, A.10 or A.11)	

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
6.5.2.1	General		
	ACCESSIBLE conductive parts, may become HAZARDOUS LIVE in SINGLE FAULT CONDITION:		—
	Bonded to the PROTECTIVE CONDUCTOR TERMINAL; or		
	Separated by conductive screen or barrier bonded to PROTECTIVE CONDUCTOR TERMINAL		
6.5.2.2	Integrity of PROTECTIVE BONDING		—
	A) PROTECTIVE BONDING consists of directly connected structural parts or discrete conductors or both; and withstands thermal and dynamic stresses		
	b) Soldered connections:		—
	Independently secured against loosening		
	Not used for other purposes		
	c) Screw connections are secured		
	D) PROTECTIVE BONDING not interrupted; or		
	except as removable part that carries MAINS SUPPLY input connection to the whole equipment		
	e) Any movable PROTECTIVE BONDING connection specifically designed, and meets 6.5.2.4		
	f) No external metal braid of cables used (not regarded as PROTECTIVE BONDING)		
	G) IF MAINS SUPPLY passes through:		—
	Means provided for passing protective conductor;		
	Impedance meets 6.5.2.4		
	H) Protective conductors bare or insulated, if insulated, green/yellow		
	Exceptions:		—
	1) earthing braids;		
	2) internal protective conductors etc.;		
	Green/yellow not used for other purposes		
	TERMINAL suitable for connection of a PROTECTIVE CONDUCTOR, and meets 6.5.2.3		
6.5.2.3	PROTECTIVE CONDUCTOR TERMINAL		—
	a) Contact surfaces are metal	Contact surfaces are metal	P
	b) Appliance inlet used	Certified appliance inlet used	P

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) For rewirable cords and PERMANENTLY CONNECTED EQUIPMENT, PROTECTIVE CONDUCTOR TERMINAL is close to MAINS supply TERMINALS	Not permanently connected equipment	N/A
	d) If no MAINS supply is required, any PROTECTIVE CONDUCTOR TERMINAL:		—
	Is near terminals of circuit for which protective earthing is necessary		N/A
	External if other terminals external		N/A
	e) Equivalent current-carrying capacity to MAINS supply TERMINALS	(see Form A.7)	
	f) If plug-in, makes first and breaks last		
	g) If also used for other bonding purposes, PROTECTIVE CONDUCTOR:		—
	Applied first;		
	Secured independently;		
	Unlikely to be removed by servicing		
	h) PROTECTIVE CONDUCTOR of measuring circuit:		—
	1) Current RATING equivalent to measuring circuit TERMINAL;		
	2) PROTECTIVE BONDING: not interrupted by any switch or interrupting device		
	i) FUNCTIONAL EARTH TERMINALS allow independent connection	No functional earth terminals	N/A
	j) If a binding screw used for PROTECTIVE CONDUCTOR TERMINAL:		—
	Suitable size for bond wire		
	Not smaller than M 4		
	At least 3 turns of screw engaged		
	Passes tightening torque test	(see Form A.8)	
	k) Contact pressure not capable being reduced by deformation of materials		
6.5.2.4	Impedance of PROTECTIVE BONDING of plug-connected equipment	(see Form A.9) Testing required	TBD
	Impedance between PROTECTIVE CONDUCTOR TERMINAL and each ACCESSIBLE part where PROTECTIVE BONDING is specified, is:		—
	– less than 0,1 Ohm; or		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– less than 0,2 Ohm if equipment is provided with non-detachable cord		
6.5.2.5	Impedance of PROTECTIVE BONDING of PERMANENTLY CONNECTED EQUIPMENT	(see Form A.10) Not permanently connected equipment	N/A
6.5.2.6	Transformer PROTECTIVE BONDING screen	(see Form A.11) Transformer part of certified power supply	N/A
	Transformer provided with screen for PROTECTIVE BONDING:		—
	screen bonding consists of directly connected structural parts or discrete conductors or both; and withstands thermal and dynamic stresses (see 6.5.2.2 a)		N/A
	screen bonding with soldered connection (see 6.5.2.2 b) is:		—
	–Independently secured against loosening		N/A
	–Not used for other purposes		N/A
6.5.3	SUPPLEMENTARY and REINFORCED INSULATION		
	Meet CLEARANCE, CREEPAGE DISTANCE and solid insulation requirements of 6.7		
6.5.4	PROTECTIVE IMPEDANCE	(see Form A.12)	
	Limits current or voltage to level of 6.3.1 in NORMAL and to level of 6.3.2 in SINGLE FAULT CONDITION		
	CLEARANCE, CREEPAGE DISTANCE between terminations of the impedance meet requirements of DOUBLE or REINFORCED INSULATION of 6.7	(see Form A.15)	
	The PROTECTIVE IMPEDANCE consists of one or more of the following:	(see TABLE 1.A and Form A.12)	—
	a) appropriate single component suitable for safety and reliability for protection, it is:		—
	1) RATED twice the maximum WORKING VOLTAGE		
	2) resistor RATED for twice the power dissipation for maximum WORKING VOLTAGE		
	b) combination of components		
	Single electronic device not used as PROTECTIVE IMPEDANCE		
6.5.5	Automatic disconnection of the supply		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	a) RATED to disconnect the load within time specified in Figure 2		
	b) RATED for the maximum load conditions of the equipment		
6.5.6	Current- or voltage-limiting devices	(see Form A.13) No such devices in equipment	N/A
	Device complies with all of:		—
	a) RATED to limit the current or voltage to the level of 6.3.2	(see Form A.6)	N/A
	b) RATED for the maximum WORKING VOLTAGE; and		N/A
	RATED for the maximum operational current if applicable		N/A
	c) CLEARANCE, CREEPAGE DISTANCE between terminations of the impedance meet requirements of SUPPLEMENTARY INSULATION of 6.7	(see Forms A.14 and A.15)	N/A
6.6	Connections to external circuits	No connection to external circuits	N/A
6.6.1	General		N/A
	Connections do not cause ACCESSIBLE parts of the following to become HAZARDOUS LIVE in NORMAL CONDITION or SINGLE FAULT CONDITION:		—
	– the external circuits		N/A
	– the equipment		N/A
	Protection achieved by separation of circuits; or		N/A
	short circuit of separation does not cause a HAZARD		N/A
	Instructions or markings for each terminal include:		—
	A) RATED conditions for TERMINAL		N/A
	B) Required RATING of external circuit insulation		N/A
6.6.2	TERMINALS for external circuits		N/A
	TERMINALS which receive a charge from an internal capacitor are not HAZARDOUS LIVE after 10 s of interrupting supply connection	(see Form A.5)	N/A
6.6.3	Circuits with terminals which are HAZARDOUS LIVE		N/A
	These circuits are:		—
	Not connected to ACCESSIBLE conductive parts; or		N/A
	Connected to ACCESSIBLE conductive parts, but are not		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	MAINS CIRCUITS and have one TERMINAL contact at earth potential		
	No ACCESSIBLE conductive parts are HAZARDOUS LIVE		N/A
6.6.4	Terminals for stranded conductors	No such conductors	N/A
	No RISK of accidental contact because:		—
	– Located or shielded		N/A
	– Self-evident or marked whether or not connected to ACCESSIBLE conductive parts		N/A
	Complies as applicable:		—
	a) Manufacturer's specified maximum length of removed insulation, or		N/A
	b) 8 mm length of insulation removed		N/A
6.7	Insulation requirements	(see Form A.14)	TBD
6.7.1	The nature of insulation		
6.7.1.1	General		
	Insulation between ACCESSIBLE parts or between separate circuits consist of CLEARANCES, CREEPAGE DISTANCES and solid insulation if provided as protection against a HAZARD		
6.7.1.2	CLEARANCES		
	Required CLEARANCES reflecting factors of 6.7.1.1	(see Forms A.14 and A.15)	
	Equipment rated for operating altitude greater than 2000 m correction factor of Table 3 of 61010-1 applied		
6.7.1.3	CREEPAGE DISTANCES		
	Required CREEPAGE DISTANCES reflecting factors of 6.7.1.1 a) to d)	(see Forms A.14 and A.15)	
	CTI material group reflected by requirements		
	CTI test performed		
6.7.1.4	Solid insulation		
	Required solid insulation reflecting factors of 6.7.1.1 a) to d)	(see Forms A.14 and A.15)	
6.7.1.5	Requirements for insulation according to type of circuit	(see Forms A.14 and A.15)	
	A) 6.7.2 MAINS circuits of OVERVOLTAGE CATEGORY II up to nominal supply voltage of 300 V		
	B) 6.7.3 secondary circuits separated from circuits defined in a) by transformer		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	C) K.1 MAINS circuits of OVERVOLTAGE CATEGORY III and IV or OVERVOLTAGE CATEGORY II over 300 V		
	D) K.2 secondary circuits separated from circuits defined in c) by transformer		
	E) K.3 circuits having one or more of:		—
	1) maximum TRANSIENT OVERVOLTAGE is limited to known level below the level of MAINS CIRCUIT		
	2) maximum TRANSIENT OVERVOLTAGE above the level of MAINS CIRCUIT		
	3) WORKING VOLTAGE is the sum of more than one circuit or a mixed voltage		
	4) WORKING VOLTAGE includes recurring peak voltage, may include non-sinusoidal or non-periodic waveform		
	5) WORKING VOLTAGE with a frequency above 30 kHz		
6.7.2	Insulation for MAINS CIRCUITS of OVERVOLTAGE CATEGORY II with a nominal supply voltage up to 300 V		
6.7.2.1	CLEARANCES and CREEPAGE DISTANCES	(see Forms A.14 and A.15)	—
	Values for MAINS CIRCUITS of Table 4 are met		
	Coatings to achieve reduction to POLLUTION DEGREE 1 comply with requirements of Annex H		
6.7.2.2	Solid insulation		
6.7.2.2.1	General		
	Withstands electrical and mechanical stresses in normal use and all RATED environmental conditions of 1.4		
	Equipment passed voltage tests of 6.8.3 with values of Table 5	(see Form A.18)	
	Complies as applicable:		—
	A) ENCLOSURE or PROTECTIVE BARRIER of Clause 8		
	b) moulded and potted parts requirements of 6.7.2.2.2		
	c) inner layers of printed wiring boards requirements of 6.7.2.2.3		
	D) thin-film insulation requirements of 6.7.2.2.4		
6.7.2.2.2	Moulded and potted parts		—
	Conductors between same two layers are separated by		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	at least 0,4 mm after moulding is completed		
6.7.2.2.3	Inner insulating layers of printed wiring boards		—
	Separated by at least 0,4 mm between same two layers		
	REINFORCED INSULATION has adequate electric strength; one of following methods used:		—
	a) thickness of insulation is at least 0,4 mm		
	b) insulation is assembled of minimum two separate layers, each RATED for test voltage of Table 5 for BASIC INSULATION		
	c) insulation is assembled of minimum two separate layers, where the combination is rated for test voltage of Table 5 for REINFORCED INSULATION		
6.7.2.2.4	Thin-film insulation		—
	Conductors between same two layers are separated by applicable CLEARANCES and CREEPAGE DISTANCE of 6.7.2.1		
	REINFORCED INSULATION have adequate electric strength; one of the following methods used:		—
	a) thickness through the insulation at least 0,4 mm		
	b) insulation is assembled of min. two separate layers, each RATED for test voltage of Table 5 for BASIC INSULATION	(see Form A.18)	
	c) insulation is assembled of min. three separate layers, where the combination of two layers passed voltage tests of 6.8.3 with values of Table 5 for REINFORCED INSULATION	(see Form A.18)	
6.7.3	Insulation for secondary circuits derived from MAINS CIRCUITS of OVERVOLTAGE CATEGORY II up to 300 V		
6.7.3.1	General		
	Secondary circuits where separation from MAINS CIRCUITS is achieved by a transformer providing:		—
	— REINFORCED INSULATION		
	— DOUBLE INSULATION		
	— screen connected to the PROTECTIVE CONDUCTOR TERMINAL		
6.7.3.2	CLEARANCES	(see Forms A.14 and A.15)	
	a) meet the values of Table 6 for BASIC INSULATION and SUPPLEMENTARY INSULATION; or		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	twice the values of Table 6 for REINFORCED INSULATION; or		
	B) pass the voltage tests of 6.8 with values of Table 6;	(see Form A.18)	
	with following adjustments:		—
	1) values for reinforced insulation are 1,6 times the values for basic insulation		
	2) if operating altitude is greater than 2000 m values of CLEARANCES multiplied with factor of Table 3		
	3) minimum CLEARANCE is 0,2 mm for POLLUTION DEGREE 2 and 0,8 mm for POLLUTION DEGREE 3		
6.7.3.3	CREEPAGE DISTANCES	(see Forms A.14 and A.15)	
	Based on WORKING VOLTAGE meets the values of Table 7 for BASIC and SUPPLEMENTARY INSULATION		
	Values for REINFORCED INSULATION are twice the values of BASIC INSULATION		
	Coatings to achieve reduction to POLLUTION DEGREE 1 comply with requirements of Annex H		
6.7.3.4	Solid insulation		
6.7.3.4.1	General		
	Withstands electrical and mechanical stresses in normal use and all RATED environmental conditions of 1.4		—
	a) Equipment passed voltage test of 6.8.3.1 for 5 s with VALUES of Table 6 for BASIC and SUPPLEMENTARY INSULATION	(see Form A.18)	
	values for REINFORCED INSULATION are 1,6 times the values of BASIC INSULATION		
	b) if WORKING VOLTAGE exceeds 300 V, equipment passed voltage test of 6.8.3.1 for 1 min with a test voltage of 1,5 times working voltage for BASIC or SUPPLEMENTARY INSULATION	(see Form A.18)	
	value for REINFORCED INSULATION are twice the WORKING VOLTAGE		
	Complies as applicable:		—
	1) ENCLOSURE or PROTECTIVE BARRIER of Clause 8		
	2) moulded and potted parts requirements of 6.7.3.4.2		
	3) inner layers of printed wiring boards		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	requirements of 6.7.3.4.3		
	4) thin-film insulation requirements of 6.7.3.4.4		
6.7.3.4.2	Moulded and potted parts		—
	Conductors between same two layers are separated by applicable distances of Table 8		
6.7.3.4.3	Inner insulation layers of printed wiring boards		—
	Separated by at least the applicable distances of Table 8 between same two layers		
	REINFORCED INSULATION have adequate electric strength; one of following methods used:		—
	a) thickness at least applicable distance of Table 8		
	b) insulation is assembled of minimum two separate layers, each RATED for test voltage of Table 6 for BASIC INSULATION	(see Form A.18)	
	c) insulation is assembled of min. two separate layers, where the combination is RATED for 1,6 times the test voltage of Table 6	(see Form A.18)	
6.7.3.4.4	Thin-film insulation		—
	Conductors between same two layers are separated by applicable CLEARANCES and CREEPAGE DISTANCE of 6.7.3.2 and 6.7.3.3		
	REINFORCED INSULATION have adequate electric strength; one of following methods used:		—
	a) thickness at least applicable distance of Table 8		
	b) insulation is assembled of min. two separate layers, each RATED for test voltage of Table 6 for BASIC INSULATION	(see Form A.18)	
	c) insulation is assembled of min. three separate layers, where the combination of two layers passed voltage tests with 1,6 time values of Table 6:	(see Form A.18)	—
	a.c. test of 6.8.3.1; or		
	d.c. test of 6.8.3.2 for circuits stressed only by d.c. voltages		
6.8	Procedure for voltage tests	(see Forms A.14 and A.18)	
6.9	Constructional requirements for protection against electric shock		
6.9.1	General		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	If a failure could cause a HAZARD:		—
	a) security of wiring connections		
	b) screws securing removable covers		
	c) accidental loosening		
	d) CLEARANCES and CREEPAGE DISTANCES not reduced below the values of basic insulation by loosening of parts or wires		
6.9.2	Insulating materials		
	Material not to be used for safety relevant insulation:		—
	a) easily damaged materials not used		
	b) non-impregnated hygroscopic materials not used		
6.9.3	Colour coding		
	Green-and-yellow insulation shall not be used except:		—
	a) protective earth conductors;		
	b) PROTECTIVE BONDING conductors;		
	c) potential equalization conductors;		
	d) functional earth conductors		
6.10	Connection to MAINS supply source and connections between parts of equipment		
6.10.1	MAINS supply cords		
	RATED for maximum equipment current (see 5.1.3 c)		
	Cable complies with IEC 60227 or IEC 60245		
	Heat-resistant if likely to contact hot parts		
	Temperature RATING (cord and inlet)..... :		—
	Green/yellow used only for connection to PROTECTIVE CONDUCTOR TERMINALS		P
	Detachable cords with IEC 60320 MAINS connectors:		—
	Conform to IEC 60799; or		P
	Have the current RATING of the MAINS connector		P
6.10.2	Fitting of non-detachable MAINS supply cords	Only detachable mains supply cords used	N/A
6.10.2.1	Cord entry		—
	a) inlet or bushing with a smoothly rounded opening; or		N/A
	b) insulated cord guard protruding >5 D (diameter)		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
6.10.2.2	Cord anchorage	All models use detachable power cords	N/A
	Protective earth conductor is the last to take the strain		N/A
	a) cord is not clamped by direct pressure from a screw		N/A
	b) knots are not used		N/A
	c) cannot push the cord into the equipment to cause a HAZARD		N/A
	d) no failure of cord insulation in anchorage with metal parts		N/A
	e) not to be loosened without a tool		N/A
	f) cord replacement does not cause a HAZARD and method of strain relief is clear		N/A
	Push-pull and or torque test	(see Form A.19)	N/A
6.10.3	Plugs and connectors		
	MAINS supply plugs, connectors etc., conform with relevant specifications		
	If equipment supplied at voltages below 6.3.2.a) or from a sole source:		—
	Plugs of supply cords do not fit MAINS sockets above rated SUPPLY voltage		
	MAINS type plugs used only for connection to MAINS supply		
	Plug pins which receive a charge from an internal capacitor	(see Form A.5)	
	Accessory MAINS socket outlets:		—
	a) marking if accepts a standard MAINS supply plug (see 5.1.3e)		
	b) input has a protective earth conductor if outlet has EARTH TERMINAL CONTACT		
6.11	Disconnection from supply source		
6.11.1	Disconnects all current-carrying conductors	Power switch provided as means of disconnecting equipment	P
6.11.2	Exceptions		N/A
6.11.3	Requirements according to type of equipment		N/A
6.11.3.1	PERMANENTLY CONNECTED EQUIPMENT and multi-phase equipment	Not permanently connected or multi-phase equipment	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Employs switch or circuit-breaker		N/A
	If switch or circuit-breaker is not part of the equipment, documentation requires:		—
	a) switch or circuit-breaker to be included in building installation		N/A
	b) suitable location easily reached		N/A
	c) marking as disconnecting for the equipment		N/A
6.11.3.2	Single-phase cord-connected equipment		
	Equipment is provided with one of the following:		—
	a) switch or circuit-breaker	Power switch provided	P
	b) appliance coupler (disconnectable without tool)		P
	c) separable plug (without locking device)		P
6.11.4	Disconnecting devices		P
6.11.4.1	General		
	Disconnecting device part of equipment		P
	Electrically close to the SUPPLY		P
	Power-consuming components not electrically located between the supply source and the disconnecting device		P
	Except electromagnetic interference suppression circuits permitted to be located on the supply side of the disconnecting device		N/A
6.11.4.2	Switches and circuit-breakers		P
	When used as disconnection device:		—
	Circuit breaker meets the relevant requirements IEC 60947-2 and is suitable for the application		N/A
	Switch meets the relevant requirements IEC 60947-3 and is suitable for the application		P
	Marked to indicate function.....:	Symbols 9 and 10 are on switch	P
	Not incorporated in MAINS cord	Not incorporated in mains cord	P
	Does not interrupt PROTECTIVE EARTH CONDUCTOR	Switch does not interrupt protective earth conductor	P
6.11.4.3	Appliance couplers and plugs		P
	Where an appliance coupler or separable plug is used as the disconnecting device (see 6.11.3.2):		—
	Readily identifiable and easily reached by the operator		P

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Single-phase portable equipment cord length not more than 3 m		P
	PROTECTIVE EARTH CONDUCTOR connected first and disconnected last		N/A

7	PROTECTION AGAINST MECHANICAL HAZARDS		P
7.1	General		P
	Equipment does not cause a mechanical HAZARD in NORMAL nor in SINGLE FAULT CONDITION		P
	Conformity is checked by 7.2 to 7.7		P
7.2	Sharp edges		P
	Easily-touched parts are smooth and rounded	All easily touched parts of all models are smooth and rounded	P
	Do not cause injury during NORMAL USE and		P
	Do not cause injury during SINGLE FAULT CONDITION		P
7.3	Moving parts	Front accessible moving part is operated via low power dc motor. Unlikely to cause any hazard	N/A
7.3.1	General		N/A
	HAZARDS from moving parts limited to a tolerable level with the conditions specified in 7.3.2 and 7.3.5		N/A
	RISK assessment in accordance with 7.3.3 carried out		N/A
7.3.2	Exceptions	Exception not used	N/A
	Access to HAZARDOUS moving parts permitted under following circumstances:		—
	a) obviously intended to operate on parts or materials external of the equipment		
	inadvertent touching of moving parts minimized by equipment design (e.g. guards or handles)		
	b) If OPERATOR access is unavoidable outside NORMAL USE following precautions have been taken:	No such	—
	1) access requires TOOL		
	2) statement about training in the instructions		
	3) warning markings on covers prohibiting access by untrained OPERATORS		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	or symbol 14 with full details in documentation		
7.3.3	RISK assessment for mechanical HAZARDS to body parts		
	RISK is reduced to a tolerable level by protective measures as specified in Table 12		
	Minimum protective measures:		—
	A. Low level measures		
	B. Moderate measures		
	C. Stringent measures		
7.3.4	Limitation of force and pressure	(see Form A.20)	
	Following levels are met in NORMAL and SINGLE FAULT CONDITION:		—
	Continuous contact pressure below 50 N / cm ² with force below 150 N		
	Temporary force below 250 N for an area at least of 3 cm ² for a maximum duration of 0,75 s		
7.3.5	Gap limitations between moving parts	(see Form A.20)	
7.3.5.1	Access normally allowed		—
	If levels of 7.3.4 exceeded and a body part may be inserted minimum gap as specified in Table 13 assured in NORMAL and in SINGLE FAULT CONDITION		
7.3.5.2	Access normally prevented		—
	Maximum gap as specified in Table 14 assured in NORMAL and in SINGLE FAULT CONDITION		
7.4	Stability		
	Equipment not secured to building structure is physical stable		
	Stability maintained after opening of drawers etc. by automatic means, or		
	warning marking requires the application of means		
	Compliance checked by following tests as applicable:	(see Form A.20A)	—
	a) 10° tilt test for other than handheld equipment	Testing required	TBD
	b) multi-directional force test for equipment exceeds height of 1 m and mass of 25 kg	Equipment height is less than 1m and weight is less than 25kg	N/A
	c) downward force test for floor-standing equipment	Not floor-standing equipment	N/A
	d) overload test with 4 times maximum load for castor or support foot that supports greatest load, or		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	e) castor or support foot that supports greatest load removed from equipment	No castor or support foot	N/A
7.5	Provisions for lifting and carrying		F
7.5.1	General		F
	Equipment more than 18 kg..... :	Equipment is 18kg	F
	Has means for lifting or carrying; or	No means for lifting or carrying	F
	Directions are given in documentation	No directions given in IFU pertaining to lifting or carrying	F
7.5.2	Handles and grips	No handles or grips	N/A
	Handles or grips withstand four times weight		N/A
7.5.3	Lifting devices and supporting parts	No such devices or parts on all models	N/A
	RATED for maximum load; or		N/A
	Tested with four times maximum static load		
7.6	Wall mounting	Not wall-mounted equipment	N/A
	Mounting brackets withstand four times weight	(see Form A.20B)	N/A
	One fastener removed and test repeated with two times weight	(see Form A.20B)	N/A
7.7	Expelled parts	Testing required to determine conformance	TBD
	Equipment contains or limits the energy		TBD
	Protection not removable without the aid of a tool		TBD

8	RESISTANCE TO MECHANICAL STRESSES		P
8.1	General		P
	Equipment does not cause a HAZARD when subjected to mechanical stresses in NORMAL USE	Testing required	TBD
	Normal protection level is 5 J	5J	P
	Levels below 5 J but not less than 1 J are acceptable if all of the following criteria are met:		—
	a) Lower level justified by RISK assessment of manufacturer		N/A
	b) Equipment installed in its intended application is not easily touched		N/A
	c) Only occasional access during NORMAL USE		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	d) IK code in accordance to IEC 62262 marked or symbol 14 used with full information in the documentation		N/A
	for non-metallic ENCLOSURES rated below 2 °C ambient temperature value chosen for minimum RATED temperature		N/A
	impact energies between IK values, the IK code marked for nearest lower value		N/A
	Conformity is checked by performing following tests:	(see Form A.16)	—
	1) Static test of 8.2.1	Testing required	TBD
	2) Impact test of 8.2.2 with 5 J except for HAND-HELD EQUIPMENT	Not hand-held equipment	N/A
	if specified impact energy is not 5 J alternate method of IEC 62262 used		
	3) Drop test of 8.3.1 or 8.3.2 except for FIXED EQUIPMENT and equipment with mass over 100 kg		
	Equipment RATED with an impact rating of IK 08 that obviously meets the criteria		
	After the tests inspection with following results:		—
	– HAZARDOUS LIVE parts above the limits of 6.3.2 not ACCESSIBLE		
	– insulation pass the voltage tests of 6.8	(see Form A.30)	
	i) No leaks of corrosive and harmful substances		
	ii) ENCLOSURE shows no cracks resulting in a HAZARD		
	iii) CLEARANCES not less than their permitted values		
	iv) Insulation of internal wiring remains undamaged		
	v) PROTECTIVE BARRIERS not damaged or loosened		
	vi) No moving parts exposed, except permitted by 7.3		
	vii) No damage which could cause spread of fire		
8.2	ENCLOSURE rigidity test		
8.2.1	Static test	(see Form A.21A)	TBD
	– 30 N with 12 mm rod applied to each part of ENCLOSURE	Testing required	TBD
	– in case of doubt test conducted at maximum RATED ambient temperature		
8.2.2	Impact test	(see Form A.21A)	TBD

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Impact applied to any part of ENCLOSURE causing a HAZARD if damaged	Testing required	TBD
	Impact energy level and corresponding IK code.....:		—
	Non-metallic ENCLOSURES cooled to minimum RATED ambient temperature if below 2 °C		
8.3	Drop test	(see Form A.21B)	P
8.3.1	Other than HAND-HELD and DIRECT-PLUG-IN EQUIPMENT	Testing required	TBD
	Tests conducted with a drop height or angle of..... :		—
8.3.2	HAND-HELD and DIRECT-PLUG-IN EQUIPMENT	Not hand-held equipment	N/A
	Non-metallic ENCLOSURES cooled to minimum RATED ambient temperature if below 2 °C		N/A
	Drop test conducted with an height of 1 m		N/A

9	PROTECTION AGAINST THE SPREAD OF FIRE		
9.1	General		
	No spread of fire in NORMAL and SINGLE FAULT CONDITION	Testing required	TBD
	MAINS supplied equipment meets requirements of 9.6 additionally		
	Conformity is checked by minimum one or a combination of the following (see Figure 11):	(see Form A.22)	—
	a) SINGLE FAULT test of 4.4; or	(see Form A.1) Testing required	TBD
	b) Application of 9.2 (eliminating or reducing the sources of ignition); or		TBD
	c) Application of 9.3 (containment of fire within the equipment)		TBD
9.2	Eliminating or reducing the sources of ignition within the equipment		
	a) 1) Limited-energy circuit (see 9.4); or		
	2) BASIC INSULATION provided for parts of different potential; or	(see Forms A.14 and A.18)	
	Bridging the insulation does not cause ignition	(see Form A.1)	
	b) Surface temperature of liquids and parts (see 9.5)		
	c) No ignition in circuits designed to produce heat	(see Form A.1) Testing required	TBD

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.3	Containment of the fire within the equipment, should it occur		
9.3.1	General		
	Spread of fire outside equipment reduced to a tolerable level if:		—
	a) Energizing of the equipment is controlled by an OPERATOR held switch		
	b) ENCLOSURE is conform with constructional requirements of 9.3.2; and		
	Requirements of 9.5 are met		
9.3.2	Constructional requirements		
	a) Connectors and insulating material have flammability classification V-2 or better	(see TABLE 1.A or Form A.23) Printed wiring board is rated at V-0	P
	b) Insulated wires and cables are flame retardant (VW-1 or equivalent)	(see TABLE 1.A or Form A.23)	P
	c) ENCLOSURE meets following requirements:	(see Form A.22)	—
	1) Bottom and sides in arc of 5 ° (see Figure 13) to non-limited circuits (9.4) meets:		—
	i) no openings; or	No such openings	P
	ii) perforated as specified in Table 16; or	Not perforated	N/A
	iii) metal screen with a mesh; or	No such construction	N/A
	iv) baffles as specified in Figure 12	No such openings	N/A
	2) Material of ENCLOSURE and any baffle or flame barrier is made of:		—
	Metal (except magnesium); or	Metal enclosure	P
	Non-metallic materials have flammability classification V-1 or better	(see TABLE 1.A or Form A.22)	N/A
	3) ENCLOSURE and any baffle or flame barrier have adequate rigidity		P
9.4	Limited-energy circuit	(see Form A.24) No limited-energy circuit	N/A
	a) Potential not more than 30 r.m.s. and 42,4 V peak, or 60 V d.c.	Secondary voltage is at 24Vdc	N/A
	b) Current limited by one of following means:		—
	1) Inherently or by impedance (see Table 17); or		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	2) Overcurrent protective device (see Table 18); or	Fuse implemented in equipment	P
	3) A regulating network limits also in SINGLE FAULT CONDITION (see Table 17)		N/A
	c) Is separated by at least BASIC INSULATION		N/A
	Fuse or a nonadjustable electromechanical device is used		N/A
9.5	Requirements for equipment containing or using flammable liquids		N/A
	Flammable liquids contained in or specified for use with equipment do not cause spread of fire	(see Form A.25) No flammable liquids contained in or specified for use with equipment	N/A
	RISK is reduced to a tolerable level:		—
	a) The temperature of surface or parts in contact with flammable liquids is 25 °C below fire point		N/A
	b) The quantity of liquid is limited		N/A
	c) Flames are contained within the equipment		N/A
	Detailed instructions for RISK-reduction provided		N/A
9.6	Overcurrent protection		P
9.6.1	General	Equipment provided with fuse	P
	MAINS supplied equipment protected		
	BASIC INSULATION between MAINS parts of opposite polarity provided	(see Forms A.14 and A.15)	
	Overcurrent protection devices not fitted in the protective conductor	No such construction	P
	Fuses or single-pole circuit-breakers not fitted in neutral (multi-phase equipment)	Not multi-phase equipment	N/A
9.6.2	PERMANENTLY CONNECTED EQUIPMENT	Not permanently connected equipment	N/A
	Overcurrent protection device:		—
	Fitted within the equipment; or		N/A
	Specified in manufacturer's instructions		N/A
9.6.3	Other equipment		P
	Protection within the equipment		P
10	EQUIPMENT TEMPERATURE LIMITS AND RESISTANCE TO HEAT		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
10.1	Surface temperature limits for protection against burns		
	Easily touched surfaces within the limits in NORMAL and in SINGLE FAULT CONDITION:	(see Form A.26A)	—
	– at an specified ambient temperature of 40 °C		
	– for equipment rated above 40 °C ambient temperature limits not exceeded raised by the difference to 40 °C		
	Heated surfaces necessary for functional reasons exceeding specified values:		—
	– Are recognizable as such by appearance or function; or		
	– Are marked with symbol 13		
	– Guards are not removable without tool		
10.2	Temperatures of windings	Transformer is part of certified power supply	N/A
	Limits not exceeded in:	(see Form A.26B)	—
	NORMAL CONDITION		N/A
	SINGLE FAULT CONDITION		N/A
10.3	Other temperature measurements		
	Following measurements conducted if applicable:	(see Form A.26A)	—
	a) Value of 60 °C of field-wiring terminal box not exceeded		
	b) Surface of flammable liquids and parts in contact with this liquids	No flammable liquids	N/A
	c) Surface of non-metallic ENCLOSURES		
	d) Parts made of insulating material supporting parts connected to MAINS supply		
	e) Terminals carrying a current more than 0,5 A		
10.4	Conduct of temperature tests	Testing required	TBD
10.4.1	General		
	Tests conducted under reference test conditions and manufacturer's instructions	(see Form A.26A)	
	Tests alternatively conducted at the least favourable ambient temperature within the RATED ambient temperature..... :		—
10.4.2	Temperature measurement of heating equipment	Not a heating equipment	N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Tests conducted in test corner	(see Form A.26A)	N/A
10.4.3	Equipment intended for installation in a cabinet or wall	Not intended for such installation	N/A
	Equipment built in as specified in installation instructions	(see Form A.26A)	N/A
10.5	Resistance to heat		
10.5.1	Integrity of CLEARANCE and CREEPAGE DISTANCES	(see Form A.16)	
10.5.2	Non-metallic ENCLOSURES	(see Form A.27) Testing required	TBD
	Within 10 min after treatment:		—
	Equipment subjected to suitable stresses of 8.2 and 8.3 complying with criteria of 8.1		
10.5.3	Insulating material		
	a) Parts supporting parts connected to MAINS supply		
	b) TERMINALS carrying a current more than 0,5 A		
	Examination of material data; or		
	in case of doubt:		
	1) Ball pressure test; or	(see Form A.28)	
	2) Vicat softening test of ISO 306	(see Form A.29)	

11	PROTECTION AGAINST HAZARDS FROM FLUIDS AND SOLID FOREIGN OBJECTS		
11.1	General		
	Protection to OPERATORS and surrounding area provided by EQUIPMENT		
	All fluids specified by manufacturer considered		
11.2	Cleaning	(see Form A.30) Testing required	TBD
11.3	Spillage	(see Form A.30) Testing required	TBD
11.4	Overflow	(see Form A.30)	N/A
11.5	Battery electrolyte		N/A
	Battery electrolyte leakage presents no HAZARD		N/A
11.6	Equipment RATED with a degree of ingress protection (IP code)	(see Form A.30)	

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
11.6.1	General		
	Equipment marked with IP code..... :		—
	Conditions specified in the documentation		
11.6.2	Conditions for testing		
	Equipment in clean and new condition, all parts in place and mounted as specified by manufacturer		
	Complete equipment tested, or		
	representative parts tested		
	HAND-HELD EQUIPMENT and PORTABLE EQUIPMENT placed in least favourable position of NORMAL use		
	Other equipment positioned or installed as specified		
	TERMINALS provided with protective cap or cover, are installed as specified by manufacturer		
	The equipment is operating (energized) during the treatment except:		—
	a) If manufacturer specifies degrees of protection for non-operating (de-energized) equipment, or		
	b) Equipment is operating or non-operating during the treatment with does not affect the test results		
11.6.3	Protection against solid foreign objects (including dust)		
	Applicable test of IEC 60529 for protection against solid foreign objects conducted		
	Additionally inspection of equipment resulted:		—
	a) No deposit on insulation parts that could lead to a HAZARD		
	b) No created accumulations that have the potential to cause spread of fire		
11.6.4	Protection against water		
	Applicable test of IEC 60529 for protection against water conducted		
	If any water has entered, safety is not impaired, inspection of equipment resulted:		—
	a) No deposit on insulation parts that could lead to a HAZARD		
	b) Water has not reached hazardous live parts or windings which are not designed to operate when wet		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) No accumulations near the end of cable nor enter the cable where it could cause a HAZARD		
	d) No accumulations where it could lead to a HAZARD taking in consideration movement of the equipment		
11.7	Fluid pressure and leakage		
11.7.1	Maximum pressure..... :	(see Form A.31)	—
	Maximum pressure of any part does not exceed P_{RATED}		
11.7.2	Leakage and rupture at high pressure		
	Fluid-containing parts checked by inspection or if a HAZARD could arise subjected to hydraulic test, if:	(see Form A.31)	—
	a) product of pressure and volume > 200 kPa·l; and		
	b) pressure > 50 kPa		
	Safety evidence established by calculation in acc. to national authorities (e.g. Pressure Equipment Directive 2014/68/EU)		
	Parts of refrigerating systems meets pressure-related requirements of EN 378-2 or IEC 60335-2-89 as applicable		
11.7.3	Leakage from low-pressure parts	(see Form A.32)	
11.7.4	Overpressure safety device		
	Does not operate in NORMAL USE		
	a) Connected as close as possible to parts intended to be protected		
	b) Easy access for inspection, maintenance and repair		
	c) Adjustment only with TOOL		
	d) No discharge towards person		
	e) No HAZARD from deposit of discharged material		
	f) Adequate discharge capacity		
	No shut-off valve between overpressure safety device and protected parts		
12	PROTECTION AGAINST RADIATION, INCLUDING LASER SOURCES, AND AGAINST SONIC AND ULTRASONIC PRESSURE		N/A
12.1	General		
	Equipment provides protection		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
12.2	Equipment producing ionizing radiation		N/A
12.2.1	Ionizing radiation	(see Form A.33)	N/A
12.2.1.1	General		N/A
	Equipment meets the following requirements:		—
	a) if intended to emit radiation meets requirements of 12.2.1.2; or		N/A
	tested, classified and marked in accordance to IEC 62598		N/A
	b) if only emits stray radiation meets requirements of 12.2.1.3		N/A
12.2.1.2	Equipment intended to emit radiation		—
	Effective dose rate of radiation measured..... :		—
	If dose rate exceeds 5 µSv/h marked with the following:		—
	a) symbol 17 (ISO 361)		
	b) abbreviations of the radionuclides..... :		—
	c) with maximum dose at 1 m; or..... :		—
	with dose rate value between 1 µSv/h and 5 µSv/h in m..... :		—
12.2.1.3	Equipment not intended to emit radiation	(see Form A.34)	—
	Limit for unintended stray radiation of 1 µSv/h at any easily reached point kept		N/A
12.2.2	Accelerated electrons		N/A
	Compartments opened only by the use of a TOOL		N/A
12.3	Optical radiation	No optical radiation	N/A
	No unintentional HAZARDOUS escape of optical radiation as ultraviolet, visible or infrared radiation, including light emitting diodes:		—
	– Checked by inspection; and		N/A
	– Radiation sources assessed in acc. to the requirements of IEC 62471, except for sources considered to be safe (Table 22) or conditionally safe (Table 23).		N/A
	– Lamp and lamp systems assessed to Risk Groups 1, 2, or 3 of IEC 62471 are labelled in acc. to IEC 62471-2		N/A
	– If labelling impractical, lamp or lamp systems marked with symbol 14		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Protective measures, restrictions on use, and operating instructions that may be necessary are provided, including the applicable conditions of use of Table 23.		N/A
12.4	Microwave radiation	No microwave radiation	N/A
	Power density does not exceed 10 W/m ² :		N/A
12.5	Sonic and ultrasonic pressure	No sonic or ultrasonic pressure	N/A
12.5.1	Sound level	(see Form A.35) No obvious high energy sound from equipment.	N/A
	No HAZARDOUS sound emission		N/A
	Maximum sound pressure level measured and calculated for maximum sound power level as specified in ISO 3746 or ISO 9614-1		N/A
	Instruction describes measures for protection	Equipment does not require user protection from sound	N/A
12.5.2	Ultrasonic pressure	(see Form A.36) No such ultrasound emission from equipment	N/A
	Equipment not intended to emit ultrasound does not exceed limit of 110 dB between 20 kHz and 100 kHz		N/A
	Equipment intended to emit ultrasound:		N/A
	Outside useful beam does not exceed limit of 110 dB between 20 kHz and 100 kHz		N/A
	If inside useful beam above values exceeded:		—
	Marked with Symbol 14 of Table 1		N/A
	and following information in the documentation:		—
	a) dimensions of useful beam		N/A
	b) area where ultrasonic pressure exceed 110 dB		N/A
	c) maximum sound pressure inside beam area		N/A
12.6	Laser sources	No laser sources employed	N/A
	Equipment meets requirements of IEC 60825-1		N/A
13	PROTECTION AGAINST LIBERATED GASES AND SUBSTANCES, EXPLOSION AND IMPLOSION		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
13.1	Poisonous and injurious gases and substances	No hazardous substances	N/A
	No hazardous substances liberated in NORMAL CONDITION and in SINGLE FAULT CONDITION		N/A
	If potentially-hazardous substances are liberated:		—
	Operator is not directly exposed to a quantity of the substance that could cause harm		N/A
	Requirements to discharge of hazardous substances during NORMAL operation in accordance to manufacturer's instructions not considered as liberation		N/A
	Attached data/test reports demonstrate conformity		N/A
13.2	Explosion and implosion		
13.2.1	Components		
	Components liable to explode:		—
	Pressure release device provided; or		
	Apparatus incorporates operator protection (see also 7.7)		
	Pressure release device:		—
	Discharge without danger		
	Cannot be obstructed		
13.2.2	Batteries and battery charging	(see Form A.37) No battery	N/A
	If explosion or fire HAZARD could occur:	No battery	—
	Protection incorporated in the equipment; or		N/A
	Instructions specify batteries with built-in protection		N/A
	In case of wrong type of battery used:		—
	No HAZARD; or		N/A
	Warning by marking and within instructions		N/A
	Equipment with means to charge rechargeable batteries:		—
	Warning against the charging of non-rechargeable batteries; and		N/A
	Type of rechargeable battery indicated; or		N/A
	Symbol 14 used		N/A
	Battery compartment design		N/A
	Single component failure		N/A
	Polarity reversal test		N/A

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
13.2.3	Implosion of cathode ray tubes	No cathode ray tubes	N/A
	If maximum face dimensions > 160 mm..... :		—
	Intrinsically protected and correctly mounted; or		N/A
	ENCLOSURE provides protection:		N/A
	If non-intrinsically protected:		—
	Screen not removable without TOOL		N/A
	If glass screen, not in contact with surface of tube		N/A

14	COMPONENTS AND SUBASSEMBLIES		
14.1	General		
	Where safety is involved, components and subassemblies meet relevant requirements	(see TABLE 1.A)	
14.2	Motors	Servo motor to be tested	TBD
14.2.1	Motor temperatures		TBD
	Does not present a HAZARD when stopped or prevented from starting; or	(see Forms A.1 and A.26B)	TBD
	Protected by over-temperature or thermal protection device conform with 14.3		TBD
14.2.2	Series excitation motors	No such motors	N/A
	Connected direct to device, if overspeeding causes a HAZARD		N/A
14.3	Overtemperature protection devices	No such devices in equipment	N/A
	Devices operating in a SINGLE FAULT CONDITION	(see Form A.38)	N/A
	a) Reliable function is ensured		N/A
	B) RATED to interrupt maximum current and voltage		N/A
	c) Does not operate in NORMAL USE		N/A
	If self-resetting device used to prevent a HAZARD, protected part requires intervention before restarting		N/A
14.4	Fuse holders	No accessible fuse holders	N/A
	No access to HAZARDOUS LIVE parts		N/A
14.5	MAINS voltage selecting devices	No such devices in equipment	N/A
	Accidental change not possible		N/A
14.6	MAINS transformers tested outside equipment	(see Forms A.39 and A.40)	
14.7	Printed wiring boards		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Data shows conformity with V-1 of IEC 60695-11-10 or better; or		
	Test shows conformity with V-1 of IEC 60695-11-10 or better	(see Form A.23)	
	Not applicable for printed wiring boards with limited-energy circuits (9.4)		
14.8	Circuits used to limit TRANSIENT OVERVOLTAGES	No such devices in equipment	N/A
	Test conducted between each pair of MAINS SUPPLY TERMINALS	(see Form A.41)	N/A
	No ignition or overheating of other materials :		—
	– no ignition		N/A
	– no heat to other parts above the self-ignition points		N/A
	Safely suppressing and properly functional after applied tests		N/A

15	PROTECTION BY INTERLOCKS		N/A
15.1	General		N/A
	Interlocks are designed to remove a HAZARD before OPERATOR exposed	No such interlocks relied for safety	N/A
15.2	Prevention of reactivation		N/A
15.3	Reliability		N/A
	Single fault unlikely to occur; or		N/A
	Cannot cause a HAZARD		N/A

16	HAZARDS RESULTING FROM APPLICATION		
16.1	REASONABLY FORESEEABLE MISUSE		
	No HAZARDS arising from settings not intended and not described in the instructions		
	Other cases of REASONABLY FORESEEABLE MISUSE addressed by RISK assessment		
16.2	Ergonomic aspects		
	Factors giving rise to a HAZARD the RISK assessment is reflecting those aspects:		—
	a) limitation of body dimensions		
	b) displays and indicators		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) accessibility and conventions of controls		
	d) arrangement of TERMINALS		

17	RISK ASSESSMENT		
	RISK assessment conducted, if HAZARD might arise and not covered by Clauses 6 to 16		
	TOLERABLE RISK achieved by iterative documented process covering the following:		—
	a) RISK analysis		
	Identifies HAZARDS and estimates RISK		
	b) RISK evaluation		
	Plan to judge acceptability of resulting RISK level based on the estimated severity and likelihood of a RISK		
	c) RISK reduction		
	Initial RISK reduced by counter measures;		
	Repeated RISK evaluation without new RISKS introduced		
	RISKS remaining after RISK assessment addressed in instructions to RESPONSIBLE BODY:		—
	Information contained how to mitigate these RISKS		
	Following principles in methods of RISK reduction applied by manufacturer in given order:		—
	1) RISKS eliminated or reduced as far as possible		
	2) Protective measures taken for RISKS that cannot be eliminated		
	3) User information about residual RISK due to any defect of the protective measures		
	Indication of particular training is required		
	Specification of the need for personal protective equipment		
	Conformity checked by evaluation of the RISK assessment documentation		

ANNEX F	ROUTINE TESTS		
	Manufacturer 's declaration		

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict

ANNEX H	QUALIFICATION OF CONFORMAL COATINGS FOR PROTECTION AGAINST POLLUTION		
H.1	General		
	Conformal coatings meet the requirements of Clause H.2 and H.3.		
H.2	Technical properties		
	Technical properties of conformal coatings are suitable for the intended application. In particular:		—
	a) Manufacturer indicate that it is a coating for PWBs;		
	b) RATED operating temperature include the temperature range of the indicated application;		
	c) CTI, insulation resistance and dielectric strength are suitable for the intended application;		
	d) Coating have adequate UV resistance, if it is exposed to sunlight;		
	e) Flammability RATING of the coating is at least the required flammability RATING of the applied PWB.		
H.3	Qualification of coatings	(see Form A.42)	
	Coating complies with the conformity requirements.		

ANNEX K	INSULATION REQUIREMENTS NOT COVERED BY CLAUSE 6.7	(see Forms A.15 and A.18)	

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
5	MARKING AND DOCUMENTATION		
5.1.5.101	Gas and liquid connections		F
	If necessary for safety, the equipment is clearly marked near to the connector on the equipment with		
	a) a means of identifying the gas or liquid to be used	None provided on the equipment	F
	Where no internationally recognized symbol (including chemical formulae) exists, the equipment is marked with symbol 14 of Table 1;		
	b) the maximum permitted pressure	None provided on the equipment	F
	Pressure (Pa).....:		
	or alternatively symbol 14 of Table 1;		
	c) flow direction of the gas and liquid, if applicable		
5.3	Durability of markings		
	Markings required by 5.1.2 to 5.2 are removable only with a TOOL or by appreciable force and remain clear and legible under conditions of NORMAL USE		
	These markings resist the effects of temperature and rubbing, and of solvent and reagents likely to be encountered in NORMAL USE, including cleaning and decontaminating agents specified by the manufacturer		
5.4.101	Removal of equipment from use for repair or disposal		
	Instructions are provided to the RESPONSIBLE BODY for eliminating or reducing HAZARDS involved in removal from use, transportation or disposal		
	Alternatively, appropriate contact information is provided in the instructions		
7	PROTECTION AGAINST MECHANICAL HAZARDS		
7.3.2	Exceptions		
	b) If OPERATOR access is unavoidable outside NORMAL USE following precautions have been taken:		—
	3) warning markings on covers prohibiting access by untrained OPERATORS		
	Markings are placed within the area requiring maintenance where they can alert the OPERATOR to the hazard		
	or symbol 14 with full details in documentation		
	4) OPERATOR maintenance instructions specify safe maintenance procedures		

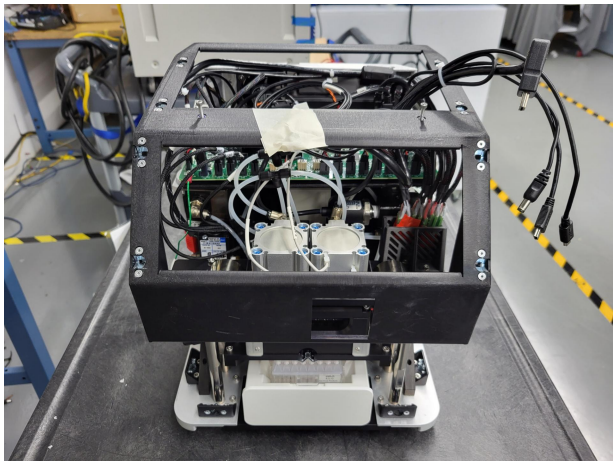
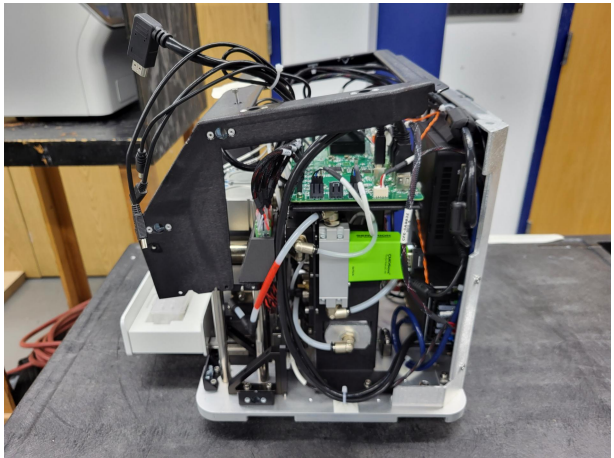
IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict
8	RESISTANS TO MECHANICAL STRESSES		
8.1	General		
	3) Drop test, as appropriate, of 8.3 except for FIXED EQUIPMENT, equipment with mass over 100 kg, or equipment whose size and weight make unintentional movement unlikely and which is not moved in NORMAL USE		
13	PROTECTION AGAINST LIBERATED GASES AND SUBSTANCES, EXPLOSION AND IMPLOSION		
13.101	Biohazardous substances		
	Equipment that can be potentially biohazardous due to the use of biohazardous substances are prominently marked with symbol 101 of Table 1		
	Alternatively, the appropriate international symbol, or (if none is available) symbol 14 of Table 1		
	A biohazard symbol is located near the sampling area and visible in NORMAL USE		
	Biohazard symbols are located near biohazardous areas accessed during OPERATOR maintenance and visible only during this maintenance		
	Any part of the equipment that contains biohazardous waste material which can be removed from the equipment during NORMAL USE or a biohazardous drain connection is marked with an appropriate biohazard symbol		
15	PROTECTION BY INTERLOCKS		
	As an alternative method, for interlock systems containing electric/electronic or programmable components (E/E/P components) the reliability and design requirements optionally determined applying e.g. IEC 62061 (SIL) or ISO 13849 (PL) (all parts) or other solutions providing equivalent functional safety		

IEC 61010-1

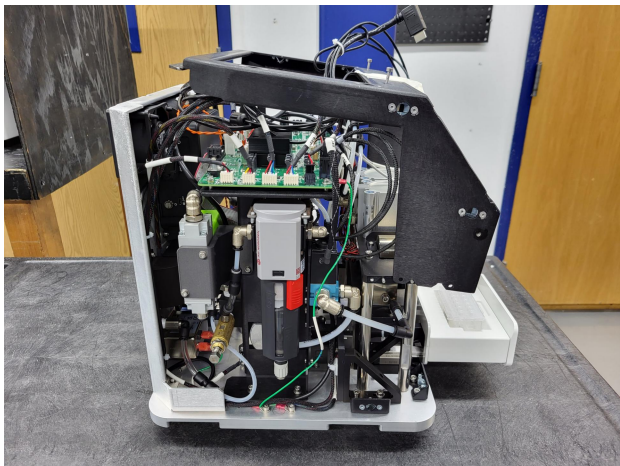
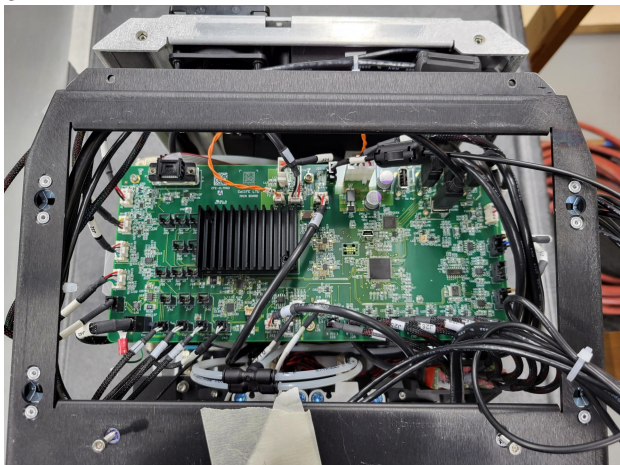
Clause	Requirement + Test	Result - Remark	Verdict
--------	--------------------	-----------------	---------

PHOTO OF EQUIPMENT	DESCRIPTION
1. 	Front view of the CellFe Infinity MTx
2. 	Rear view of the CellFe Infinity MTx
3. 	Left view of the CellFe Infinity MTx

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict

PHOTO OF EQUIPMENT		DESCRIPTION
4.		Right view of the CellFe Infinity MTx
5.		Top internal view of the CellFe Infinity MTx
6.		Right side internal view of the CellFe Infinity MTx

IEC 61010-1			
Clause	Requirement + Test	Result - Remark	Verdict

PHOTO OF EQUIPMENT		DESCRIPTION
7.		Left side internal view of the CellFe Infinity MTx
8.		Internal view of the PCB of the CellFe Infinity MTx
9.		

[illegible]

