
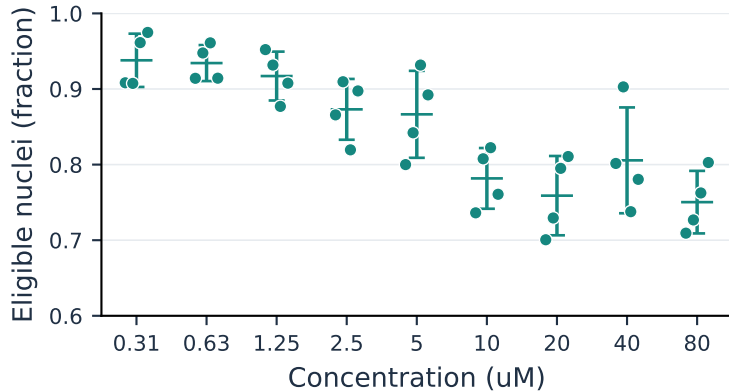




Task-only analysis recovers a dose response

BBBC013 · final self-repaired blind method · 96 paired DNA/GFP wells

A LY294002

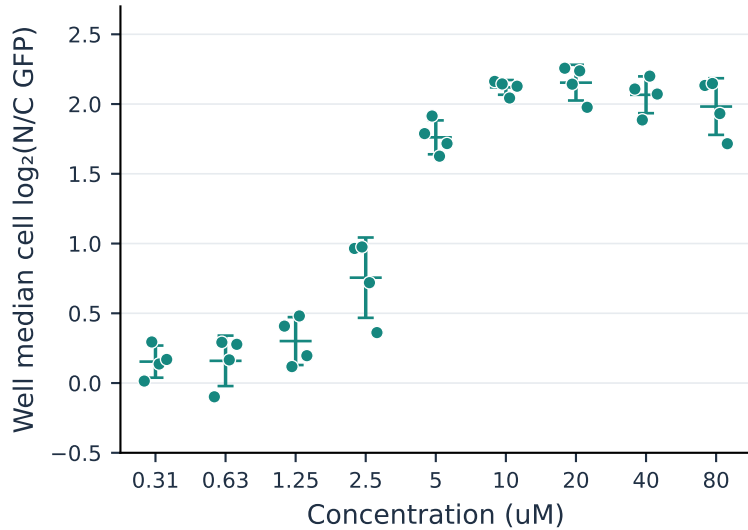

B Wortmannin

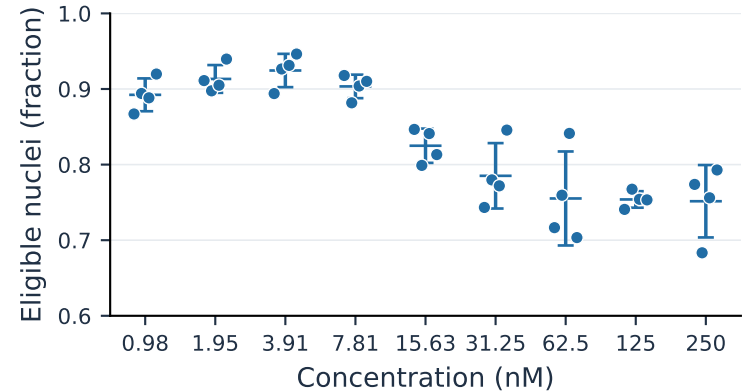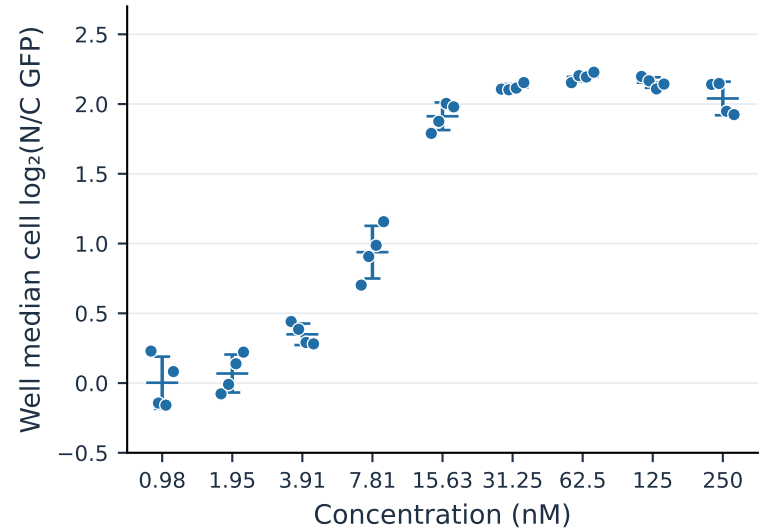

Dots: four wells per dose. Horizontal marks and whiskers: mean $\pm$ between-well SD.

Dose positions are equally spaced; dots offset for visibility. Lower panels use the same wells.

Response is conditional on eligible compartments; not calibrated potency or mask accuracy.