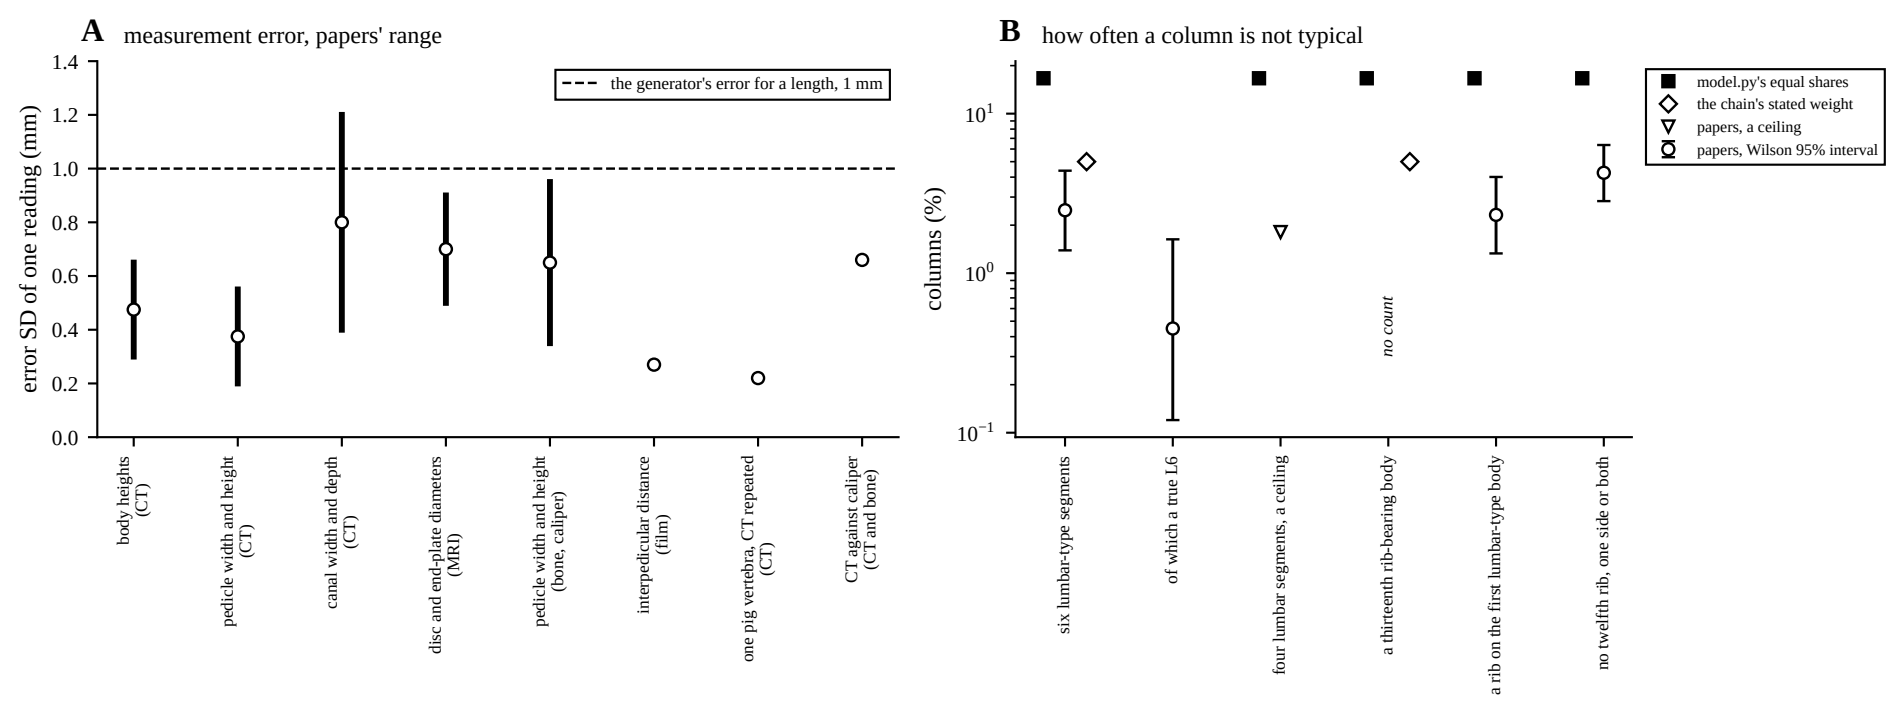
A
measurement error, papers' range
error SD of one reading (mm)
1.4
1.2
1.0
0.8
0.6
0.4
0.2
0.0
the generator's error for a length, 1 mm
body heights (CT)
pedicle width and height (CT)
canal width and depth (CT)
disc and end-plate diameters (MRI)
pedicle width and height (bone, caliper)
interpedicular distance (film)
one pig vertebra, CT repeated (CT)
CT against caliper (CT and bone)
B
how often a column is not typical
columns (%)
10^1
10^0
10^{-1}
model.py's equal shares
the chain's stated weight
papers, a ceiling
papers, Wilson 95% interval
no count
six lumbar-type segments
of which a true L6
four lumbar segments, a ceiling
a thirteenth rib-bearing body
a rib on the first lumbar-type body
no twelfth rib, one side or both