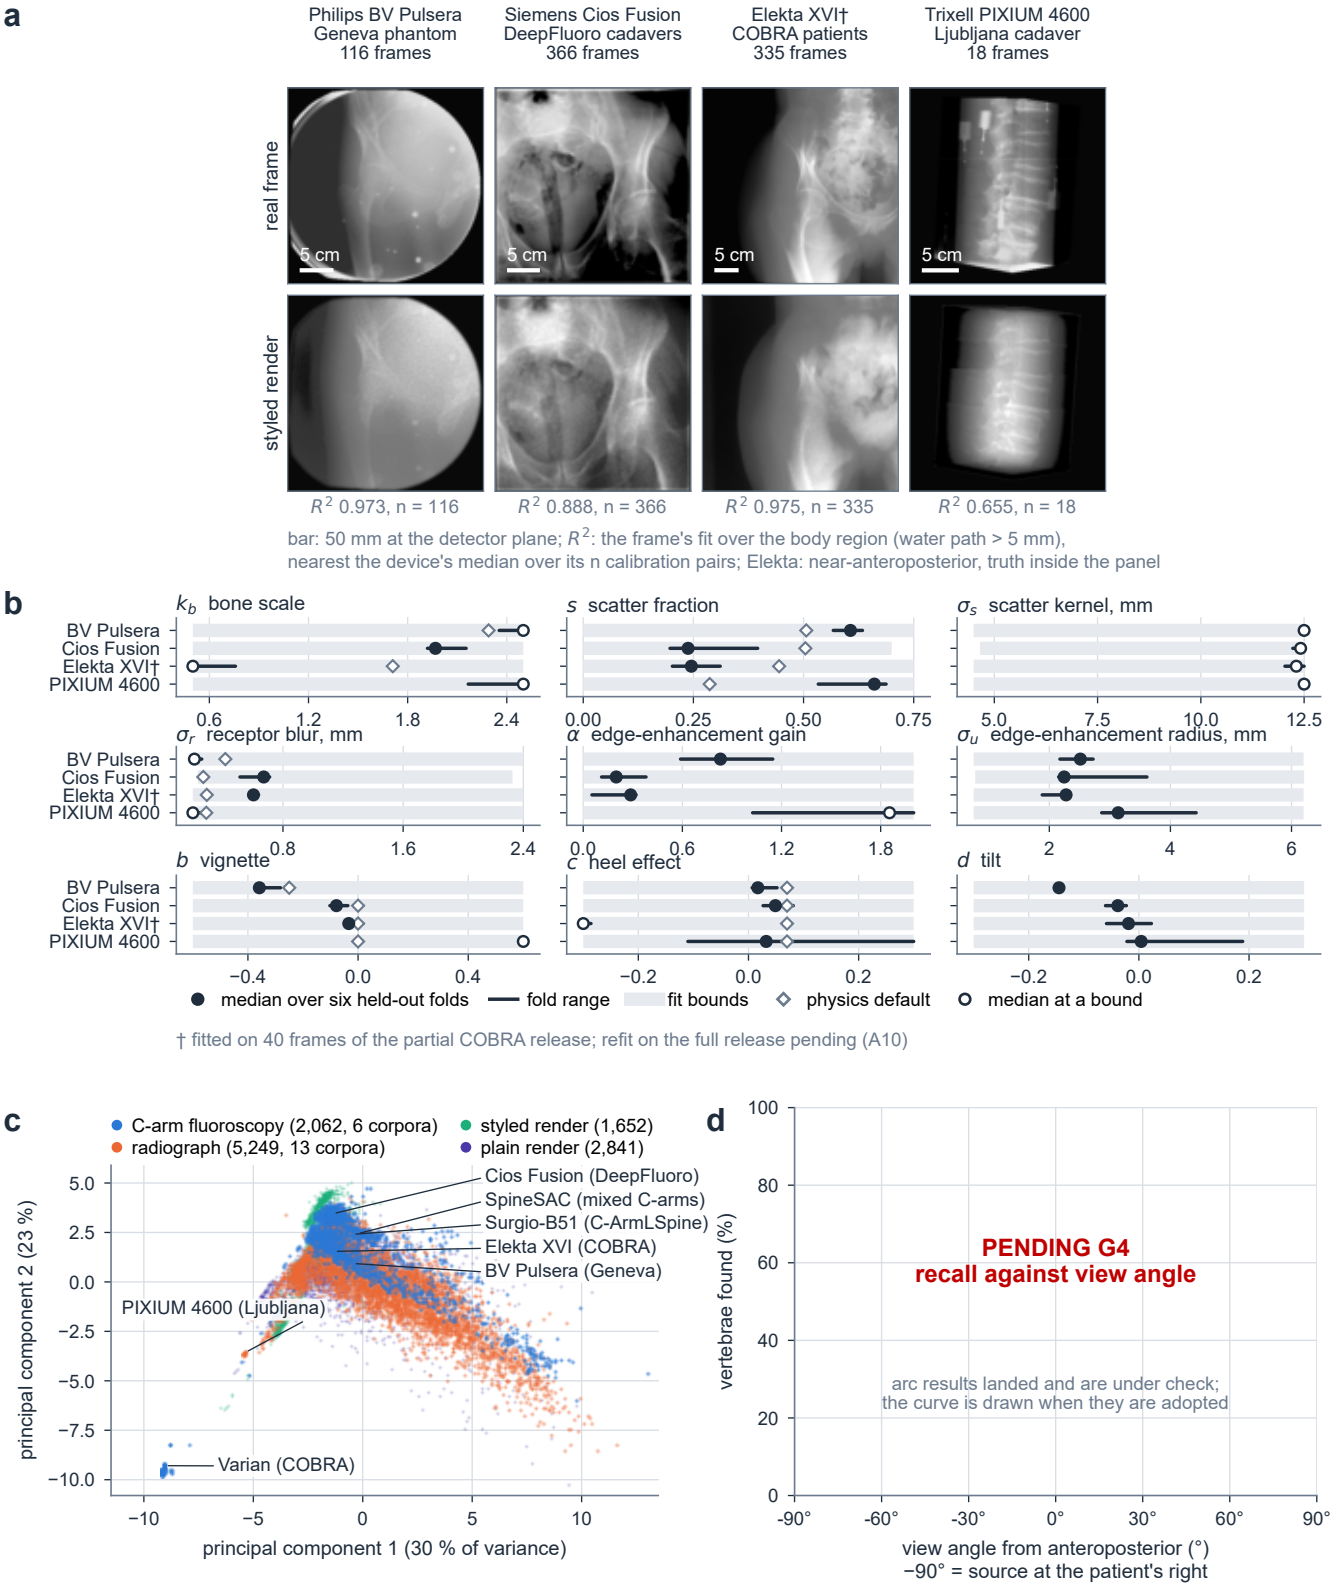

a
Philips BV Pulsera
Geneva phantom
116 frames
Siemens Cios Fusion
DeepFluoro cadavers
366 frames
Elekta XVI†
COBRA patients
335 frames
Trixell PIXIUM 4600
Ljubljana cadaver
18 frames
real frame
styled render
5 cm
R² 0.973, n = 116
R² 0.888, n = 366
R² 0.975, n = 335
R² 0.655, n = 18
bar: 50 mm at the detector plane; R²: the frame's fit over the body region (water path > 5 mm),
nearest the device's median over its n calibration pairs; Elekta: near-anteroposterior, truth inside the panel
b
k_b bone scale
s scatter fraction
σ_s scatter kernel, mm
σ_r receptor blur, mm
α edge-enhancement gain
σ_u edge-enhancement radius, mm
b vignette
c heel effect
d tilt
BV Pulsera
Cios Fusion
Elekta XVI†
PIXIUM 4600
median over six held-out folds
fold range
fit bounds
physics default
median at a bound
† fitted on 40 frames of the partial COBRA release; refit on the full release pending (A10)
c
C-arm fluoroscopy (2,062, 6 corpora)
radiograph (5,249, 13 corpora)
styled render (1,652)
plain render (2,841)
Cios Fusion (DeepFluoro)
SpineSAC (mixed C-arms)
Surgio-B51 (C-ArmLSpine)
Elekta XVI (COBRA)
BV Pulsera (Geneva)
PIXIUM 4600 (Ljubljana)
Varian (COBRA)
principal component 2 (23 %)
principal component 1 (30 % of variance)
d
PENDING G4
recall against view angle
arc results landed and are under check;
the curve is drawn when they are adopted
vertebrae found (%)
view angle from anteroposterior (°)
−90° = source at the patient's right