S100A9
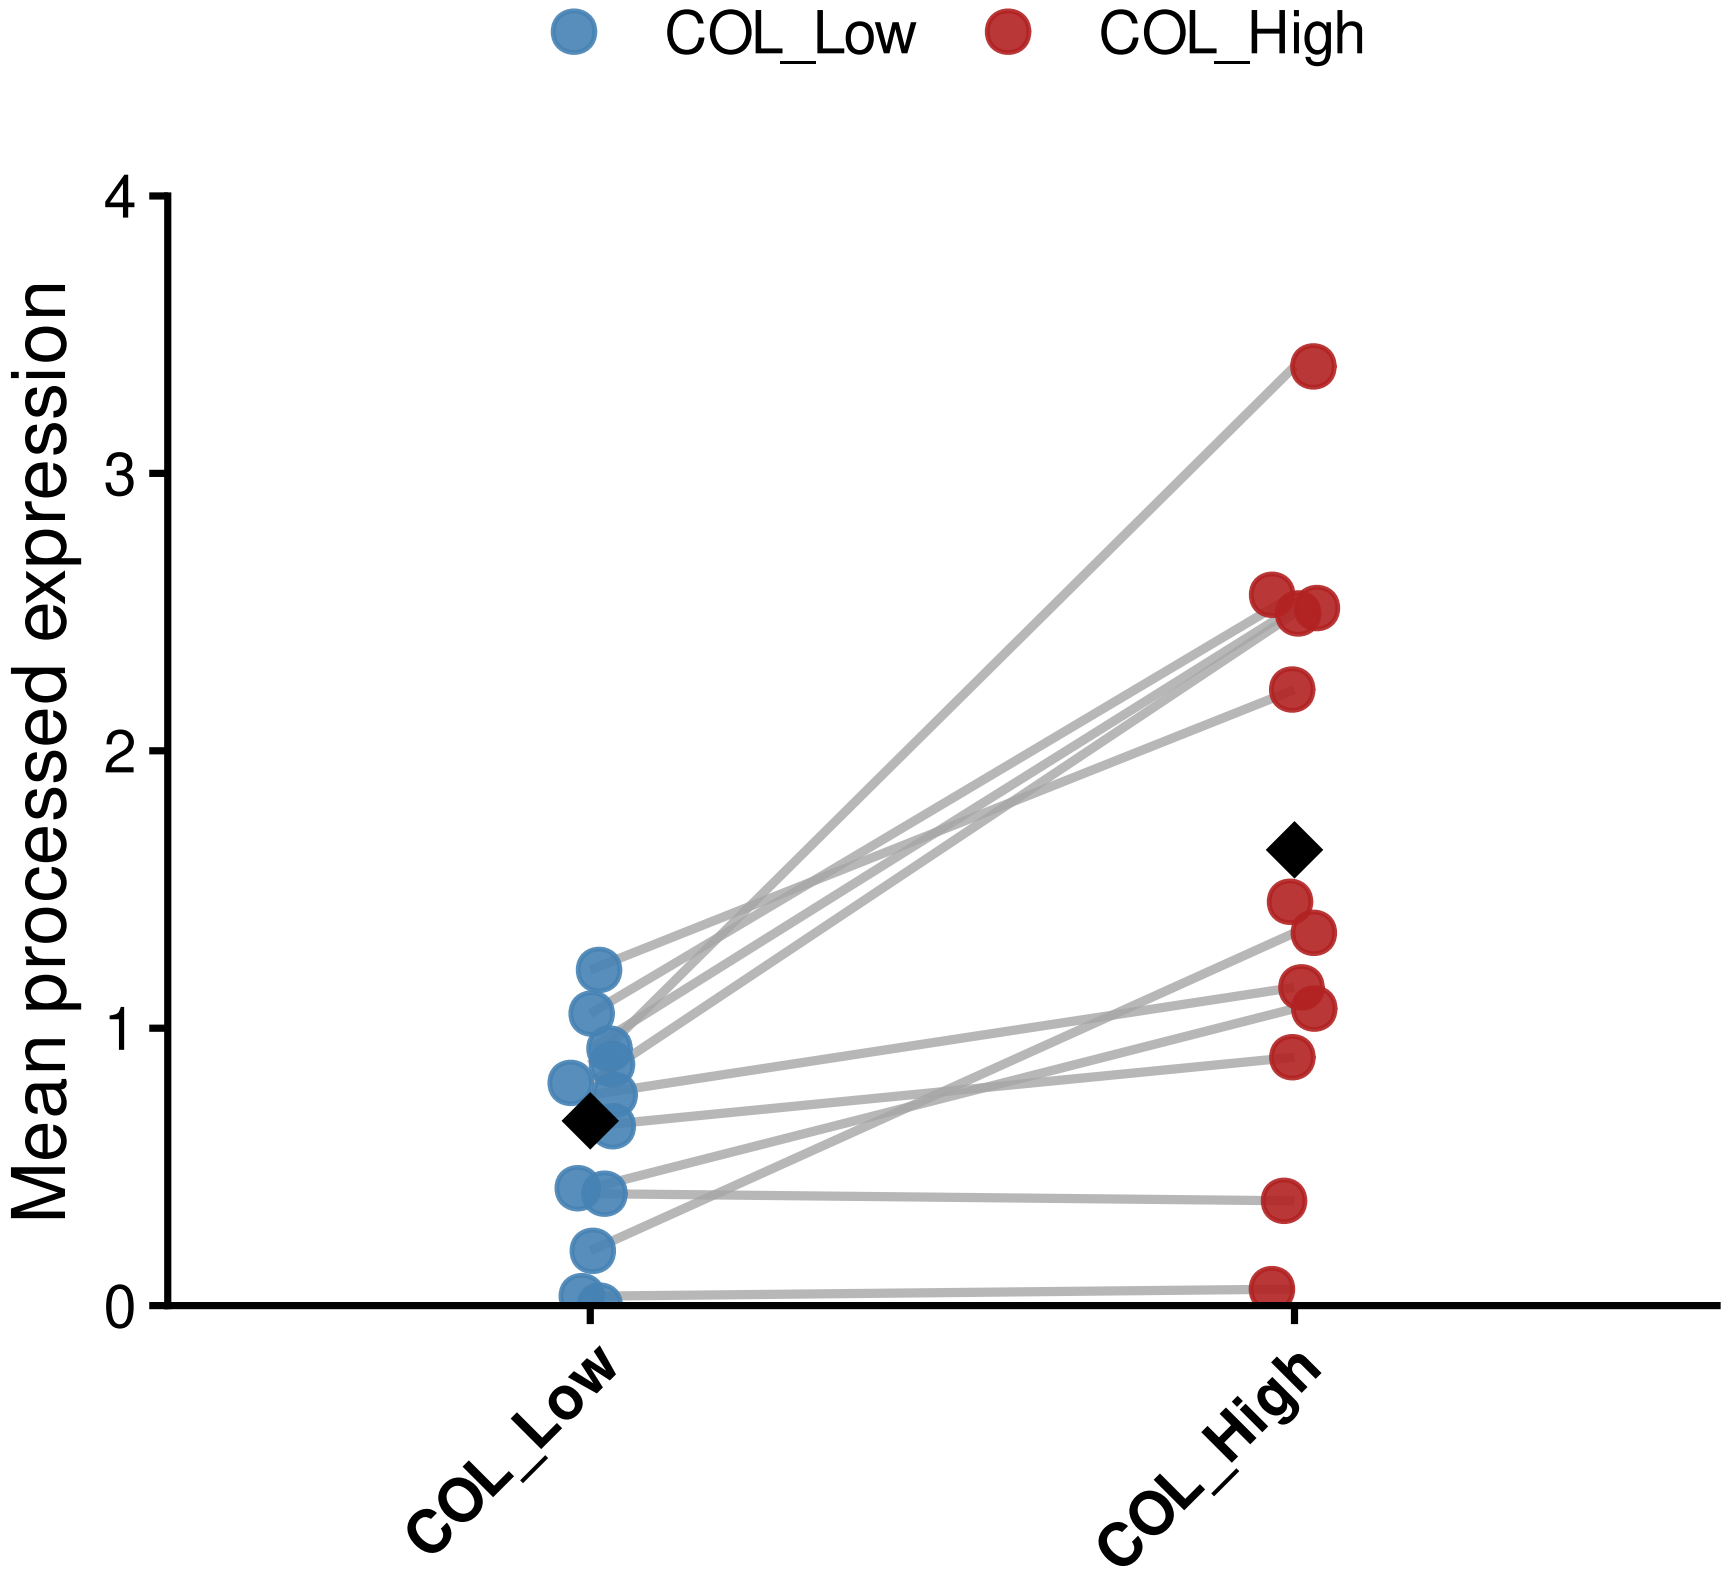
CT and IT regions only; paired Wilcoxon test
p = 0.007; FDR = 0.012; paired n = 11