

College of Science and Engineering

School of Physics and Astronomy

PHYS5036 – Detection and Analysis of Ionising Radiation

Welcome to PHYS5036. Detection and Analysis of Ionising Radiation

In [1]:
```
# Importing the required modules

import matplotlib.pyplot as plt             # Common python package for plotti
ng
import numpy as np                          # For many numerical operation (e.
g. arrays, sine functions, maths constants)
import pandas as pd                         # Common python dataframe package
used in industry and academia
from scipy.optimize import curve_fit        # Commonly used fitting package -
has some tricky syntax but useful to learn to use.
from scipy.odr import ODR, Model, RealData  # Another fitting package (alterna
tive fitting package that allows for errors in x and y)
import os                                   # For getting current working dire
ctory
```

In [2]:
```
%pwd
```

Out[2]:
```
'/home/acheyne/code/glaLabs/prod/Notebooks'
```

Attenuation of Gamma-Radiation in Matter

Data collection steps are typically indicated with a blue title.

Computational work is indicated with a red title.

The purpose of this experiment is to familiarise the student with the calibration of a scintillation counter by observing gamma-ray spectra of several radioisotopes. This data will then be analysed and a Monte Carlo simulation utilised to determine the factors describing gamma-ray attenuation in aluminium and lead.

Absolute Determination Objectives:

- Produce γ-ray spectra using a scintillation counter coupled to a multichannel analyser (MCA).
- Produce a calibration for a scintillation counter, taking into account any experimental uncertainties.
- Measure and identify unknown γ-emitting isotopes, taking the performance characteristics and any uncertainties evaluated into account.
- Calculate the relationship between energy resolution and the γ-ray energy for a scintillation counter.
- Use a Monte Carlo simulation to better understand detector systems and particle interactions.
- Combine simuation with experimental results to determinate the source activity.

Hints:

1. Save your data from Maestro as .Spe file format.
2. All the data-taking for this experiment can be performed in two lab days with proper planning.
3. The code given in this notebook may be incomplete. Make sure you understand the limits and what you are expecting.

Safety in the lab

The experiment makes use of a scintillation counter, various radioactive sources and unvarnished lead bricks used for shielding.

Handling radioactive sources

- Any source removed from the safe **must** be done by one of the demonstators. You are required to sign out any source and **you** are responsible for it until it is returned to the safe.
- Do not "lend" or give your source to a colleague when you are finished with it. Notify a demonstrator who can sign the source back in so it is available for anyone to use.
- Keep exposure to a minimum by handling sources quickly, thinking before handling the source and keeping sources as far away from you and anyone else as much as possible.
    - If the source is not being used for a short time, the source should be put behind lead shielding provided.
        - If the source is not being used for a extended time, it should be returned to the safe. This should be done by a demonstrator who can confirm the source is correctly returned.
        - Sources are wrapped, placed inside containers or have a protective shielding around them. **Do not tamper with the containers and shielding**.
        - Replace the pen sources into the shielding container when not in use.

Operating electronics

Under no circumstances should the HV cables be removed without the lab head present. Make sure you are happy with the setting before turning on the crate and the HV. Ensure you switch the equipment off properly at the end of the day.

Handling Lead Bricks

They are heavy and can cause significant damage if dropped. Do not handle the lead bricks with bare hands. Nitrile (blue rubber) gloves are provided for handling lead bricks. Wash hands thoroughly after contact with lead.

General Rules

Eating and drinking is strictly prohibited in the radiation laboratory. Go into the corridor or stairwell if you need a snack or a drink.

Further safety guidance can be found in the Radioactive Sources in Teaching Labs located on top of the source safe. Please also adhere to the general and specific lab safety guidelines found elsewhere. 1

Section 1 - Background Theory

A Scintillation Detector operates by absorbing energy from fast-moving charged particles and generating a large number of visible and ultraviolet photons. The number of photons generated is a measure of the energy absorbed in the detector. In this experiment, the scintillation material is optically coupled to a silicon photomultiplier.

- Research how a silicon photomultiplier works, and if it is not clear ask a demonstrator.

A typical pulse profile as shown below. The main pulse (negative) is followed by a positive overshoot. It is important to analyse the first portion of the pulse.

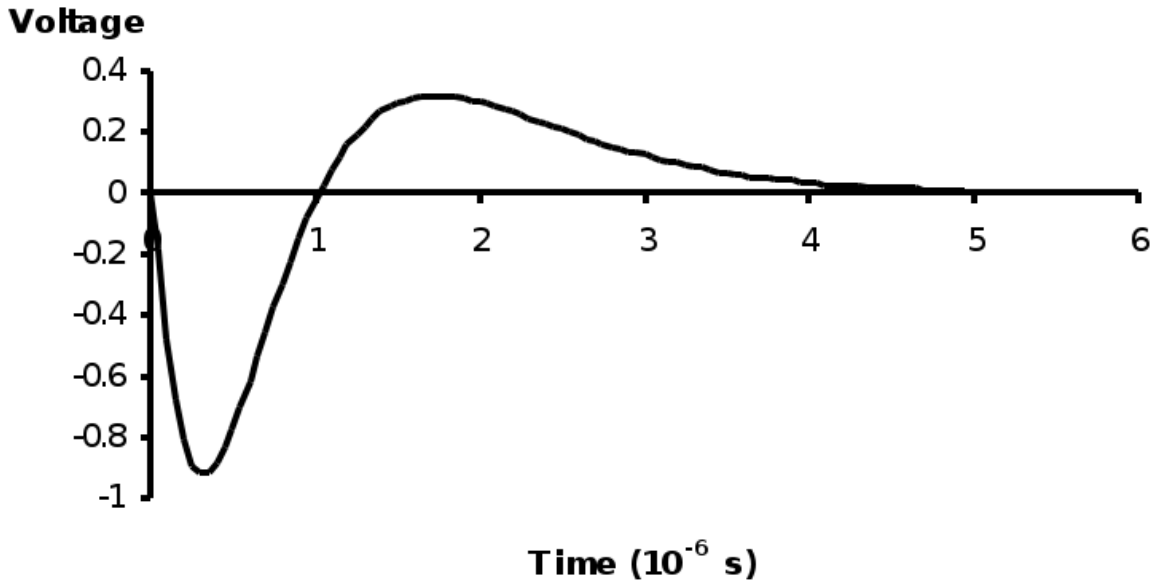


Figure 1: Typical pulse profile for a Sodium Iodide scintillation detector.

1.1. Gamma-ray Interactions:

In this experiment the Scintillation Detector is used to detect gamma-rays emitted by a radioactive source. There are three primary processes by which the gamma-rays can interact with the scintillation material:

1. Photoelectric Effect
2. Compton Scattering
3. Pair Production (for gamma rays of energy >1.02 MeV)

Compton Scattering:

Compton Scattering is the purely kinematic collision of a gamma-ray and a loosely bound electron. The energies of the gamma-ray ($E_{\gamma'}$) and the electron after the collision depend only on the initial gamma-ray energy (E_{γ}) and the angle of deflection (θ) of the gamma ray:

$$E_{\gamma'} = \frac{E_{\gamma}}{1 + \frac{E_{\gamma}}{m_e c^2}(1 - \cos\theta)}$$

where m_e is the electron mass and c is the velocity of light. Thus, the maximum energy that can be transferred to the electron occurs when the photon is deflected through 180°.

Energy Deposited in the Scintillator:

The amount of energy deposited in the scintillator depends on the interactions of the gamma-ray with the scintillator. The three most distinct features, observed in typical energy spectra, are:

1. All the energy of the incident gamma-ray is absorbed by the detector. This produces the Total Energy Peak (also called the Photo Peak) in a spectrum.
2. The gamma-ray Compton Scatters in the scintillator, and the scattered gamma-ray escapes from the crystal without any further interaction. In this case only the energy imparted to the Compton electron is absorbed. This gives rise to a distribution of energies up to the maximum allowed electron energy. The corresponding cut-off is called the Compton Edge because it is an edge, it is less easy to define its position than the Total Energy Peak.
3. The gamma-ray may Compton Scatter outside the scintillator and the scattered gamma-ray may then enter the scintillator and interact. This gives rise to a small Backscatter Peak where the energy of the photon corresponds to a deflection of 130° to 180°. It generally has very low intensity and sits on top of the Compton distribution. Its position is even harder to define experimentally than the Compton Edge.

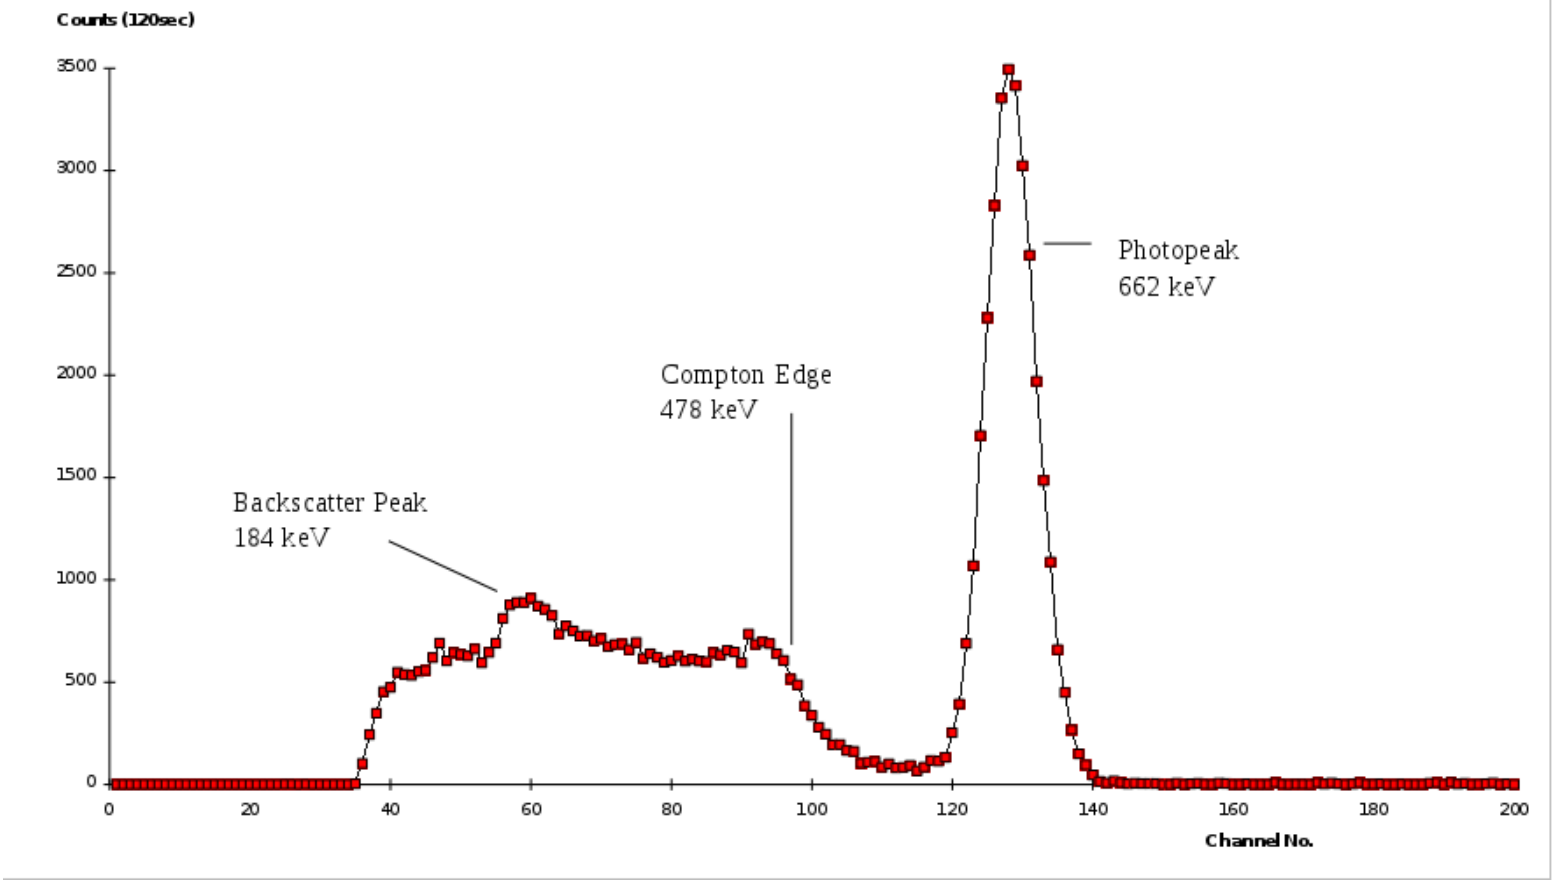


Figure 2: Sodium Iodide spectrum for 137Cs. .

Section 2: Digitisation of the Detector Output Signal

The raw output of the detector is an electrical pulse, the height of which is dependent on the total energy deposited in the detector, while its shape is related to the time profile of the detector material. In order to build up a spectrum of the energy deposited in the detector, the output is usually amplified and then the pulse height digitised in an Analogue-to-Digital Converter (ADC).

2.1. Multi-Channel Analyser and Data Acquisition (DAQ) software

The hardware set-up contains a multi-channel analyser (MCA) with an analogue to digital converter (ADC) that sorts input pulses from the scintillation counter by their amplitudes into 4096 channels (or bins). The MCA used in this experiment is capable or sorting pulses up to 10V.

The Maestro software is used to control the hardware and process this channel data. Ensure your MCA is set to 4096 channels.

The power supply has three channels, turn it on using the POWER button at the bottom left.

Channel 1 — Detector: set to 25.7 V (do not exceed 30 V)
Channel 2 — Pre-amp: set to 5.0 V
Channel 3 — Adjustable: hold the CH3 button to set it and confirm the bottom-right LED reads 5 V

When you are happy with your settings, turn on the detector using the On/Off button. The display on the power supply should show CV under CH1 and CH2 (detector receiving voltage).

Start by inserting the Sr-90, Am-241, Cs-137 mixed source into the source holder in front of the detector.

After a few seconds, you should see tall amplified noise counts in the 0-100 channel range. Remove this by opening Acquire → MCB Properties and raising the Lower Level Discriminator (LLD) to just above that feature (typically 50–120 channels, detector-dependent). Ask for help if you need to cut off more than this.

Clear your measurement and a sharp peak corresponding to the 662 keV photopeak of Cs-137 should now be visible. To keep all sources for this experiment within the available channel range, align this peak to roughly channel 1700 by increasing or decreasing the gain from the amplifier in the crate. Read the exact channel by clicking the spectrum and checking the Marker value.

ASK A DEMONSTRATOR BEFORE ADJUSTING THE VOLTAGE

Clear and restart the acquisition to see the effect of any changes. Once you are satisfied, do not change the high voltage or amplifier gain further for the remainder of the experiment.

Now obtain a spectrum for Cs-137 and save the file in ASCII SPE format. If you are using this notebook, upload to JupyterHub to an appropriatly named folder.

All measurements of this type are affected by background signals due to factors such as electronic noise and cosmic radiation. To obtain a true energy spectrum arising from just the source radiation, you will also need a background measurement taken the same day as your source data. The background spectrum will be subtracted from each source spectrum.

2.2. Acquisition time and Poisson statistics.

Radiation counts follow Poisson statistics. The fractional (relative) statistical uncertainty of ε on a measured peak area, can be described as

$$\varepsilon \approx \frac{1}{\sqrt{N}}$$

where N is the net counts in the peak after background subtraction. So in order to get a 10% measurement, for example, we need N = 100 counts.

General tips:

- Pick a target fractional uncertainty for key measurements
- If background is non-neglibible, aim for more counts than this
- Ensure background measurement will be at least as long as each source run, longer will help reduce background uncertainties.
- You can estimate counts using the peak, or use the region-of-interest (ROI) feaure in the acquisition software to check the integrated peak counts in that region.

2.3. Analysis introduction

Below you will find a function made to read in the .spe files and return a data frame for use in analysis. Please read through it in order to understand its function, but you are not expected to edit this.

In [3]:

```
## The code below extracts the data from your .spe files and returns it as a p
andas dataframe.
## you are not expected to edit this - but feel free to make changes if you ar
e confident.

def extract_data(filename):
    """Extracts channel range, counts, and measurement times from .spe file"""
    start = end = None
    counts = None
    livetime = realtime = None

    with open(filename, "r") as f:
        lines = f.readlines()
    i = 0
    while i < len(lines):
        line = lines[i].strip()
        if line == "$MEAS_TIM:":
            # Extract measurement times (from header. Syntax: livetime, realti
me)
            livetime, realtime = map(float, lines[i+1].split())
        elif line == "$DATA:":
            # Extract channel start and end (from header)
            start, end = map(int, lines[i+1].split())
            nochannels = end - start + 1
            # Read channel values
            block = lines[i+2:i+2+nochannels]
            counts = np.array([int(x.strip()) for x in block], dtype=int)
        i += 1
    return start, end, counts, livetime, realtime


def read_spe_files(data_file, background_file, bin_num=4096):
    # Extract data and background
    data_start, data_end, yield1, data_livetime, data_realtime = extract_data
(data_file)

    if background_file is None:
        # No background file provided - return data only
        print("No background file provided - returning data only. Please ensur
e you have accounted for background in your analysis!")
        channel = np.arange(data_start, data_end + 1, dtype=int)
        error1 = np.sqrt(yield1.astype(float))
        df = pd.DataFrame({
            "channel": channel,
            "data": yield1,
            "err_data": error1,
        })
        return df

    else:
        bg_start, bg_end, yield2, bg_livetime, bg_realtime = extract_data(back
ground_file)

        # check that they are the same length
        if (data_start, data_end) != (bg_start, bg_end):
            raise ValueError("data and background files have different channel
ranges!")

        # Background-subtracted counts (scaled by uptime)
        yield3 = yield1 - yield2*(data_livetime/bg_livetime)
```

```
        # Channels
        channel = np.arange(data_start, data_end + 1, dtype=int)

        # Poisson errors
        error1 = np.sqrt(yield1.astype(float))
        error2 = np.sqrt(yield2.astype(float))
        error3 = np.sqrt((error1**2) + (error2*(data_livetime/bg_livetime))**
2)

        # Assemble into a DataFrame
        df = pd.DataFrame({
            "channel": channel,
            "data": yield1,
            "err_data": error1,
            "background": yield2,
            "err_background": error2,
            "data_bgsubtracted": yield3,
            "err_data_bgsubtracted": error3,
        })

        # Rebin if requested. I.e. if bin_number = 512, rebin to 512 channels
        if bin_num is not None:
            if bin_num not in [512, 1024, 2048, 4096, 8192, 16384]:
                raise ValueError("bin_num must be one of [512, 1024, 2048, 409
6, 8192, 16384]")
            if (data_end - data_start + 1) % bin_num != 0:
                raise ValueError(f"Cannot rebin to {bin_num} channels - origin
al number of channels is {data_end - data_start + 1}, which is not a multiple
of {bin_num}")
            rebin_factor = (data_end - data_start + 1) // bin_num
            df_rebinned = df.groupby(df.index // rebin_factor).sum().reset_ind
ex(drop=True)
            df_rebinned["channel"] = np.arange(bin_num)
            df = df_rebinned

        return df
```

Upload your saved Caesium-137 and background measurements to an appropriate folder and edit the code below.

The code below shows how to read in the files with the above function (`read_spe_files`) and some simple analysis methods to get your started.

Edit the code below to plot the Cs-137 data you just recorded.

In [4]:
```
# example of using the read in function

# print current folder from os
print(f"Current working folder: {os.getcwd()}, make sure to set path relative
to this")

# set file paths here to YOUR OWN files
data_file = "cs137mix.spe"
background_file = "background.spe"

# define our pandas data frame by reading in the spe files
df_source = read_spe_files(data_file, background_file)

# show a few lines of the dataframe to check it looks OK and view the column n
ames
df_source[40:50]
```

```
Current working folder: /home/acheyne/code/glaLabs/prod/Notebooks, make sure t
o set path relative to this
```

Out[4]:


	channel	data	err_data	background	err_background	data_bgsubtracted	err_data_bgsubtracted
40	40	145	12.041595	22	4.690416	136.016230	12.192971
41	41	168	12.961481	18	4.242641	160.649643	13.076756
42	42	154	12.409674	19	4.358899	146.241289	12.536678
43	43	160	12.649111	18	4.242641	152.649643	12.767206
44	44	177	13.304135	19	4.358899	169.241289	13.422678
45	45	169	13.000000	19	4.358899	161.241289	13.121292
46	46	137	11.704700	12	3.464102	132.099762	11.789870
47	47	137	11.704700	27	5.196152	125.974464	11.895474
48	48	152	12.328828	11	3.316625	147.508115	12.402995
49	49	178	13.341664	13	3.605551	172.691409	13.422659


Below we show a very simple method to plot a column of the dataframe and how to select a subset.

In [5]:

```
# Simple plot of the data and how to select a subset
plt.plot(df_source["channel"],df_source["data_bgsubtracted"])
plt.plot(df_source["channel"][1100:1500],df_source["data_bgsubtracted"][1100:1
500]) # only plot channels 1200:1999
plt.show()

# Alternate way using variables to define the range with some extra features
# Plotting just chosen range, but with error bars
min, max = 1450, 2000
plt.errorbar(df_source["channel"][min:max], df_source["data_bgsubtracted"][mi
n:max], yerr=df_source["err_data_bgsubtracted"][min:max], fmt='o', label='Subs
et with error bars')
plt.xlabel('Channel')
plt.ylim(0, 500)
plt.legend()
plt.show()
```

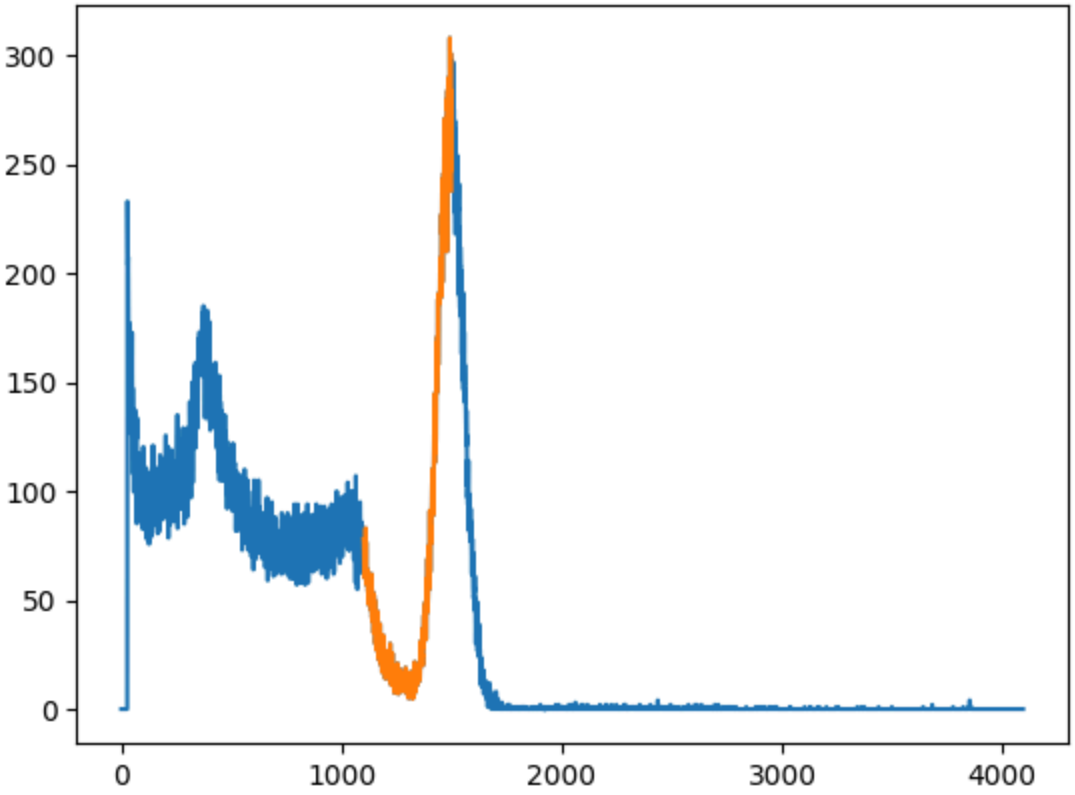

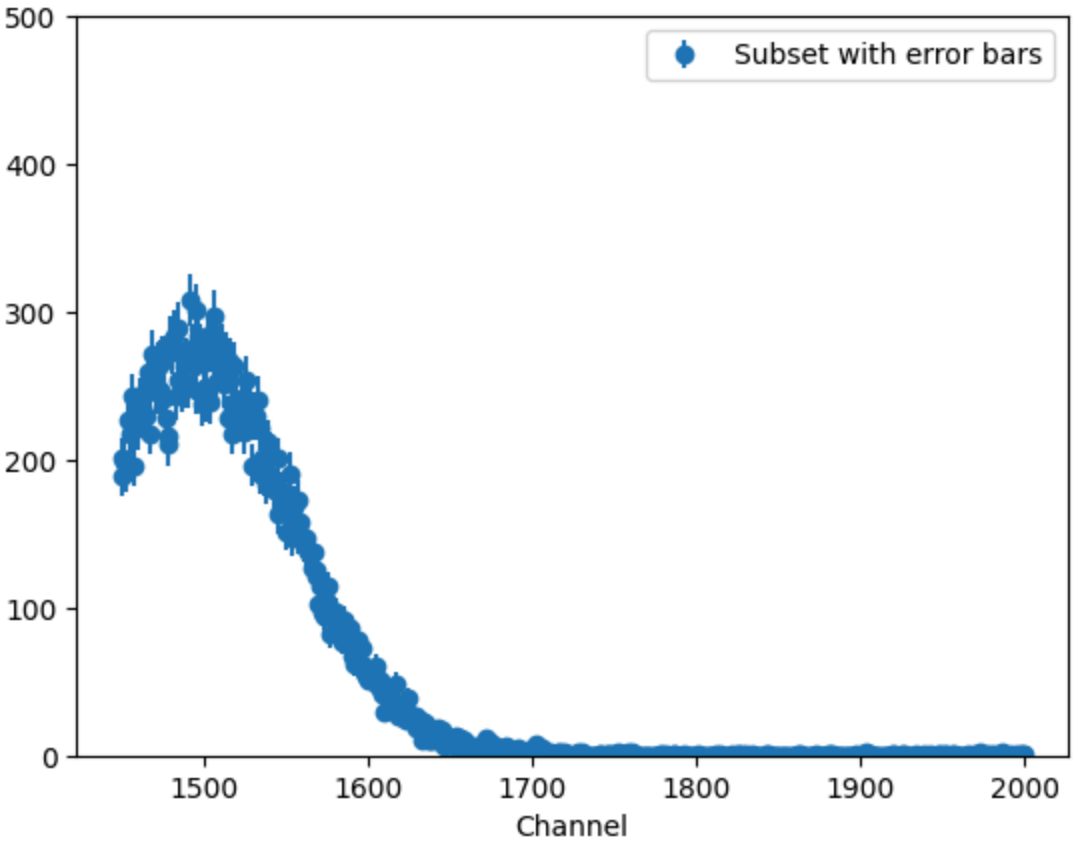

Discuss with peer(s) or staff your thoughts on the following:

- Can you name the features shown in the spectrum?
- Is the data taking up the full channel range, if not why?

2.3.1 Energy Calibration data

In order to calibrate the detectors, we will need to find the relationship between the known energy of the different gamma-ray photopeaks and the corresponding measured ADC channel.

The aim of this section is to performing fits to the main photopeaks and fill in the table below. Some of the values in this table will be needed later in the analysis.

Photopeak data

Source	Peak channel	Error (ch)	Peak σ (ch)	Error	Integral (counts)	Error
Co-57						
Co-60						
Co-60						
Cs-137						
Na-22						
Na-22						

To do this as accurately as possible, the photopeaks must be fitted with a function that describes both the background under the photo peak and the peak itself. Consider the shape of the photopeak and how you can use this knowledge to fit an appropriate model and extract its parameters. Note that the uncertainty on the peak position is required.

Ask the demonstrators if you are unsure and need some pointers.

In [6]:
```
# Write a function to model a Gaussian peak + polynomial background. An exampl
e of writing a fit function is shown below for a polynomial background.

def polybackground(x,const,lin,quad):
    background = const+lin*x+quad*x*x
    return background

def peakfit():
    return peak

def signalFit():
    return peak+background

def doubleSignalFit():
    return peak1 + peak2 + background
```

In [7]:
```
# Plot the photopeak region of Cs-137 and perform a fit to the data here
```

At this stage, check with a demonstrator that your code is correct and that you have obtained a reasonable value for Cs-137.

Now repeat this procedure. Note the shape of the photopeaks of Co-60 and how you should adapt your model to reflect this.

Discuss with peer(s) or staff your thoughts on the following:

> - When fitting the photo peak, which fitting function is recommended—Gaussian, Lorentzian, or something else?
> - How do you identify multiple peaks in the spectrum if they overlap?

2.3.2 Energy Calibration Fitting

To accurately determine the energy of detected events, the detector readouts (recorded in channel numbers) must be calibrated against known photon energies. This converts spectra from an arbitrary channel scale into a meaningful energy scale.

Using the known photopeak energies in the table below, we will:

1. Plot the relationship between the measured photopeak channel number and the known photopeak energy.
2. Fit this relationship using orthogonal distance regression (ODR), since the uncertainties are primarily in the x-values.
3. Evaluate the quality of each fit by examining residuals and computing the reduced chi-squared (χ^2) value.

Reference Photopeak Energies

Isotope	Photopeak (keV)
Am-241	59.5
Co-57	122
Co-60	1172
Co-60	1333
Cs-137	662
Na-22	511
Na-22	1275

Procedure

1. Plot the Data

- Create a scatter plot of energy (keV) versus channel number for your measured photopeaks (include horizontal error bars)

In [8]:
```
# Space for analysis code
```

2. Calibration Fitting

Fit the calibration curve with a straight line, using ODR.

$$E(x) = a_0\, x + a_1$$

- x is the channel number measured by the detector.
- $E(x)$ is the predicted energy in keV.
- The parameters a_0, a_1 are determined from the fitting procedure.
- Remember to include errors in your fit.

How to fit a straight line Using ODR

Since the uncertainties are in x, we will use `scipy.odr`, a fitting package designed for errors in both variables.

Below is an example of how to fit a straight line to your data:

```
from scipy.odr import ODR, Model, RealData

# Define straight line function for ODR
def straightLine(B, x):
    m, c = B

    return m*x + c

# Prepare the data, including x-errors, you can add y-errors with sy
data = RealData(Channel, Energy, sx=Channel_Error)

# Create the model
model = Model(straightLine)

# Set up and run ODR
odr = ODR(data, model, beta0=[1, 1])  # beta0 is your initial guess for slope and int
ercept
output = odr.run()

# Extract optimal parameters and their uncertainties
popt, perr = output.beta, output.sd_beta

print("Optimal parameters:", popt)
print("Parameter uncertainties:", perr)
```

3. Assessing Fit Quality: Residuals and Chi-Squared

Residuals

To evaluate the quality of your fit, it is helpful to start with a visual inspection of the residuals before moving on to statistical measures.

The residuals are the differences between the measured energies and the energies predicted by the fitting function:

$$\text{Residual}_i = E_i - E_{\text{fit},i}$$

Dividing this by the error is often referred to as the 'pull'.

Plotting residuals as a function of channel number can reveal:

- Systematic trends suggesting the model does not capture the data fully.
- Outliers with unusually large deviations.
- Whether the scatter of residuals is consistent with expected experimental uncertainty.

Did you assess the quality of your peak fitting in section 2.3.1? Should you?

```
In [9]: # Space for analysis code
```

Chi-squared

In order to assess the quality of your fit, we need to define a criterion for what makes a "good" fitting function. The most common statistical measure for evaluating how well a model describes data is the chi-squared (χ^2) statistic.

The chi-squared statistic quantifies the total deviation between your measured values and those predicted by the fitted function, weighted by measurement uncertainties:

$$\chi^2 = \sum_i \left(\frac{E_i - E_{\text{fit},i}}{\sigma_{x,i}} \right)^2$$

where E_i is the measured energy (in keV), $E_{fit,i}$ is the energy predicted by the model, and $\sigma_{x,i}$ is the uncertainty in meausred channel position.

A smaller number then is generally better as you predicted energies match the known energies well. However, it depends on how many data points and free parameters are in the model. To compare models with different numbers of parameters, we calculate the reduced chi-squared statistic, defined as

$$\chi^2_{reduced} = \frac{\chi^2}{N - p}$$

where N is the number of data points, and p is the number of parameters in your fit.

A good fit will generally yield a reduced $\chi^2_{reduced}$ value close to 1:

- $\chi^2_{reduced}$ = 1. The model describes the data within expected uncertainties.
- $\chi^2_{reduced}$ < 1. The data scatter is smaller than expected (possibly overestimated errors).
- $\chi^2_{reduced}$ > 1. The model does not describe the data well or uncertainties are underestimated.

Will a good fit give exactly 1? How much deviation is acceptable? Ask a demonstrator if unsure.

4. Compare and Conclude

- Plot the fitted function over your data for visual comparison.
- Select and justify the if this is a good fit for your energy calibration curve.

> Would adding more parameters (e.g., quadratic vs. linear) meaningfully improves the fit, or merely overfit the data?

```
In [10]: # Space for analysis code
```

Estimating Uncertainty on Energy

If the fit function is:

$$E = f(x, a_0, a_1, \ldots, a_n)$$

where x is the measured channel and $a_0, a_1, \ldots, a_n$ are the fitted parameters.

The uncertainty in E is:

$$\sigma_E^2 = \left(\frac{\partial f}{\partial x}\sigma_x\right)^2 + \sum_i \left(\frac{\partial f}{\partial a_i}\sigma_{a_i}\right)^2 + 2\sum_{i<j} \frac{\partial f}{\partial a_i}\frac{\partial f}{\partial a_j}\operatorname{cov}(a_i, a_j)$$

Where:

- $\frac{\partial f}{\partial x}$ is the partial derivative of the function with respect to the channel measurement.
- σ_x is the uncertainty in your channel measurement.
- $\frac{\partial f}{\partial a_i}$ is the partial derivative with respect to each fitted parameter.
- σ_{a_i} is the uncertainty in the fitted parameter a_i (obtained from ODR).
- $\operatorname{cov}(a_i, a_j)$ is the covariance between fitted parameters a_i and a_j (the off-diagonal elements of the covariance matrix from ODR).

  The covariance terms is important here because the fitted parameters are correlated, they also combine in the Energy conversion formula so ignoring this can over- or under-estimate σ_E.

In matrix form (convenient in code), with $J = \left(\frac{\partial f}{\partial a_0}, \frac{\partial f}{\partial a_1}, \ldots\right)$ and V the covariance matrix of the parameters:

$$\sigma_E^2 = \left(\frac{\partial f}{\partial x}\sigma_x\right)^2 + J\,V\,J^T$$

> - Convert channel to energy and propagate the uncertainty from your fit.
> - Compare your result with and without the covariance terms.
> - Which parameters are most strongly correlated?

```
In [ ]: # space for analysis code
```

Section 3 - Determination of unknown sources

In real-life, measurements like this can be used to help determine the presence of unknown radioactive sources based on their characteristics discussed in this lab.

Using the same method as before:

- take measurements for the "unknown" sources labelled A1145 and 1270,
- find the channel number of their photopeak (or photopeaks) and
- use your energy calibration curve to determine the photopeak energies.

Use the table below to help determine what you think the unknown sources are, justifying your answer. When more than one peak is present in the spectrum, the relative intensities of the photopeaks may provide additional information to help your identification.

Isotope	Half-life ($T_{1/2}$)	γ-ray Energy (keV)	Relative Intensity (%)
Am-241	433 years	14	13.5
		18	21.0
		21	5.0
		26	2.5
		60	35.3
		32–38	8.0

Cs-137 30.1 years 66285.1 Ba-133 10.8 years 30–36123 802.4 8133.8 2767.1 30318.7 35661.9 3848.9 Cd-109 453 days 88100 Co-57 270.5 days 149.4 12285.2 13611.1 Co-60 5.27 years 117399.86 133399.98 Na-22 2.60 years 511181 127599.95

Discuss with peer(s) or staff your thoughts on the following:

- How closely do the measured energies need to match tabulated gamma energies to confidently identify a source?
- What should we do if our measured peak energy falls between two known gamma lines?
- Are there common gamma sources that show up as background contaminants in the lab?

In [12]:
```
# Space for analysis code
```

Section 4 - Resolution of the Detector

At this stage you should compute the Full Width Half Maximum (FWHM) for each of the photopeaks. This can be obtained by multiplying the standard deviation of the photopeak by 2.355 (specifically $2\sqrt{2ln2}$). The uncertainty in the FWHM should also be obtained.

The finite width of the observed photopeaks is a result of the same energy deposit in a detector not giving the same pulse height for successive measurements. This is because there is an intrinsic variation in the number of (in this case) optical scintillation photons, subject to the familiar counting statistics rules. The spread is proportional to $\sqrt{N}$, where N is the total number of optical scintillation photons for a given energy deposit. It is not possible to reliably simulate a detector system without first determining how this resolution varies with the energy of the incident radiation.

The resolution of a photopeak is defined as:

$$R = \frac{\text{FWHM of Peak}}{\text{Peak Value}} = kE^n$$

Where E is the photopeak gamma-ray energy and k, n are constants.

Using your energy calibrated values:

- Find the resolution for each of the photopeaks.
- Plot your resolution values as a function of photopeak energy.
- Using the equation above, determine values for k, n. Consider also if there are any mathematical operations that can be applied to the equation to make the resulting model easier to fit.

Discuss with peer(s) or staff your thoughts on the following:

> - What does the extracted value of n tell you about the operation of this type of scintillation detector?
> - How does your extracted n comapre to the expected value? What does this suggest?

In [13]:
```
# Space for analysis code
```

Section 5 - Absorption of Gamma Radiation

The intensity of gamma radiation decreases exponentially as it passes through an absorber, described by Lambert's Law of Absorption:

$$I(x) = I_0 e^{-\mu x}$$

where I_0 is the initial intensity, $I(x)$ is the transmitted intenstiy after absorber thickness x, and μ is the linear attenuation coefficientfor the absorbing material. The half-value depth, $d_{½}$, is the thickness of the absorbing material that will reduce the original intensity by half.

- Derive a formula for $d_{½}$, expressing it in terms of μ
- Determine the linear attenuation coefficient,μ, and thus $d_{½}$, for aluminium and lead at different γ-radiation energies.
- Make suitable measurements using at least four different thicknesses of both aluminium and lead **(make sure to use the blue nitrile (rubber) gloves when handling lead)**. Think about how you can use the information about the photopeak to get the intesnsity. Check with a demonstrator if you are unsure.
- Discuss the dependence of μ and $d_{½}$ on energy and material. Compare with standard values.
- Sometimes linear absorption coefficients are expressed in units of $cm^2 g^{-1}$. Discuss why this is appropriate and how the conversion between this and cm^{-1} is made.

Task: Measure the linear attenuation coefficients, μ

Measure μ and half-value depth $d_{½}$ for aluminium, steel, and lead at 2 different γ-ray energies.

Hints:

- Use the table known photopeak energies from before and your experience of counting rates to suggest suitable sources for this measurement.
- Use at least four different absorber thicknesses per material, chosen to span a sufficient range of transmission.
- Ensure background subtraction is applied when extracting peak counts.
- Plan measurement times so that statistical uncertainties remain reasonable even at higher absorber thicknesses - all measurements must be the same duration for this section.
- Intensity can be determined by integraintg the counts under the peak

Discuss with peer(s) or staff your thoughts on the following:

> - How do attenuation coefficients vary with absorber material and photon energy?
> - In what practical contexts (e.g. shielding design, medical physics, nuclear safety) is this knowledge applied?

In [14]:
```
# Space for analysis code
```

Section 6 - Simulation: Run a Monte Carlo Simulation

A numerical simulation based upon Monte Carlo techniques is employed in this experiment in order to demonstrate how important and widely-used these types of software tools are in sub-atomic and detector physics.

Research how these type of numerical methods are used to simulate the interaction of radiation with matter and therefore the response of detectors.

6.1. Getting started:

First, if not done so already, follow the steps in the “First Computing Set Up Steps” document, found on the Lab Moodle page, under the Lab Material→Computing section. It provides some useful introductory reading for using the School’s computing. Once you are happy with that document, log into JupyterHub in the normal way (remember if you are working remotely, you will need to first connect via VPN).

https://jupyter.physics.gla.ac.uk/hub/login (https://jupyter.physics.gla.ac.uk/hub/login)

Then - if not done so already - as detailed in the "Experiment Computing Set Up Document" found on the Lab Moodle page, under the Lab Material→Computing section, execute the command:

```
source /local/cern/software/Sim/SoftwareSetup.sh
```

The simulation we will use is a Geant4 particle transport Monte Carlo simulation called SodiumIodideMC which has been designed specifically for this laboratory. The simulated set up is shown in Figure 3. Although we are simulating a sodium iodide detector here, the principles are transferable to this experiment and it will suffice for the intended purposes of this exercise.

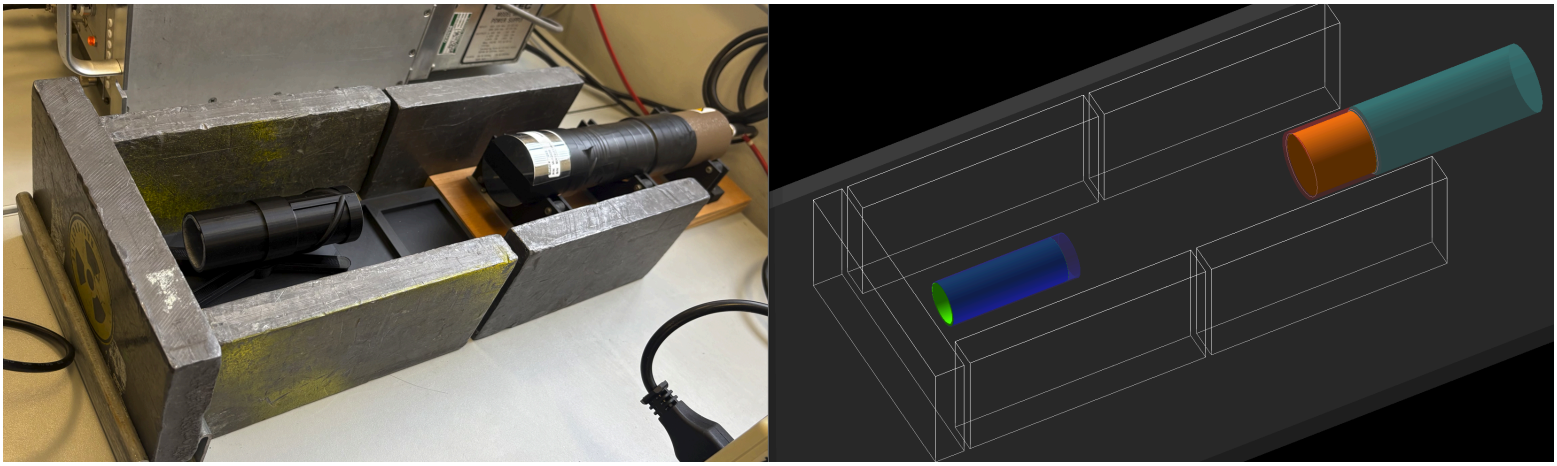


Figure 3: Left shows a sodium iodide scintillation counter in the lab. Right shows a simulation of the detector. detector.

Advanced: *For students interested in the Geant4 software details, the C++ class definition files can be found on Moodle in the Computing section, in a folder called “SodiumMC Source Code.” Have a look at the folders and files inside. The class implementation files are in SodiumIodideMC/src/ subdirectory. Have a look through these classes if you are curious how the C++ code for a Geant4 simulation is run and ask if you have any questions or if you would like someone to explain it to you.*

6.2. Run the simulation

The simulation should be run four times to simulate the measurements that were taken in the lab during the energy calibration with the four different radioactive sources.

To set up the simulation, you will need to change the config.json file. This file contains all the parameters that define the simulation, and should look something like this:

```
{
    "sourceName": "Cs137",
    "nEvents": "250000",
    "detectorHolderDistance": "50",
}
```

Note: To edit this json, you may have to right-click -> Open With -> Editor.

The other four parameters used for this experiment are:

- sourceName: This is the name of the source you are simulating. The options are Am241, Na22, Cs137 and Co60.
- nEvents: This is the number of decay events you want to simulate. A value of 250,000 is a good compromise between computational speed and statistical quality.
- detectorHolderDistance: This is the distance **in mm** between the source and the front face of the detector. **You will need to measure this with a ruler and input into the config yourself**.

Once you have set the set your desired simulation parameters, you can run the simulation by running the following commands in the terminal:

```
cd ~/PHYS_5036-labs
runGammaLabMC.py
```

Alternatively, if you make more than one config and its not named config.json, you can specify which config to use by running:

```
cd ~/PHYS_5036-labs
runGammaLabMC.py <configFileName>.json
```

This will run the simulation and generate two output files (with file format `G4_<detectorType>_<sourceName>.spe/pdf`):

- an .spe file containing the simulated energy spectrum, and
- a .pdf file containing a quick-look plot of the simulated spectrum.

Note that a simulated background file is also generated. The output files will be written into the data folder. You can run the simulation elsewhere if you prefer, but please note that the data files will always be created in the same folder which the simulation is executed from.

6.3. Analyse the simulated spectra

Once you have ran all four source simulations (it can take a while), plot the simulated spectra for the four sources. You should be able to use the analysis method that you previously used for experimental data for the analysis of simulated data.

Discuss with peer(s) or staff your thoughts on the following:

> - How well do they agree with your experimental data?
> - Are there any significant differences, and what are the possible reasons for these differences?

In [ ]: