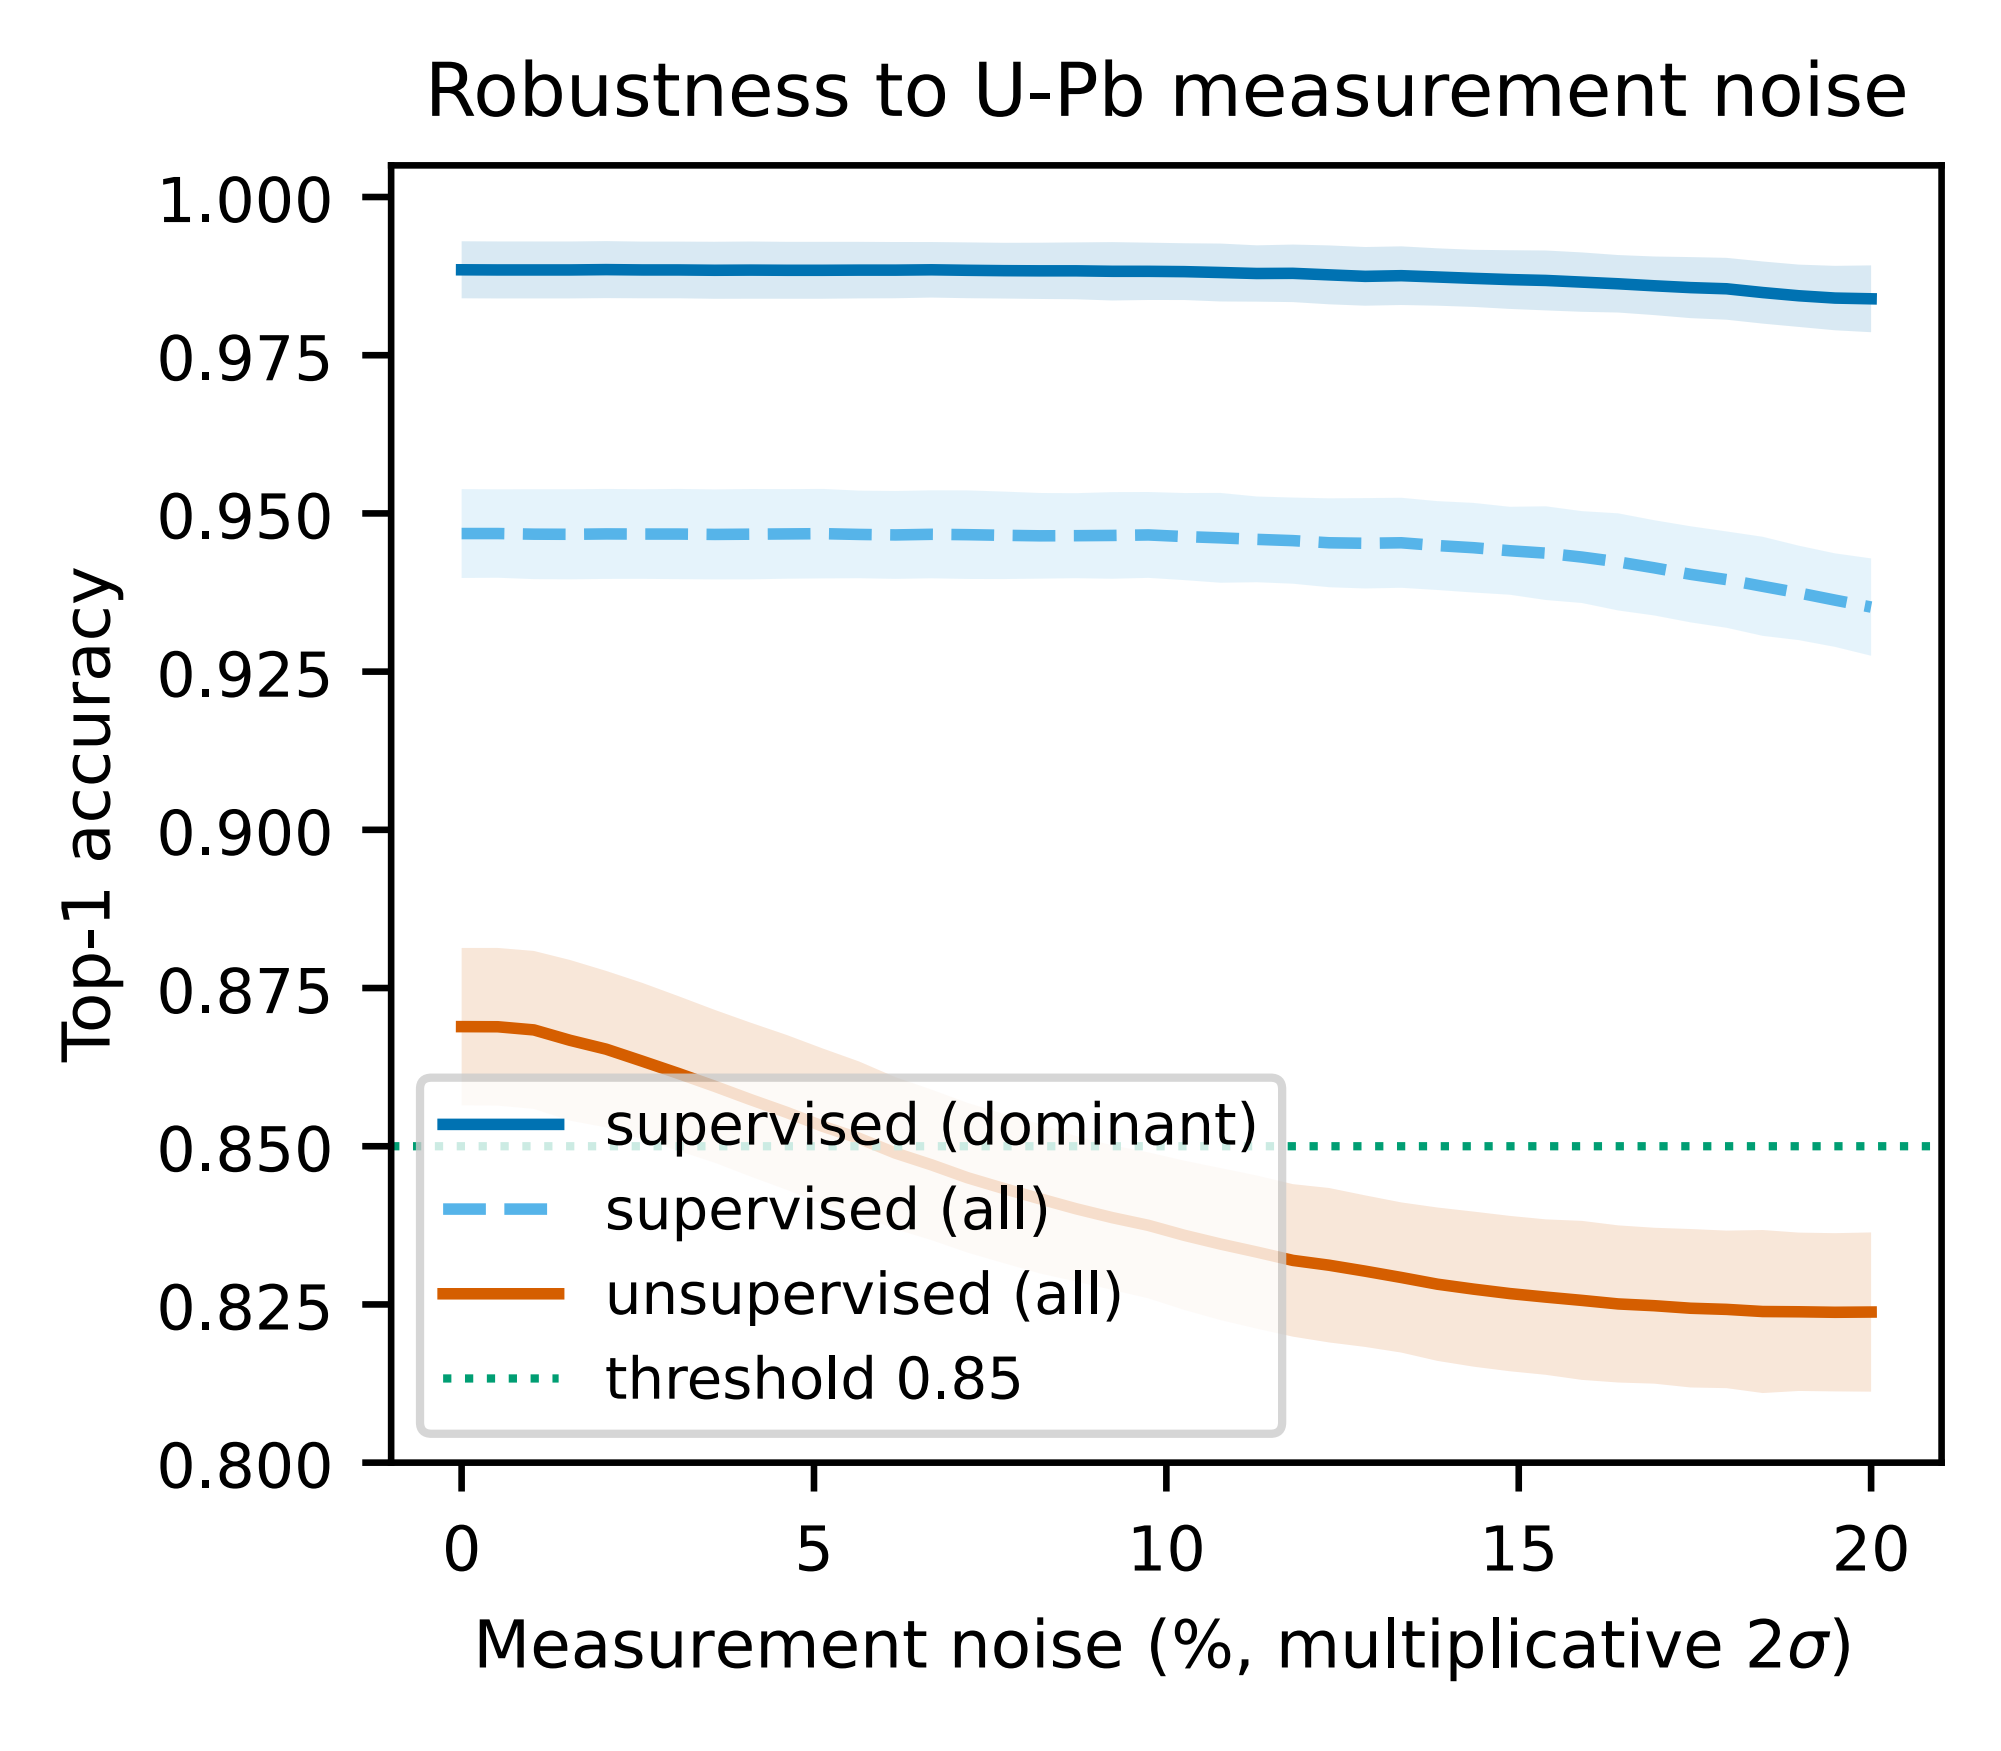
Robustness to U-Pb measurement noise
Top-1 accuracy
1.000
0.975
0.950
0.925
0.900
0.875
0.850
0.825
0.800
0
5
10
15
20
Measurement noise (%, multiplicative 2σ)
supervised (dominant)
supervised (all)
unsupervised (all)
threshold 0.85