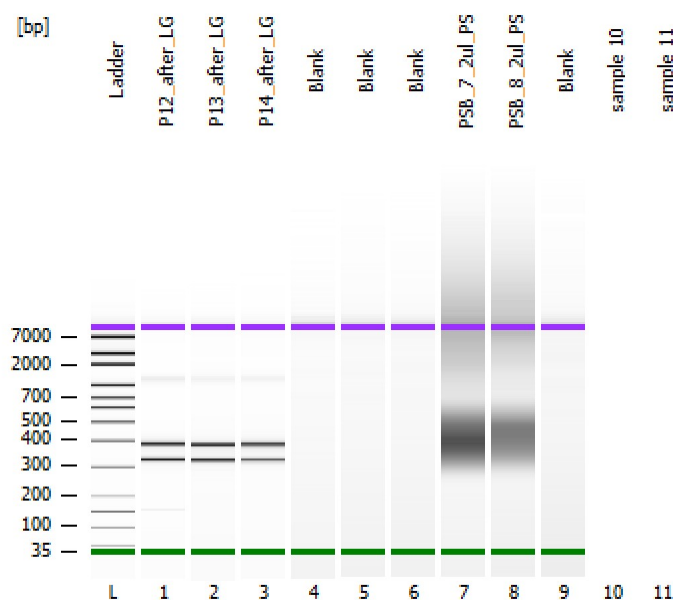


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

Electrophoresis File Run Summary



Instrument Information:

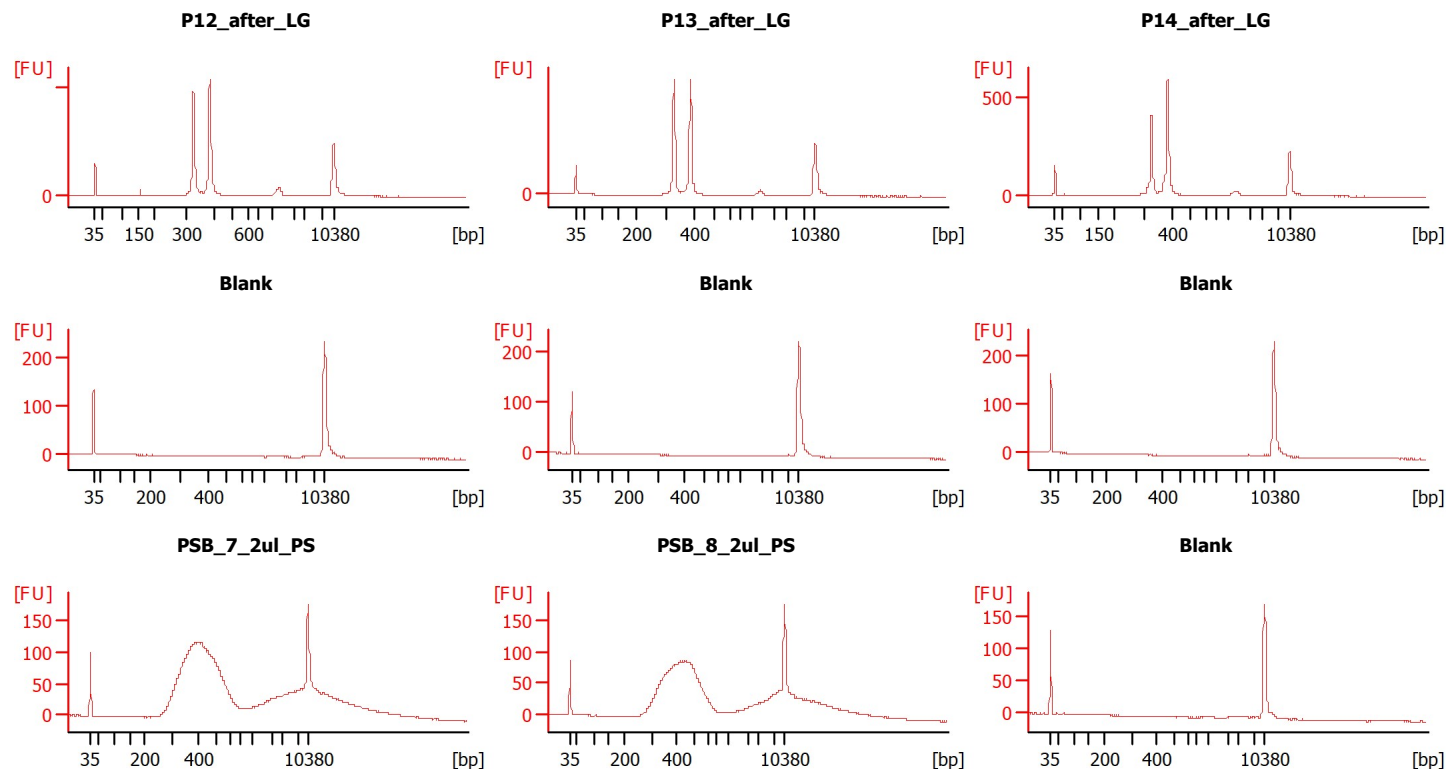
Instrument Name: DE54107817 Firmware: C.01.069
Serial#: DE54107817 Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:



Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest . Digest	St at on	Observati	Result Label	Result Color
P12_after_LG		☐	✓			
P13_after_LG		☐	✓			
P14_after_LG		☐	✓			
Blank		☐	✓			
Blank		☐	✓			
Blank		☐	✓			
PSB_7_2ul_PS		☐	✓			
PSB_8_2ul_PS		☐	✓			
Blank		☐	✓			
sample 10		☐				
sample 11		☐				
Ladder		☐	✓			

Chip Lot #**Reagent Kit Lot #****Chip Comments :**

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4

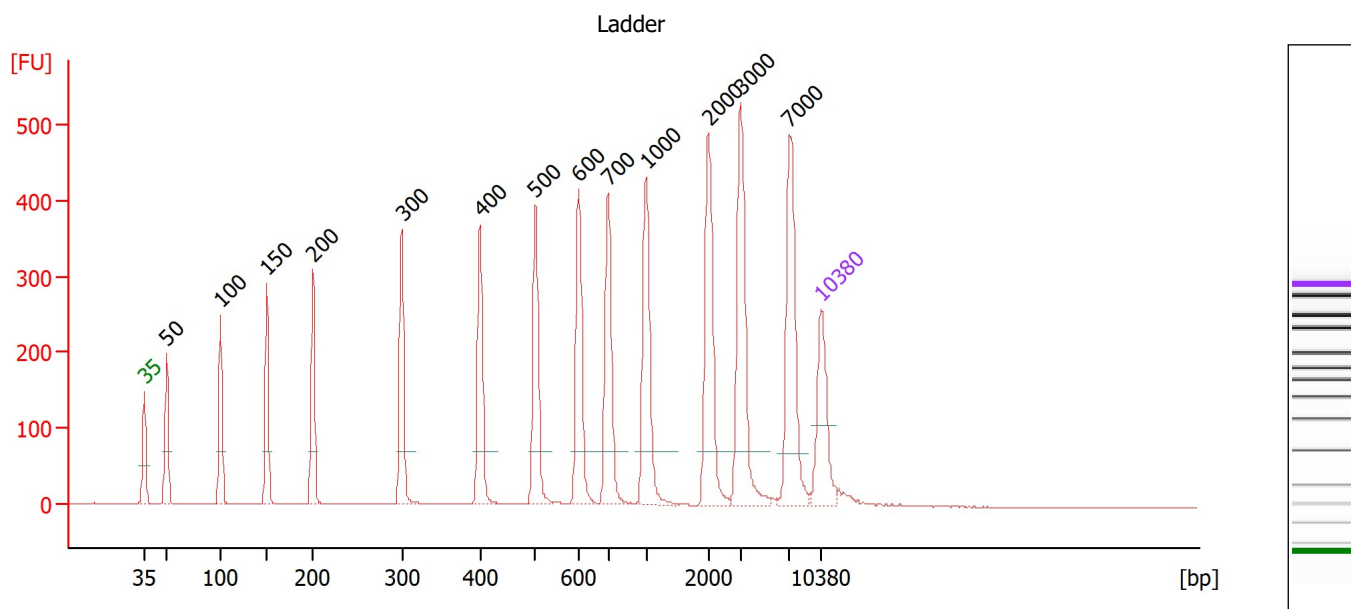
Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary



Overall Results for Ladder

Noise: 0.3

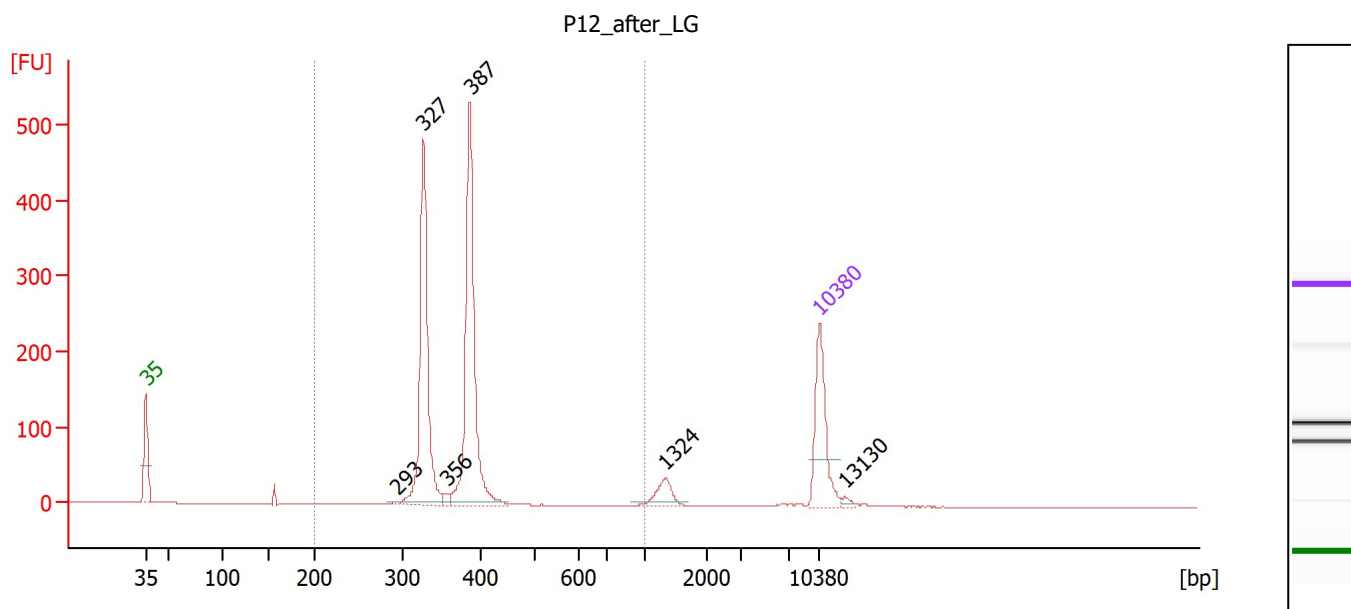
Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...



Overall Results for sample 1 : P12_after_LG

Number of peaks found: 6 Corr. Area 1: 1,353.8
 Noise: 0.3

Peak table for sample 1 : P12_after_LG

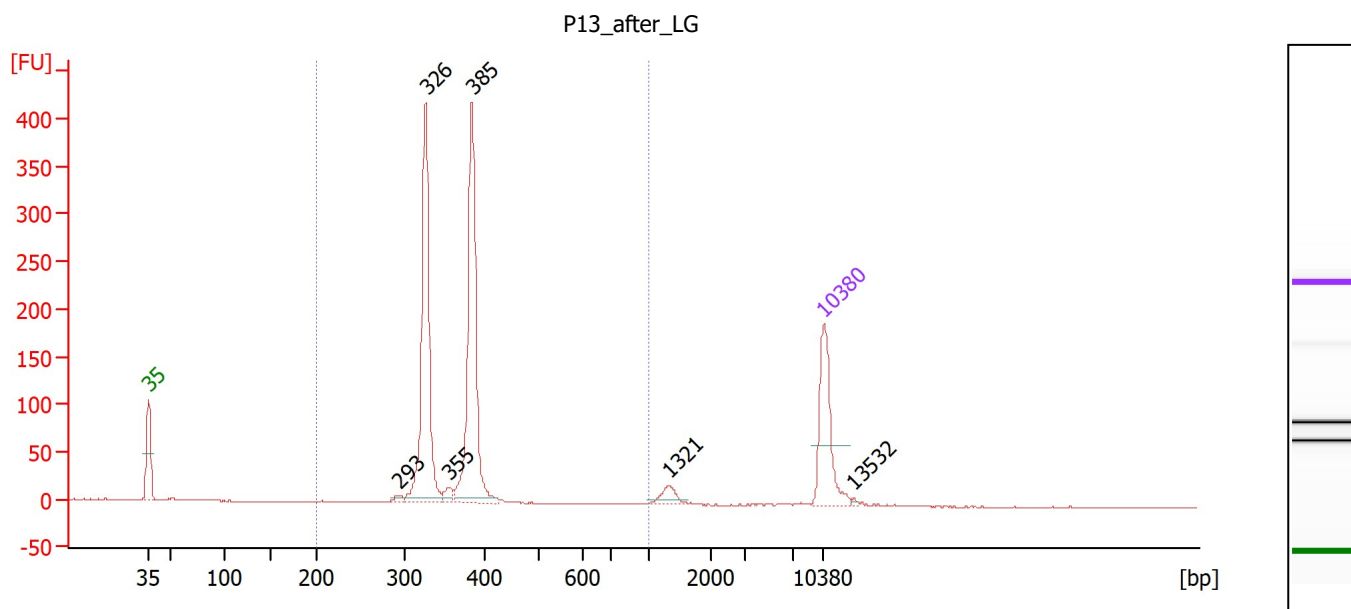
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	293	2.67	13.8	
3	327	264.25	1,223.5	
4	356	7.44	31.7	
5	387	286.86	1,124.1	
6	1,324	23.17	26.5	
8	13,130	0.00	0.0	

Region table for sample 1 : P12_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,353.8	93	362	9.7	552.13	2,318.4	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...**Overall Results for sample 2 : P13 after LG**

Number of peaks found: 6 Corr. Area 1: 1,104.3
 Noise: 0.4

Peak table for sample 2 : P13 after LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	293	5.28	27.3	
3	326	264.98	1,232.6	
4	355	10.30	44.0	
5	385	257.48	1,013.3	
6	1,321	14.39	16.5	
8	13,532	0.00	0.0	

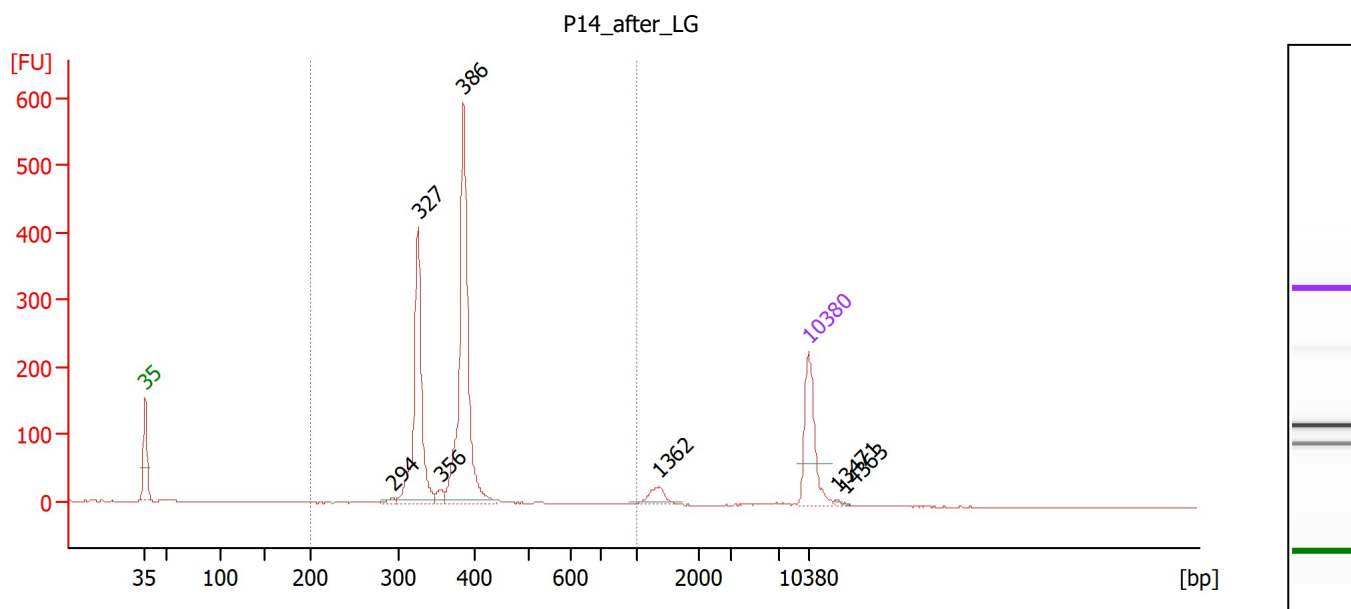
Region table for sample 2 : P13 after LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,104.3	96	357	8.8	533.65	2,270.4	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...



Overall Results for sample 3 : P14 after LG

Number of peaks found: 7 Corr. Area 1: 1,400.8
 Noise: 0.4

Peak table for sample 3 : P14 after LG

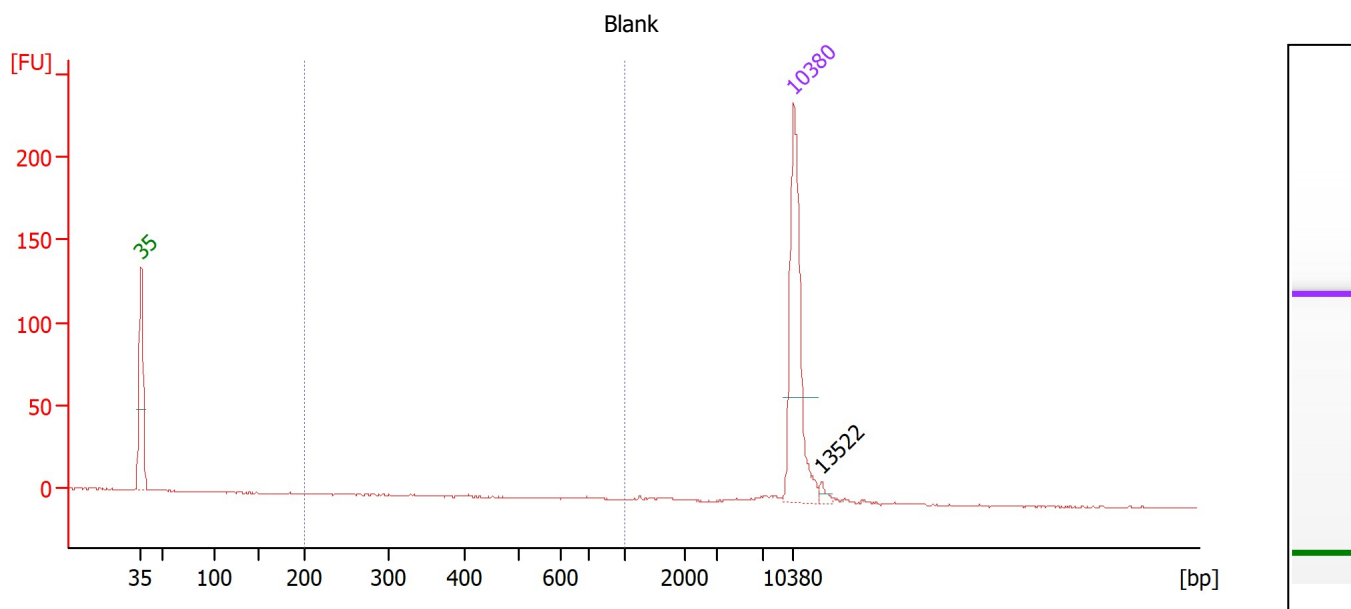
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	294	4.52	23.3	
3	327	240.54	1,115.5	
4	356	10.67	45.4	
5	386	347.57	1,365.3	
6	1,362	18.59	20.7	
8	13,471	0.00	0.0	
9	14,363	0.00	0.0	

Region table for sample 3 : P14 after LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,400.8	93	367	12.4	614.22	2,556.9	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...**Overall Results for sample 4 : Blank**

Number of peaks found: 1 Corr. Area 1: 0.1
 Noise: 0.3

Peak table for sample 4 : Blank

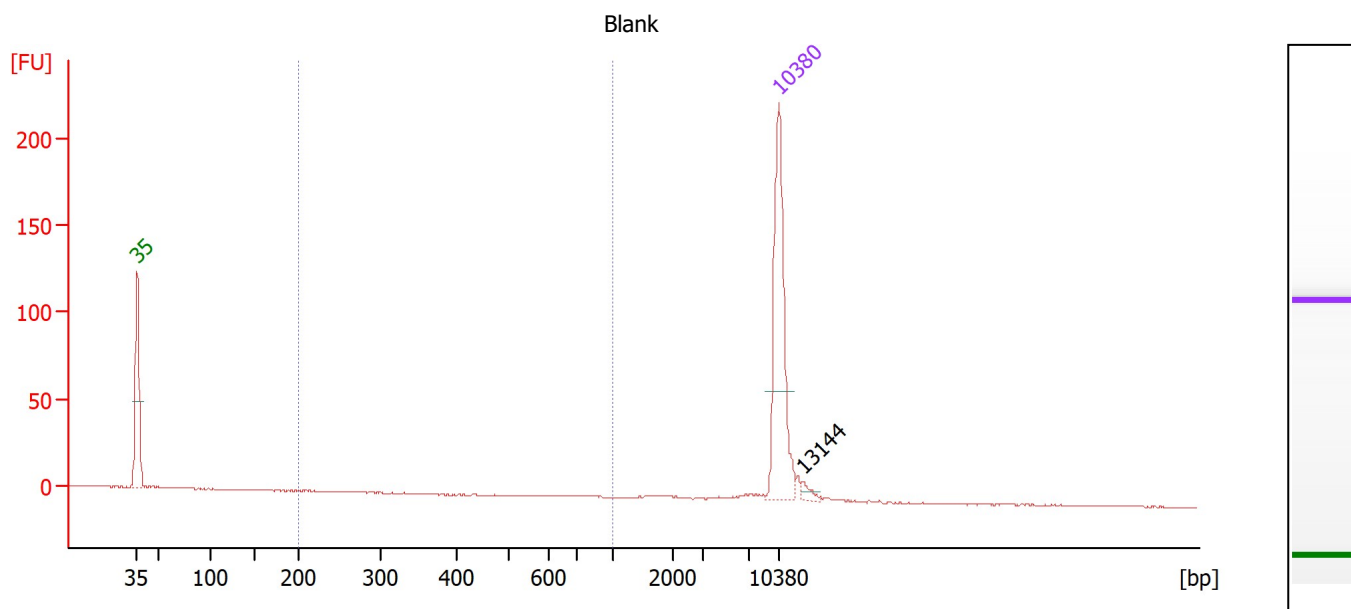
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
3	13,522	0.00	0.0	

Region table for sample 4 : Blank

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	0.1	1	603	22.8	0.04	0.1	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...**Overall Results for sample 5 : Blank**

Number of peaks found: 1 Corr. Area 1: 1.0
 Noise: 0.3

Peak table for sample 5 : Blank

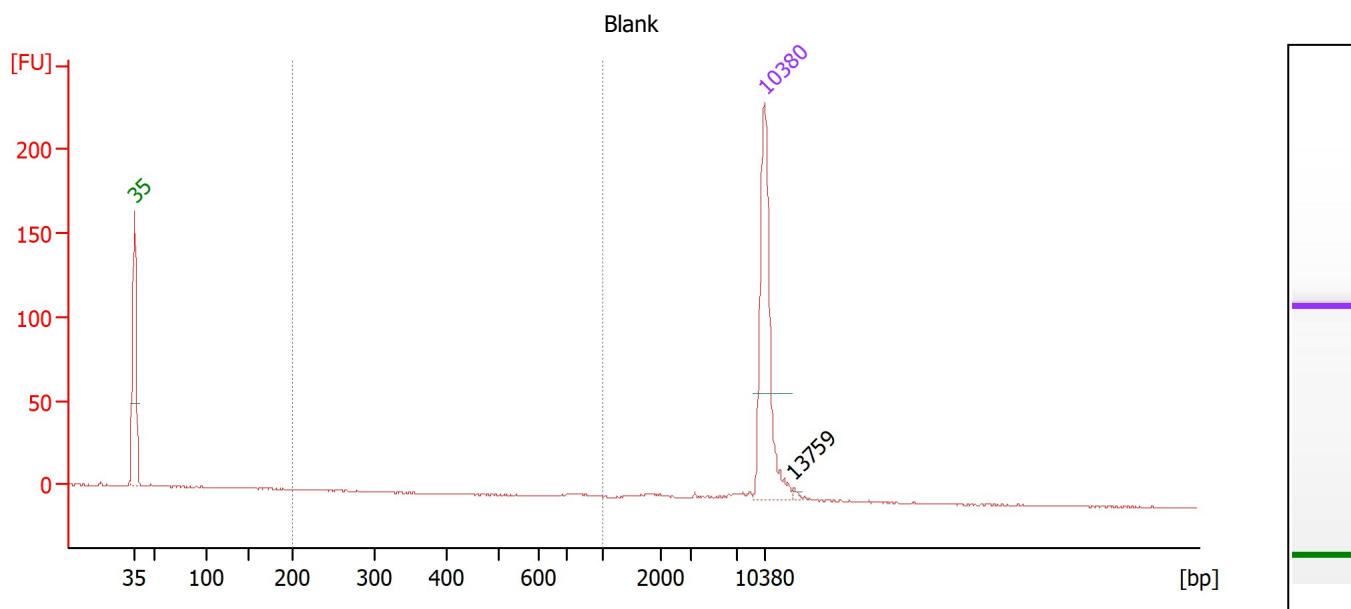
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
3	13,144	0.00	0.0	

Region table for sample 5 : Blank

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1.0	2	723	14.9	0.40	0.9	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...**Overall Results for sample 6 : Blank**

Number of peaks found: 1 Corr. Area 1: 0.7
 Noise: 0.3

Peak table for sample 6 : Blank

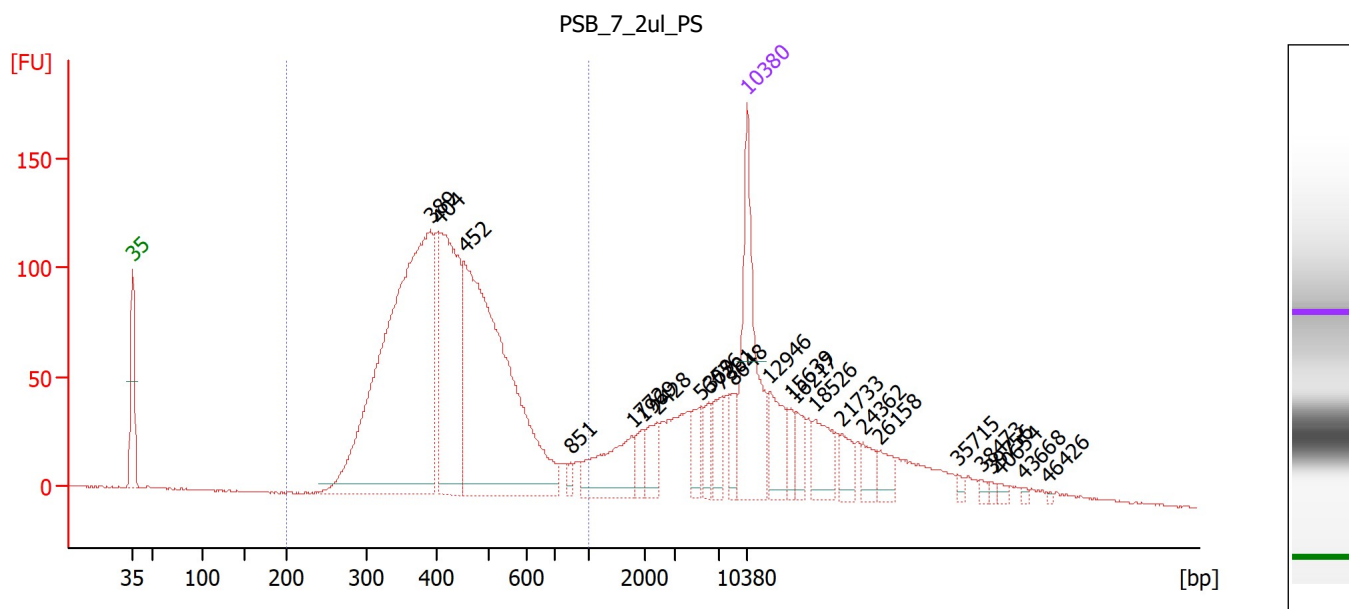
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
3	13,759	0.00	0.0	

Region table for sample 6 : Blank

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	0.7	3	783	5.9	0.26	0.5	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...**Overall Results for sample 7 : PSB_7_2ul_PS**

Number of peaks found: 24 Corr. Area 1: 2,213.0
 Noise: 0.4

Peak table for sample 7 : PSB_7_2ul_PS

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	389	399.46	1,555.1	
3	404	152.22	571.2	
4	452	313.49	1,049.8	
5	851	4.57	8.1	
6	1,772	38.75	33.1	
7	1,969	9.61	7.4	
8	2,428	13.92	8.7	
9	5,359	15.39	4.4	
10	6,076	11.06	2.8	
11	7,301	15.34	3.2	
12	8,648	11.71	2.1	
14	12,946	0.00	0.0	
15	15,639	0.00	0.0	
16	16,217	0.00	0.0	
17	18,526	0.00	0.0	
18	21,733	0.00	0.0	
19	24,362	0.00	0.0	
20	26,158	0.00	0.0	
21	35,715	0.00	0.0	
22	38,473	0.00	0.0	
23	39,756	0.00	0.0	
24	40,654	0.00	0.0	
25	43,668	0.00	0.0	
26	46,426	0.00	0.0	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

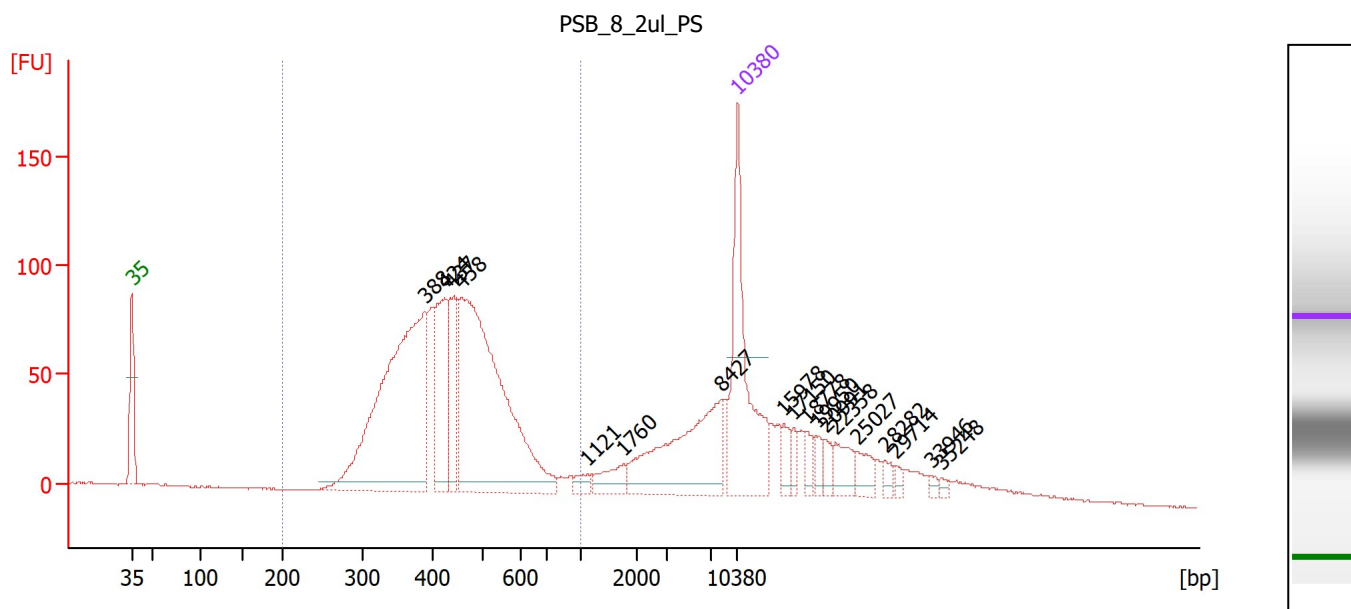
Electropherogram Summary Continued ...

... Region table for sample 7 : PSB_7_2ul_PS

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp] r	To [bp]
Region 1	2,213.0	67	439	26.3	928.76	3,450.4	 200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...**Overall Results for sample 8 : PSB_8_2ul_PS**

Number of peaks found: 18 Corr. Area 1: 1,602.5
 Noise: 0.4

Peak table for sample 8 : PSB_8_2ul_PS

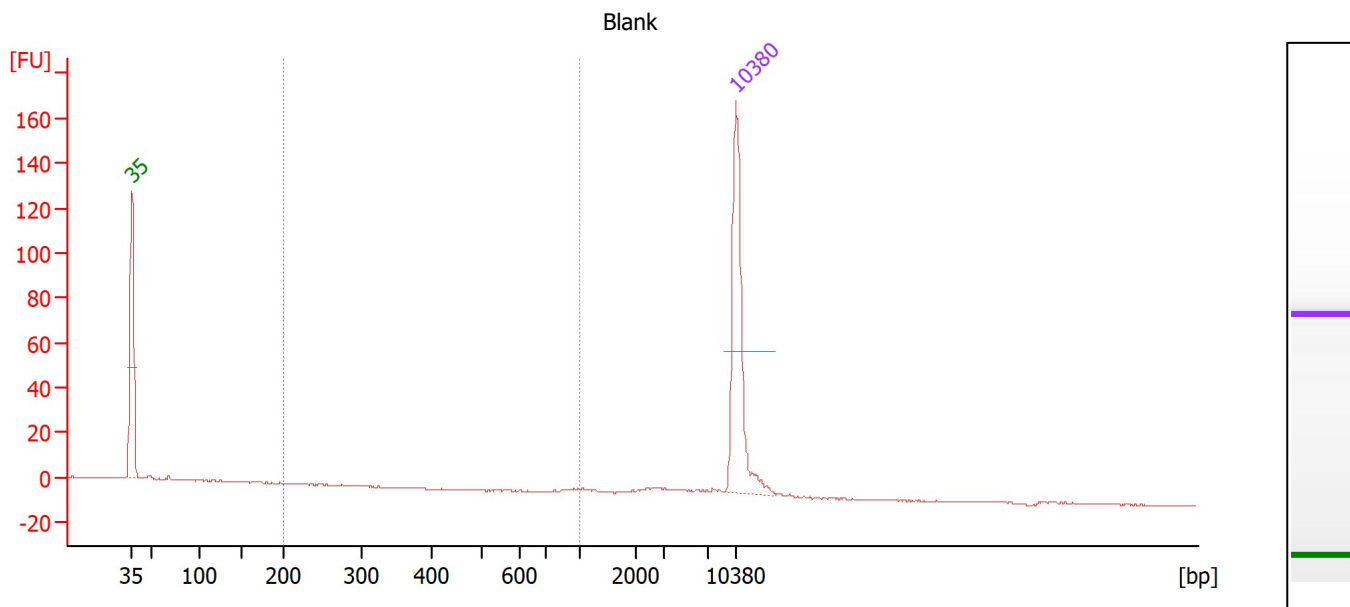
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	388	231.28	903.5	
3	424	63.91	228.6	
4	437	39.53	137.2	
5	458	233.18	771.4	
6	1,121	5.49	7.4	
7	1,760	11.49	9.9	
8	8,427	71.98	12.9	
10	15,978	0.00	0.0	
11	17,150	0.00	0.0	
12	18,778	0.00	0.0	
13	19,950	0.00	0.0	
14	20,991	0.00	0.0	
15	22,358	0.00	0.0	
16	25,027	0.00	0.0	
17	28,282	0.00	0.0	
18	29,714	0.00	0.0	
19	33,946	0.00	0.0	
20	35,248	0.00	0.0	

Region table for sample 8 : PSB_8_2ul_PS

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,602.5	68	444	23.8	614.21	2,235.7	200	1,000

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

Electropherogram Summary Continued ...**Overall Results for sample 9 : Blank**

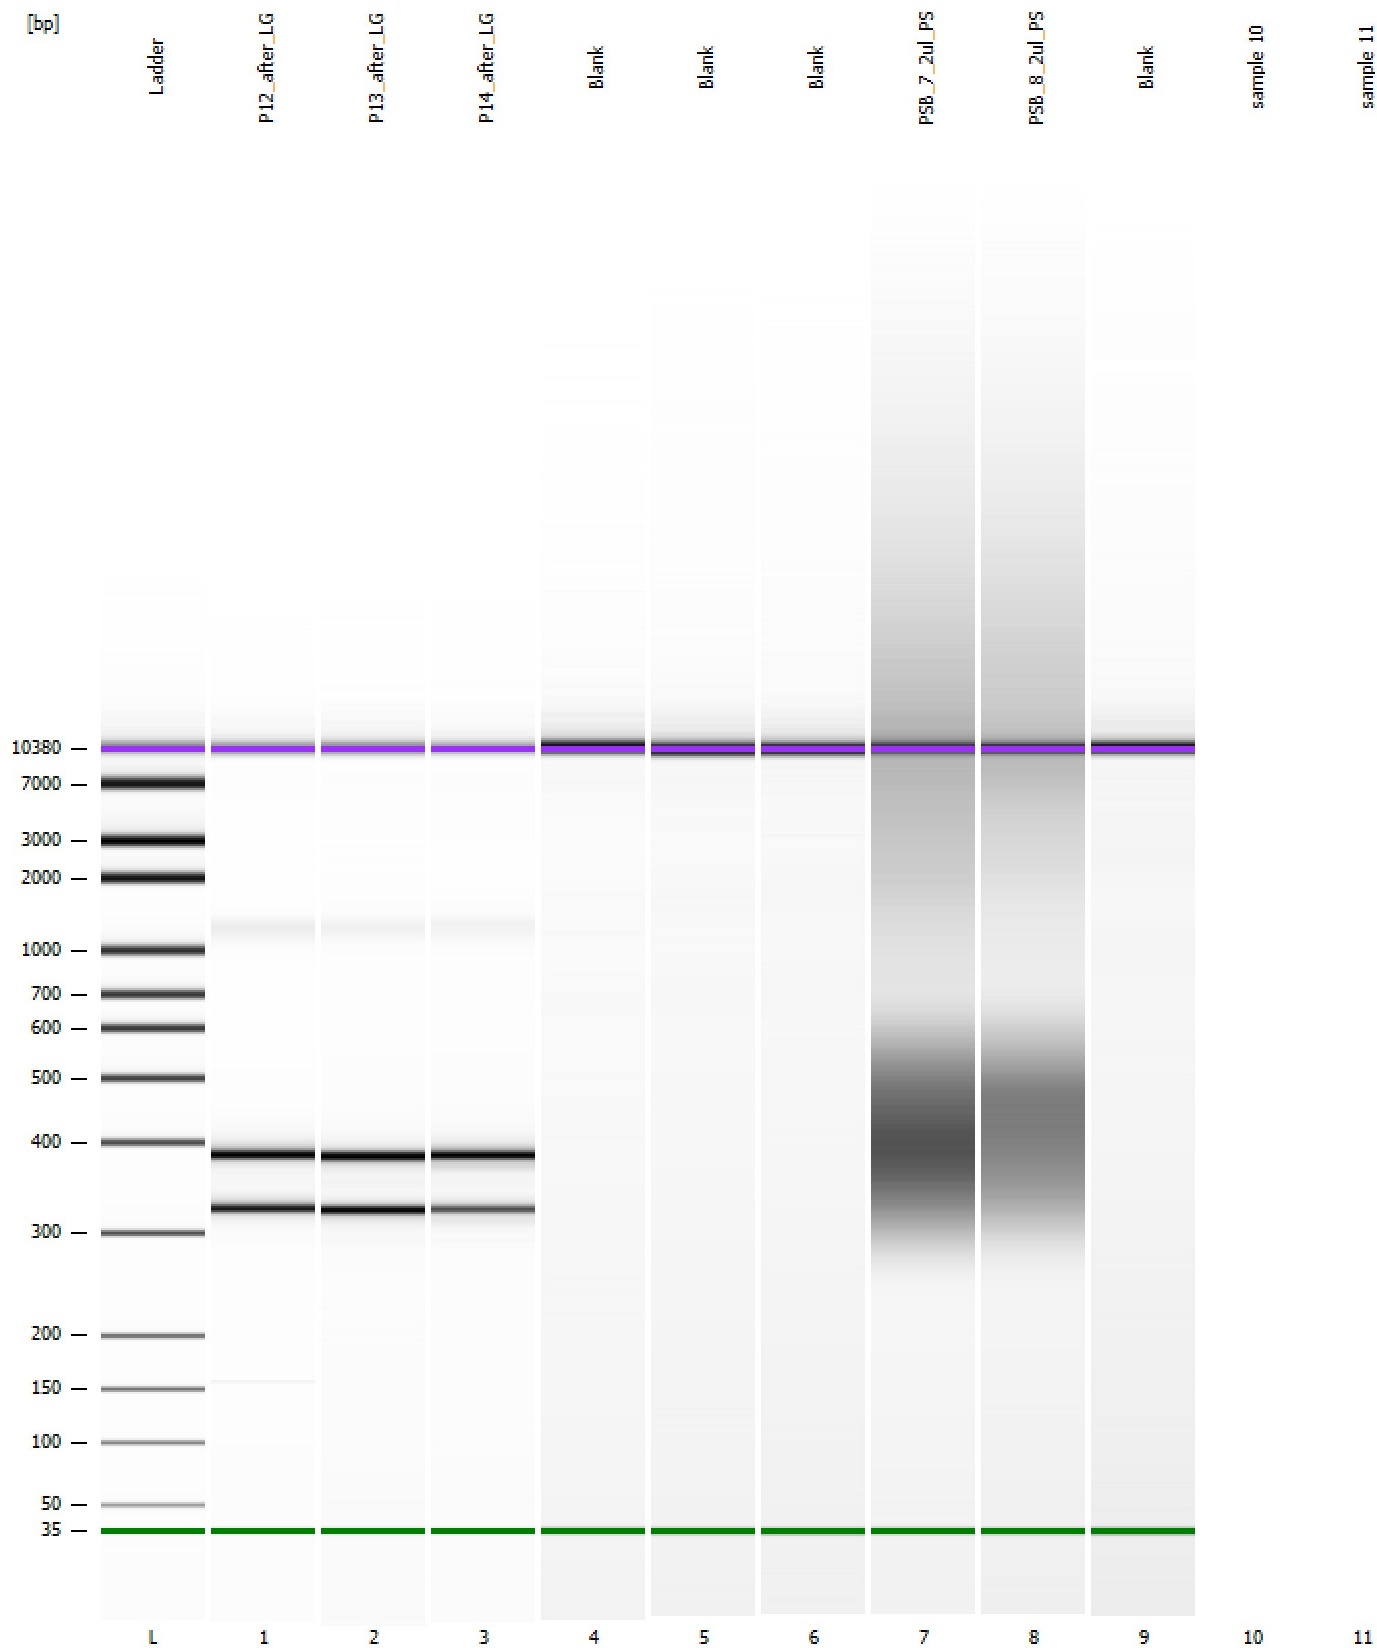
Number of peaks found: 0 Corr. Area 1: 0.7
Noise: 0.3

Region table for sample 9 : Blank

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	0.7	3	951	3.6	0.33	0.5	200	1,000

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

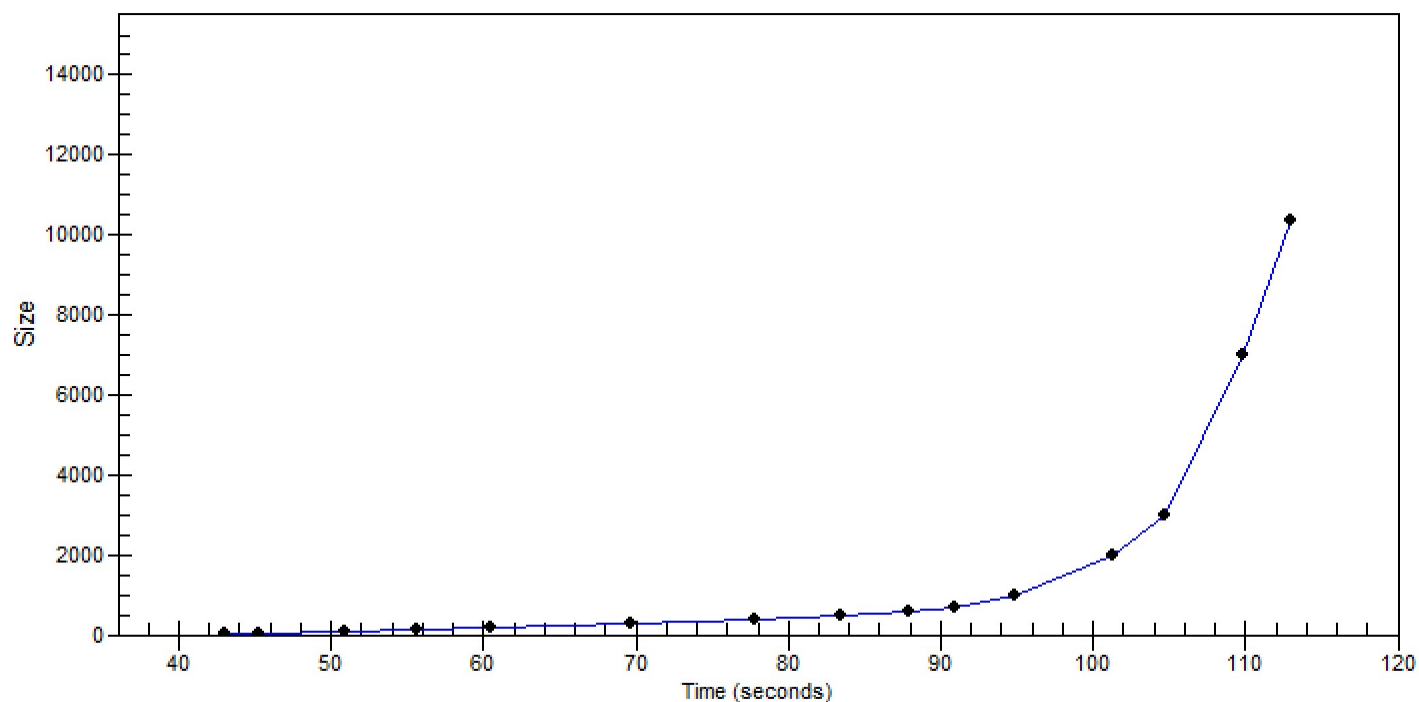
Gel Image

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

Curves

Standard Curve



Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
Modified: 7/17/2026 11:12:42 AM

Invalid Samples

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad

Created: 7/17/2026 10:30:01 AM
 Modified: 7/17/2026 11:12:42 AM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 10)		Instrument	Run		7/17/2026 11:05:37 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\Data\2026-07-17\2100 expert_High Sensitivity DNA Assay_DE54107817_2026-07-17_10-30-02.xad)		Instrument	Run		7/17/2026 10:30:07 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Product Number : G2939A		Instrument	Run		7/17/2026 10:30:07 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Name :		Instrument	Run		7/17/2026 10:30:07 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Vendor : Agilent Technologies		Instrument	Run		7/17/2026 10:30:07 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Serial# : DE54107817		Instrument	Run		7/17/2026 10:30:07 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Firmware : C.01.069		Instrument	Run		7/17/2026 10:30:07 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Cartridge : Electrode		Instrument	Run		7/17/2026 10:30:07 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC