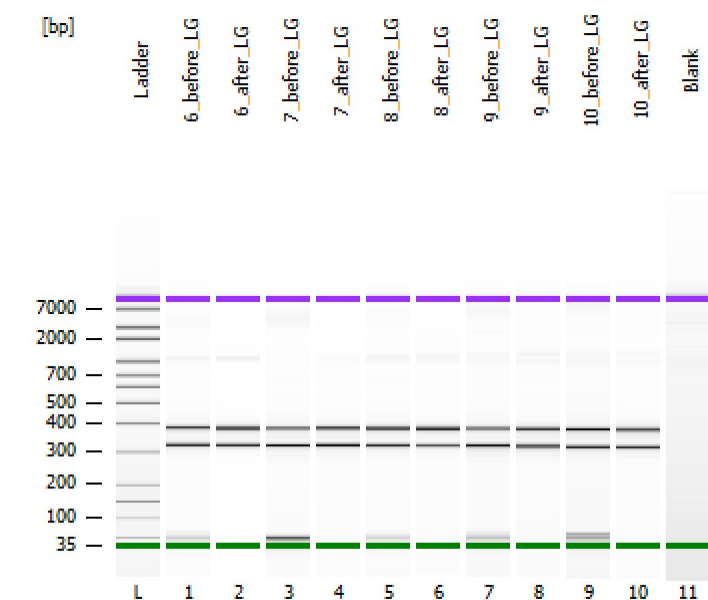


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
Modified: 4/27/2026 3:44:28 PM

Electrophoresis File Run Summary



Instrument Information:

Instrument Name: DE54107817 Firmware: C.01.069
Serial#: DE54107817 Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy

Assay Class: High Sensitivity DNA Assay

Version: 1.03

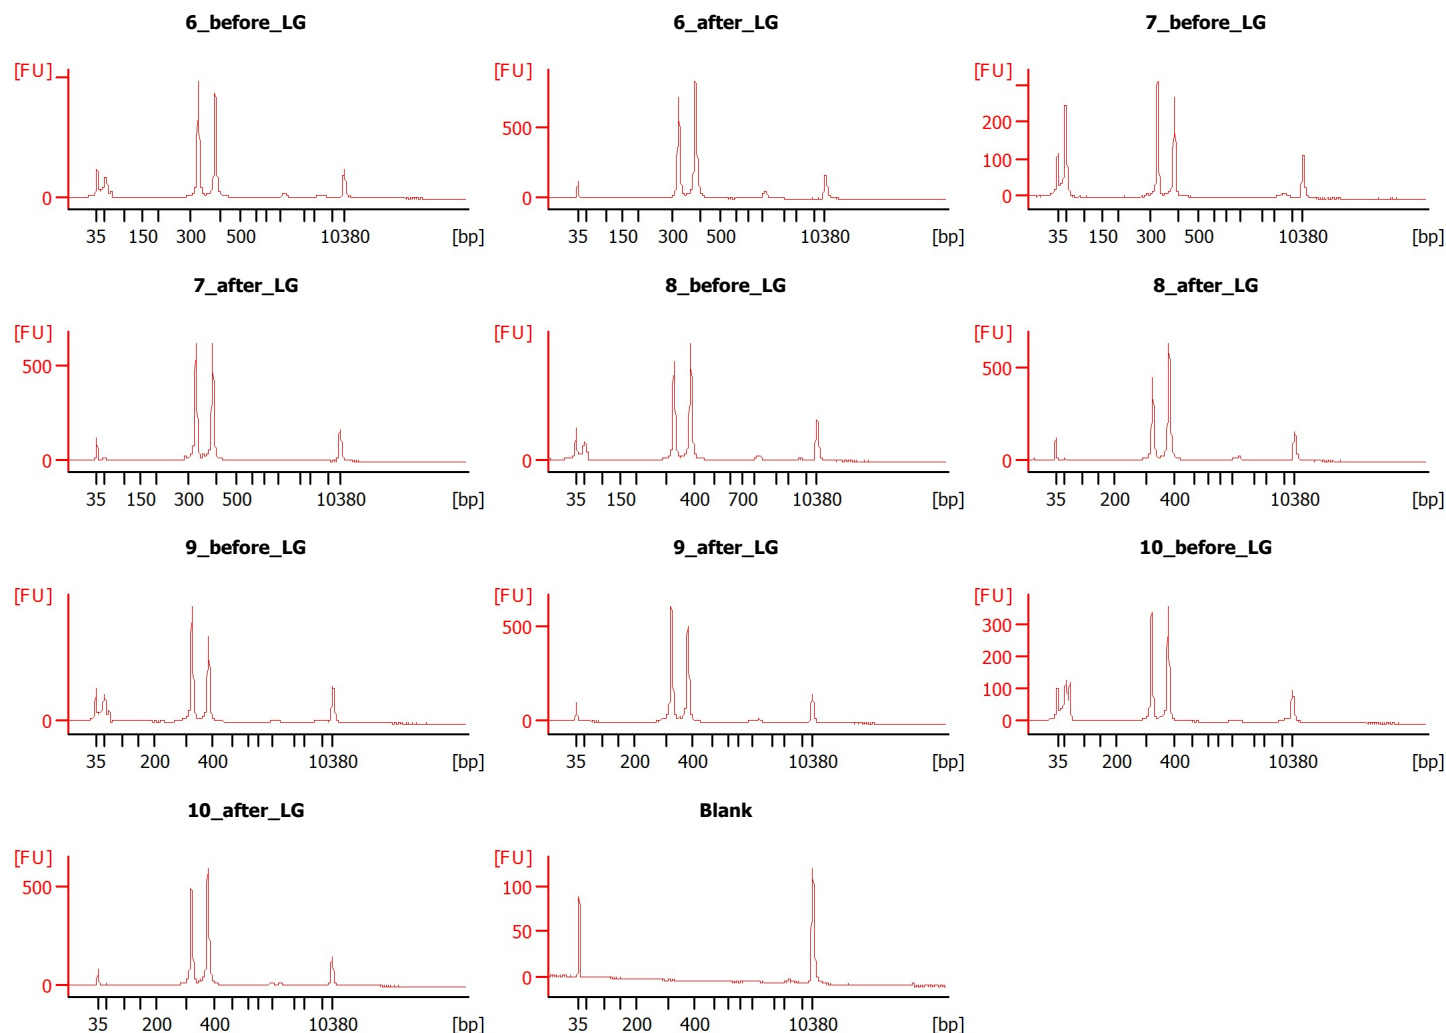
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:



Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
Modified: 4/27/2026 3:44:28 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
6_before_LG		☐	✓			
6_after_LG		☐	✓			
7_before_LG		☐	✓			
7_after_LG		☐	✓			
8_before_LG		☐	✓			
8_after_LG		☐	✓			
9_before_LG		☐	✓			
9_after_LG		☐	✓			
10_before_LG		☐	✓			
10_after_LG		☐	✓			
Blank		☐	✓			
Ladder		☐	✓			
Chip Lot #			Reagent Kit Lot #			

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
Modified: 4/27/2026 3:44:28 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/ μ l] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/ μ l] : 125
Upper Marker Concentration [pg/ μ l] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4

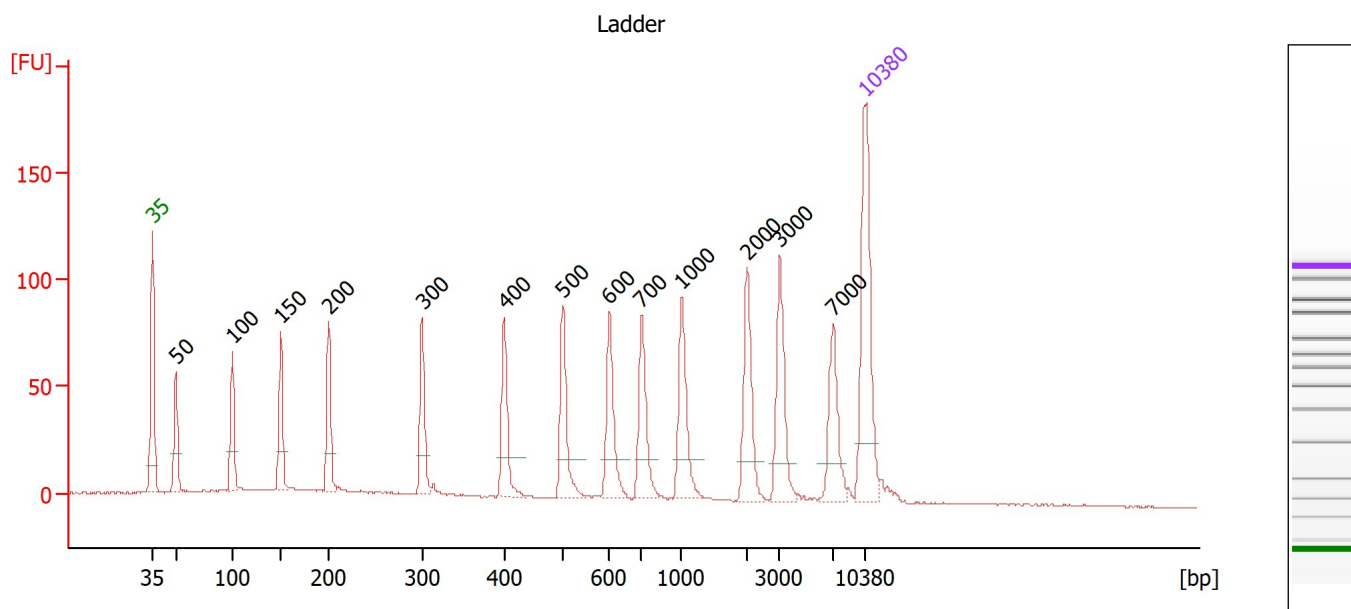
Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary



Overall Results for Ladder

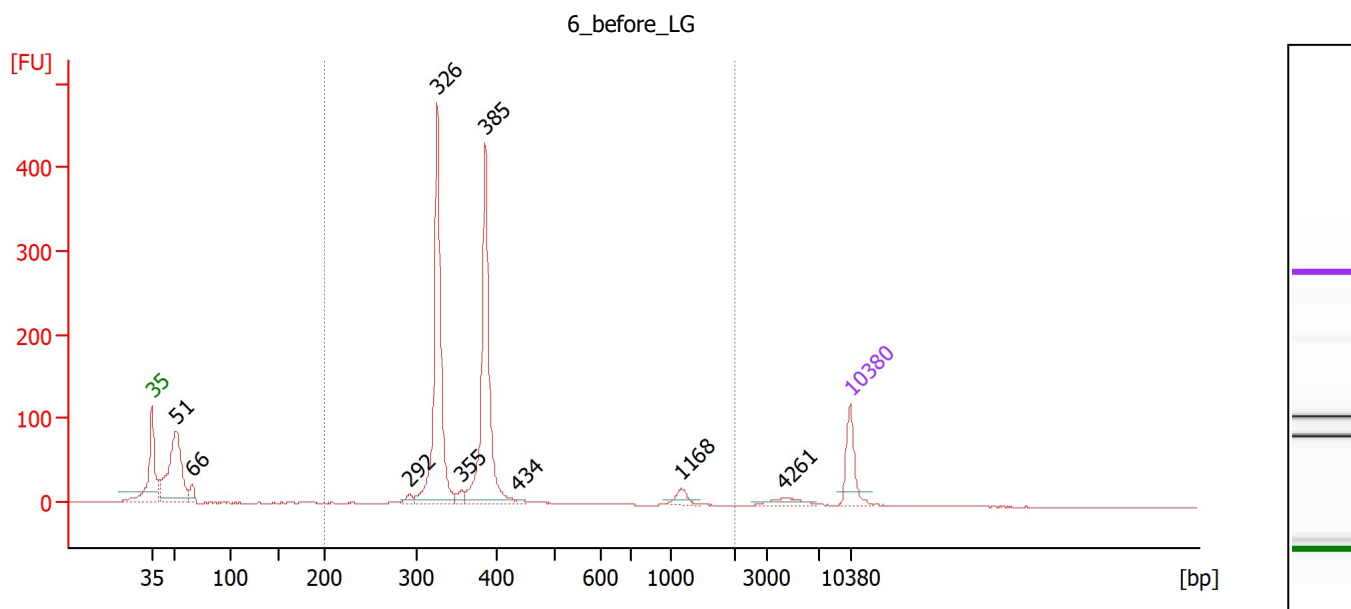
Noise: 0.4

Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 1 : 6 before LG**

Number of peaks found: 9 Corr. Area 1: 1,132.4
 Noise: 0.4

Peak table for sample 1 : 6 before LG

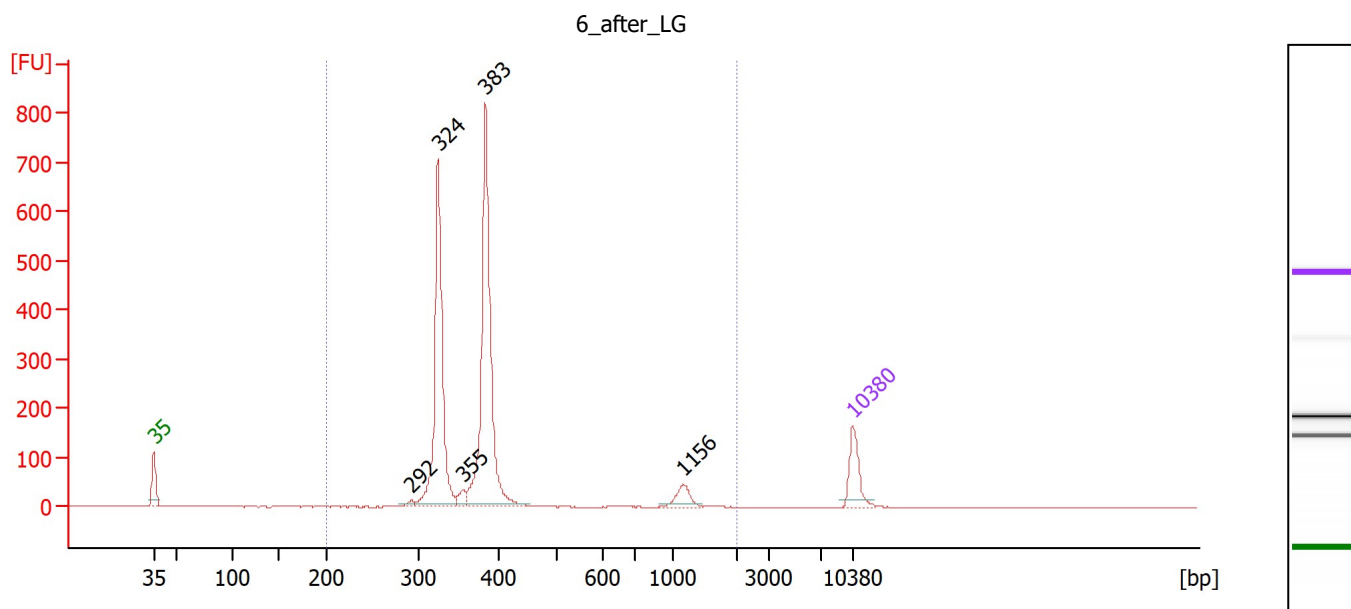
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	51	411.62	12,141.9	
3	66	38.35	883.0	
4	292	14.74	76.4	
5	326	582.92	2,707.5	
6	355	19.53	83.3	
7	385	510.14	2,005.4	
8	434	6.48	22.6	
9	1,168	23.29	30.2	
10	4,261	23.89	8.5	

Region table for sample 1 : 6 before LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,132.4	75	389	42.1	1,188.48	4,977.9	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 2 : 6_after_LG**

Number of peaks found: 5 Corr. Area 1: 2,167.5
 Noise: 0.3

Peak table for sample 2 : 6_after_LG

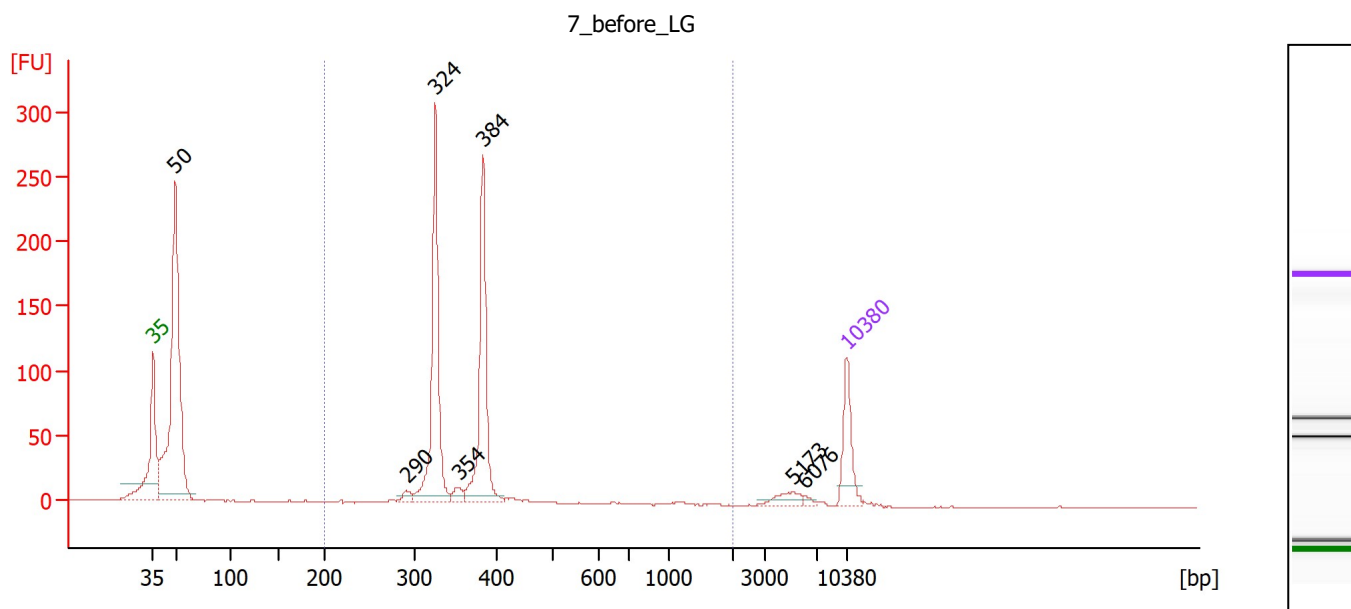
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	292	11.30	58.5	
3	324	611.36	2,855.8	
4	355	26.16	111.8	
5	383	716.13	2,834.3	
6	1,156	40.84	53.5	

Region table for sample 2 : 6_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	2,167.5	99	404	47.5	1,427.50	5,895.6	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 3 : 7_before_LG**

Number of peaks found: 7 Corr. Area 1: 641.6
 Noise: 0.4

Peak table for sample 3 : 7_before_LG

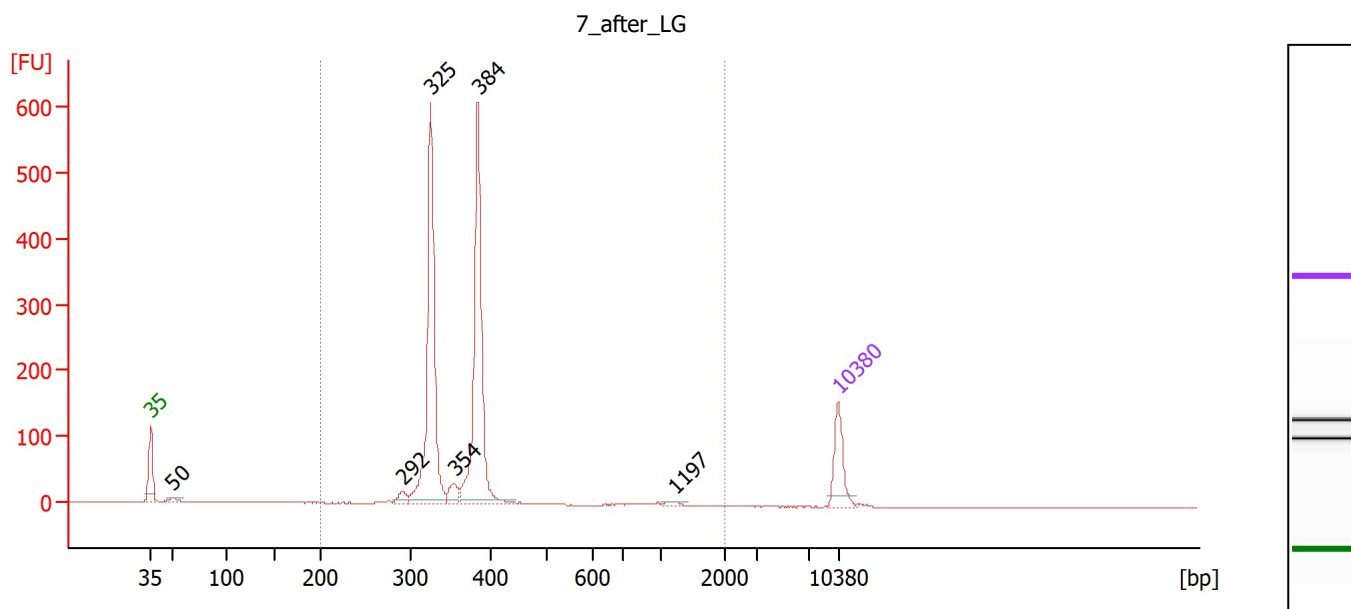
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	50	858.35	26,180.1	
3	290	15.20	79.4	
4	324	376.41	1,758.0	
5	354	19.53	83.5	
6	384	303.94	1,199.3	
7	5,173	23.88	7.0	
8	6,076	5.99	1.5	

Region table for sample 3 : 7_before_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	641.6	52	356	17.5	729.16	3,139.2	 200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 4 : 7_after_LG**

Number of peaks found: 6 Corr. Area 1: 1,526.2
 Noise: 0.2

Peak table for sample 4 : 7_after_LG

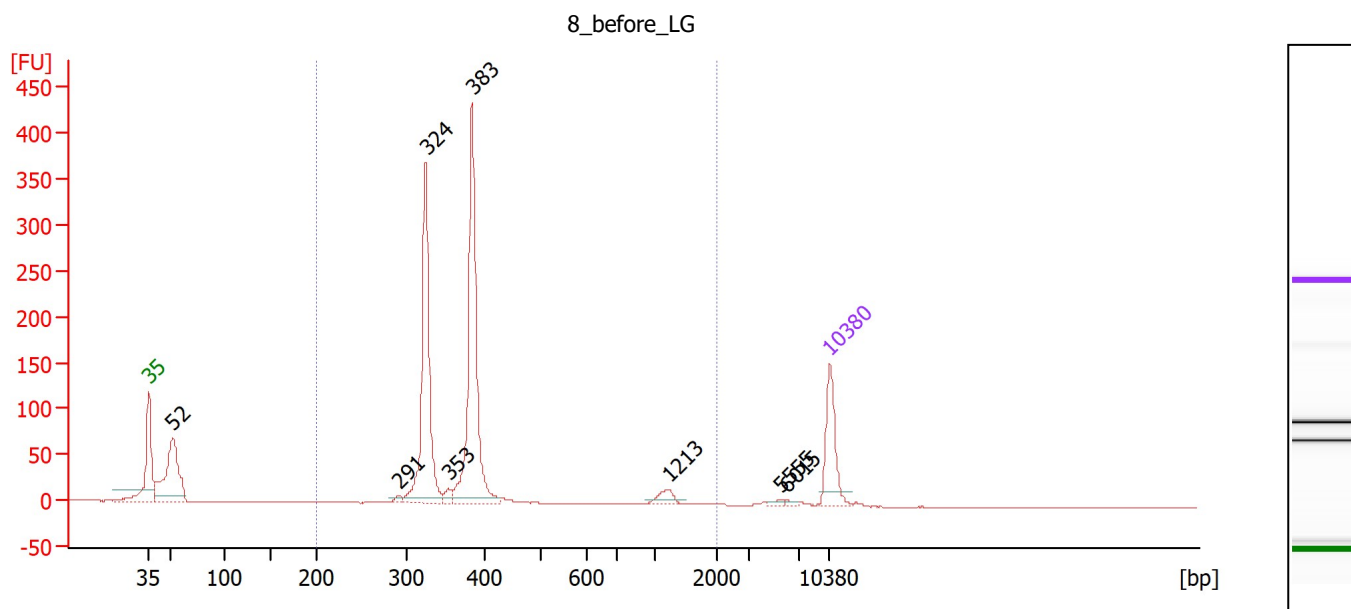
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	50	10.48	316.2	
3	292	22.10	114.8	
4	325	558.05	2,603.9	
5	354	33.34	142.7	
6	384	520.17	2,051.7	
7	1,197	5.86	7.4	

Region table for sample 4 : 7_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,526.2	97	361	22.0	1,143.33	4,883.4	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 5 : 8_before_LG**

Number of peaks found: 8 Corr. Area 1: 1,070.1
 Noise: 0.4

Peak table for sample 5 : 8_before_LG

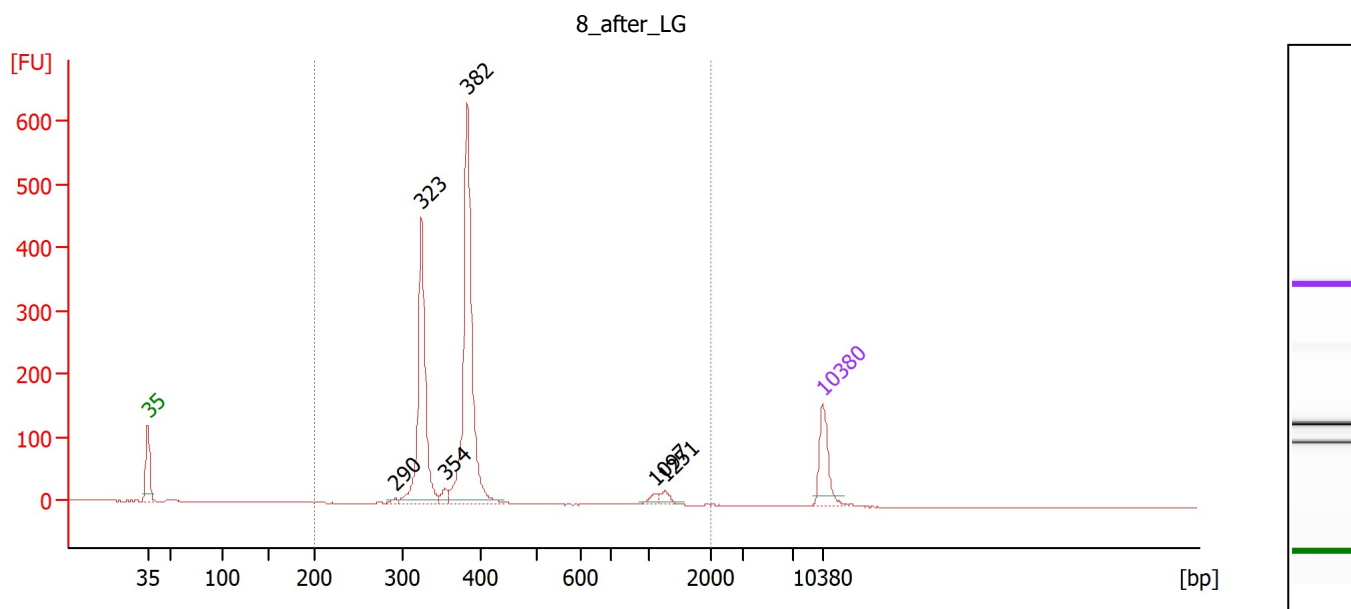
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	52	240.66	7,024.8	
3	291	7.95	41.4	
4	324	347.10	1,622.0	
5	353	13.77	59.1	
6	383	389.45	1,541.0	
7	1,213	17.80	22.2	
8	5,555	4.34	1.2	
9	6,015	3.10	0.8	

Region table for sample 5 : 8_before_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,070.1	81	390	41.8	782.53	3,264.6	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 6 : 8_after_LG**

Number of peaks found: 6 Corr. Area 1: 1,440.2
 Noise: 0.2

Peak table for sample 6 : 8_after_LG

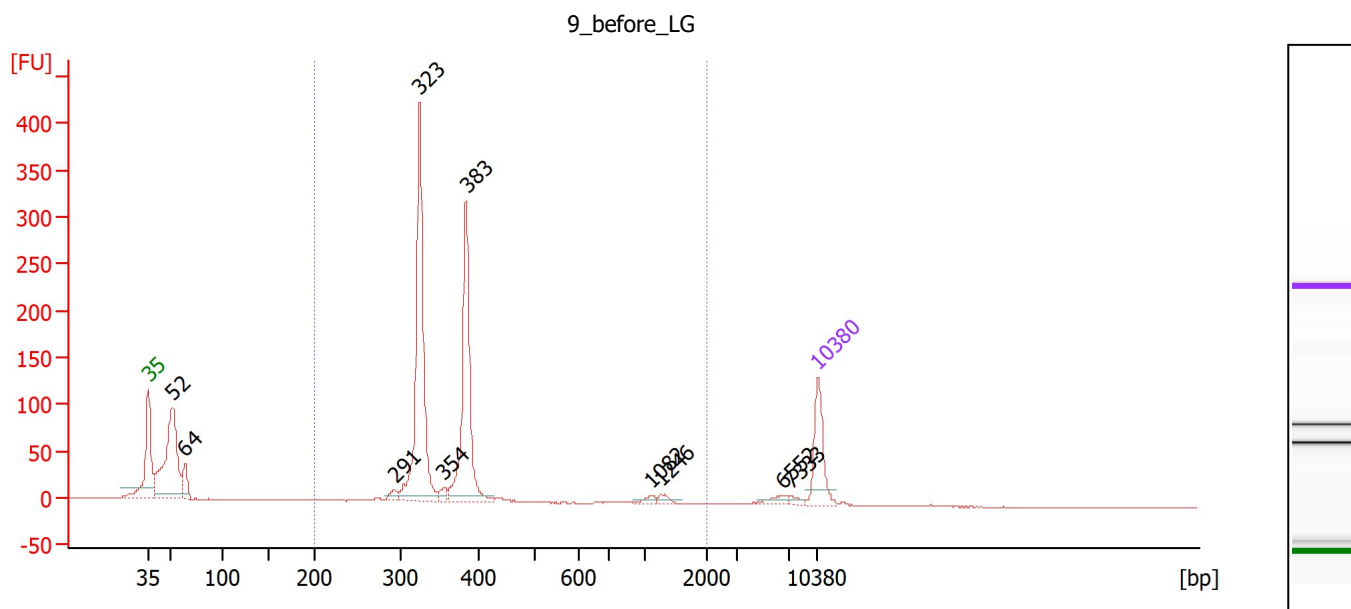
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	290	7.03	36.7	
3	323	414.00	1,940.8	
4	354	19.49	83.5	
5	382	569.84	2,261.9	
6	1,097	10.64	14.7	
7	1,251	14.18	17.2	

Region table for sample 6 : 8_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,440.2	100	393	42.1	1,020.47	4,229.5	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 7 : 9 before LG**

Number of peaks found: 10 Corr. Area 1: 965.9
 Noise: 0.3

Peak table for sample 7 : 9 before LG

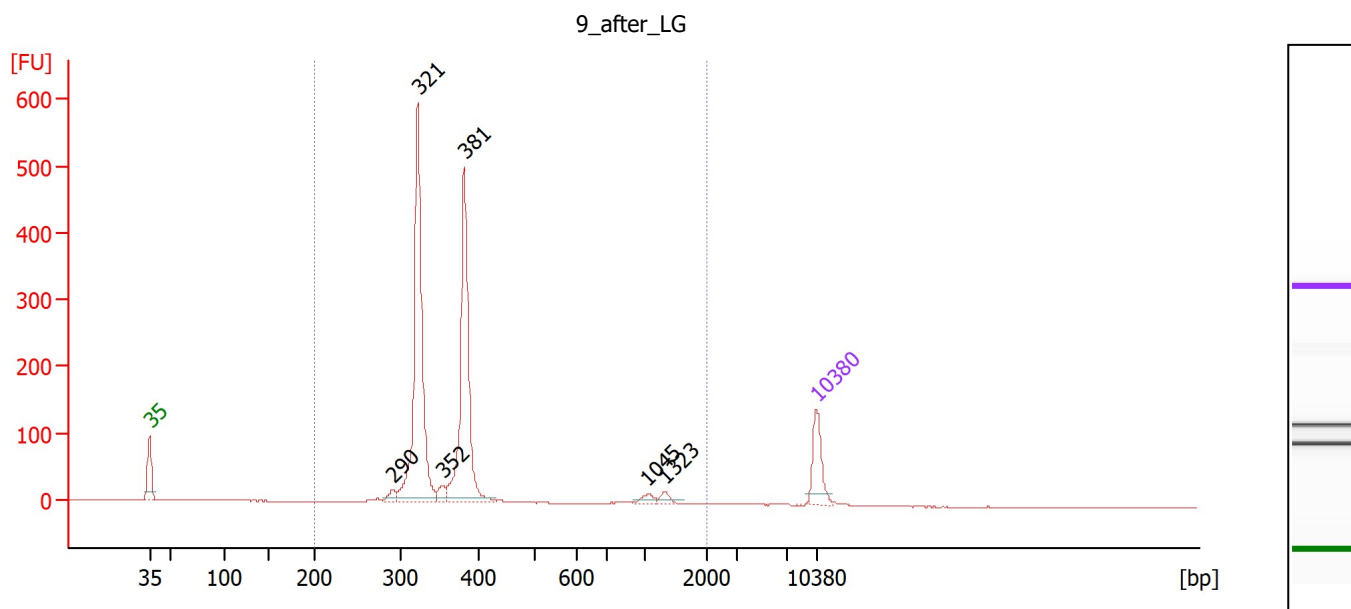
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	52	361.52	10,474.0	
3	64	53.68	1,264.2	
4	291	13.34	69.5	
5	323	449.57	2,110.0	
6	354	13.82	59.2	
7	383	305.69	1,208.6	
8	1,082	8.90	12.5	
9	1,246	8.46	10.3	
10	6,552	11.49	2.7	
11	7,333	6.34	1.3	

Region table for sample 7 : 9 before LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	965.9	71	375	39.8	810.77	3,480.4	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 8 : 9_after_LG**

Number of peaks found: 6 Corr. Area 1: 1,564.5
 Noise: 0.4

Peak table for sample 8 : 9_after_LG

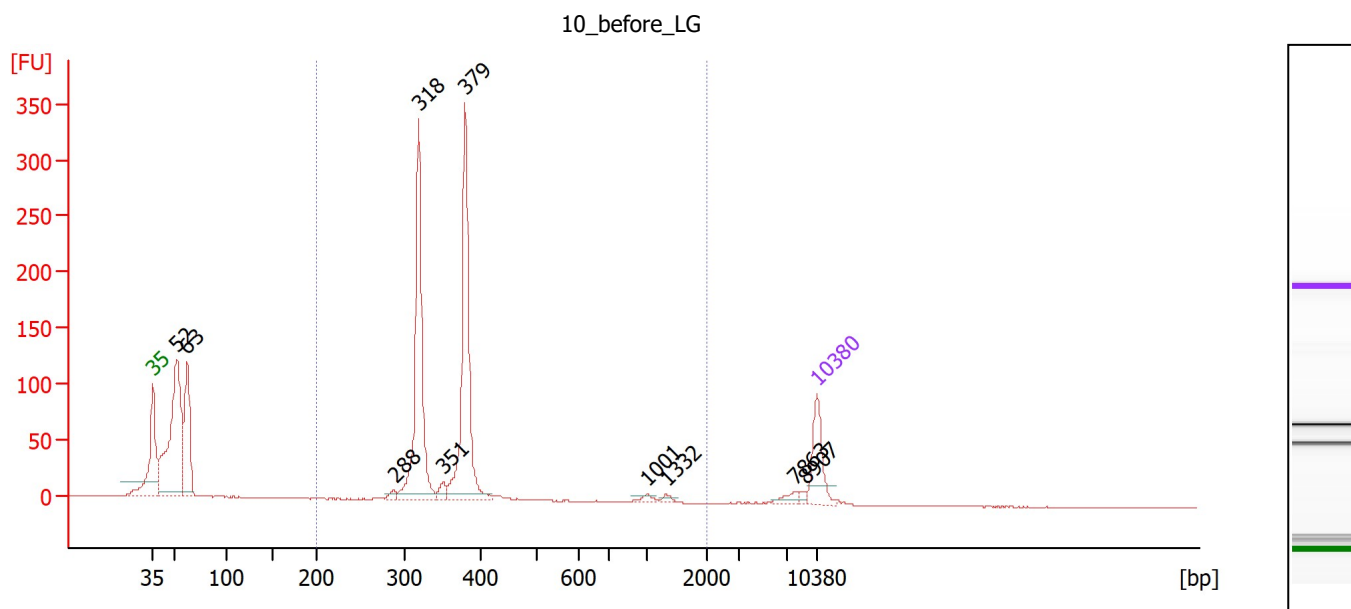
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	290	20.33	106.3	
3	321	654.15	3,089.8	
4	352	23.57	101.3	
5	381	501.13	1,994.3	
6	1,045	15.35	22.3	
7	1,323	13.44	15.4	

Region table for sample 8 : 9_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,564.5	97	387	46.6	1,270.34	5,431.8	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 9 : 10_before_LG**

Number of peaks found: 10 Corr. Area 1: 826.9
 Noise: 0.4

Peak table for sample 9 : 10_before_LG

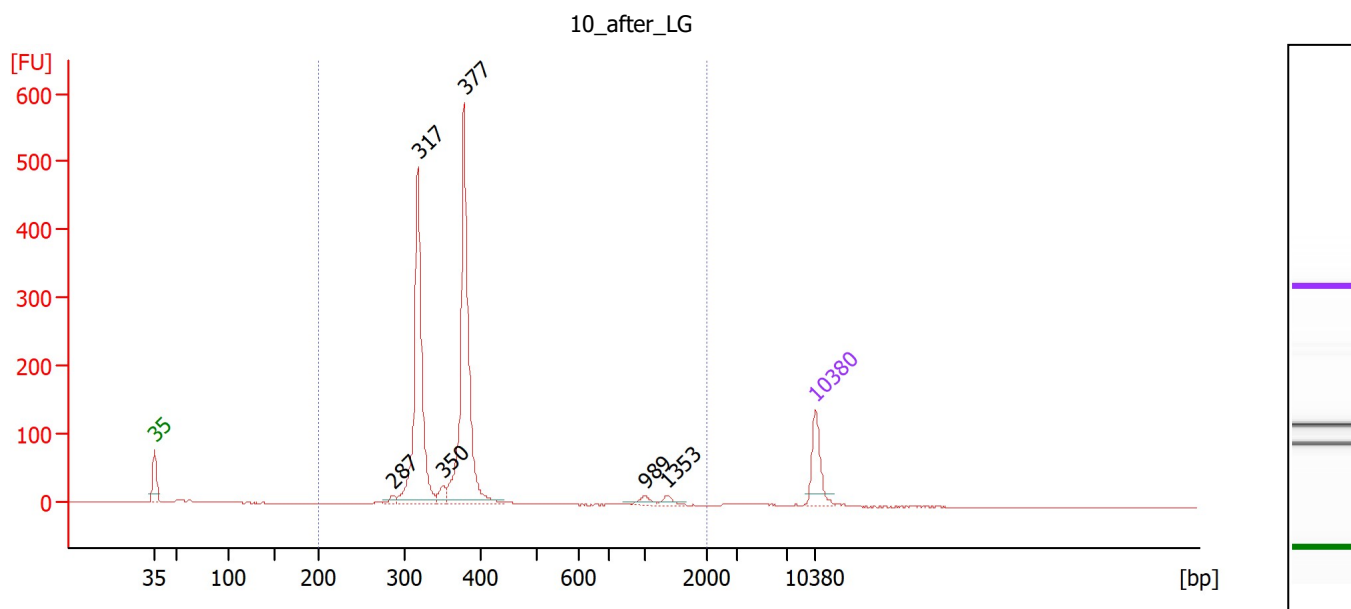
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	52	564.13	16,293.3	
3	63	241.51	5,848.4	
4	288	10.17	53.5	
5	318	435.39	2,071.6	
6	351	18.62	80.4	
7	379	409.79	1,637.1	
8	1,001	9.20	13.9	
9	1,332	6.80	7.7	
10	7,863	13.88	2.7	
11	8,907	5.95	1.0	

Region table for sample 9 : 10_before_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	826.9	59	373	36.3	906.61	3,877.3	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 10 : 10_after_LG**

Number of peaks found: 6 Corr. Area 1: 1,418.5
 Noise: 0.3

Peak table for sample 10 : 10_after_LG

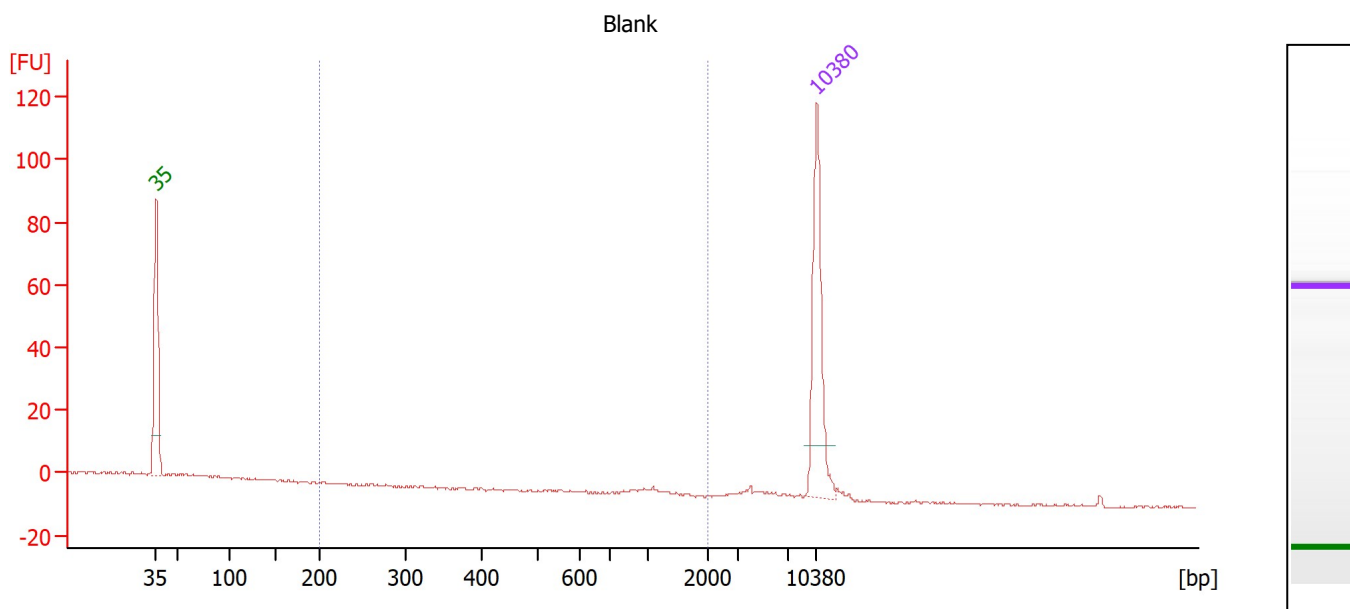
Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	287	13.46	71.2	
3	317	559.48	2,674.9	
4	350	28.84	124.8	
5	377	607.34	2,438.4	
6	989	15.33	23.5	
7	1,353	11.25	12.6	

Region table for sample 10 : 10_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,418.5	98	382	42.5	1,236.73	5,259.3	200	2,000

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
Modified: 4/27/2026 3:44:28 PM

Electropherogram Summary Continued ...**Overall Results for sample 11 : Blank**

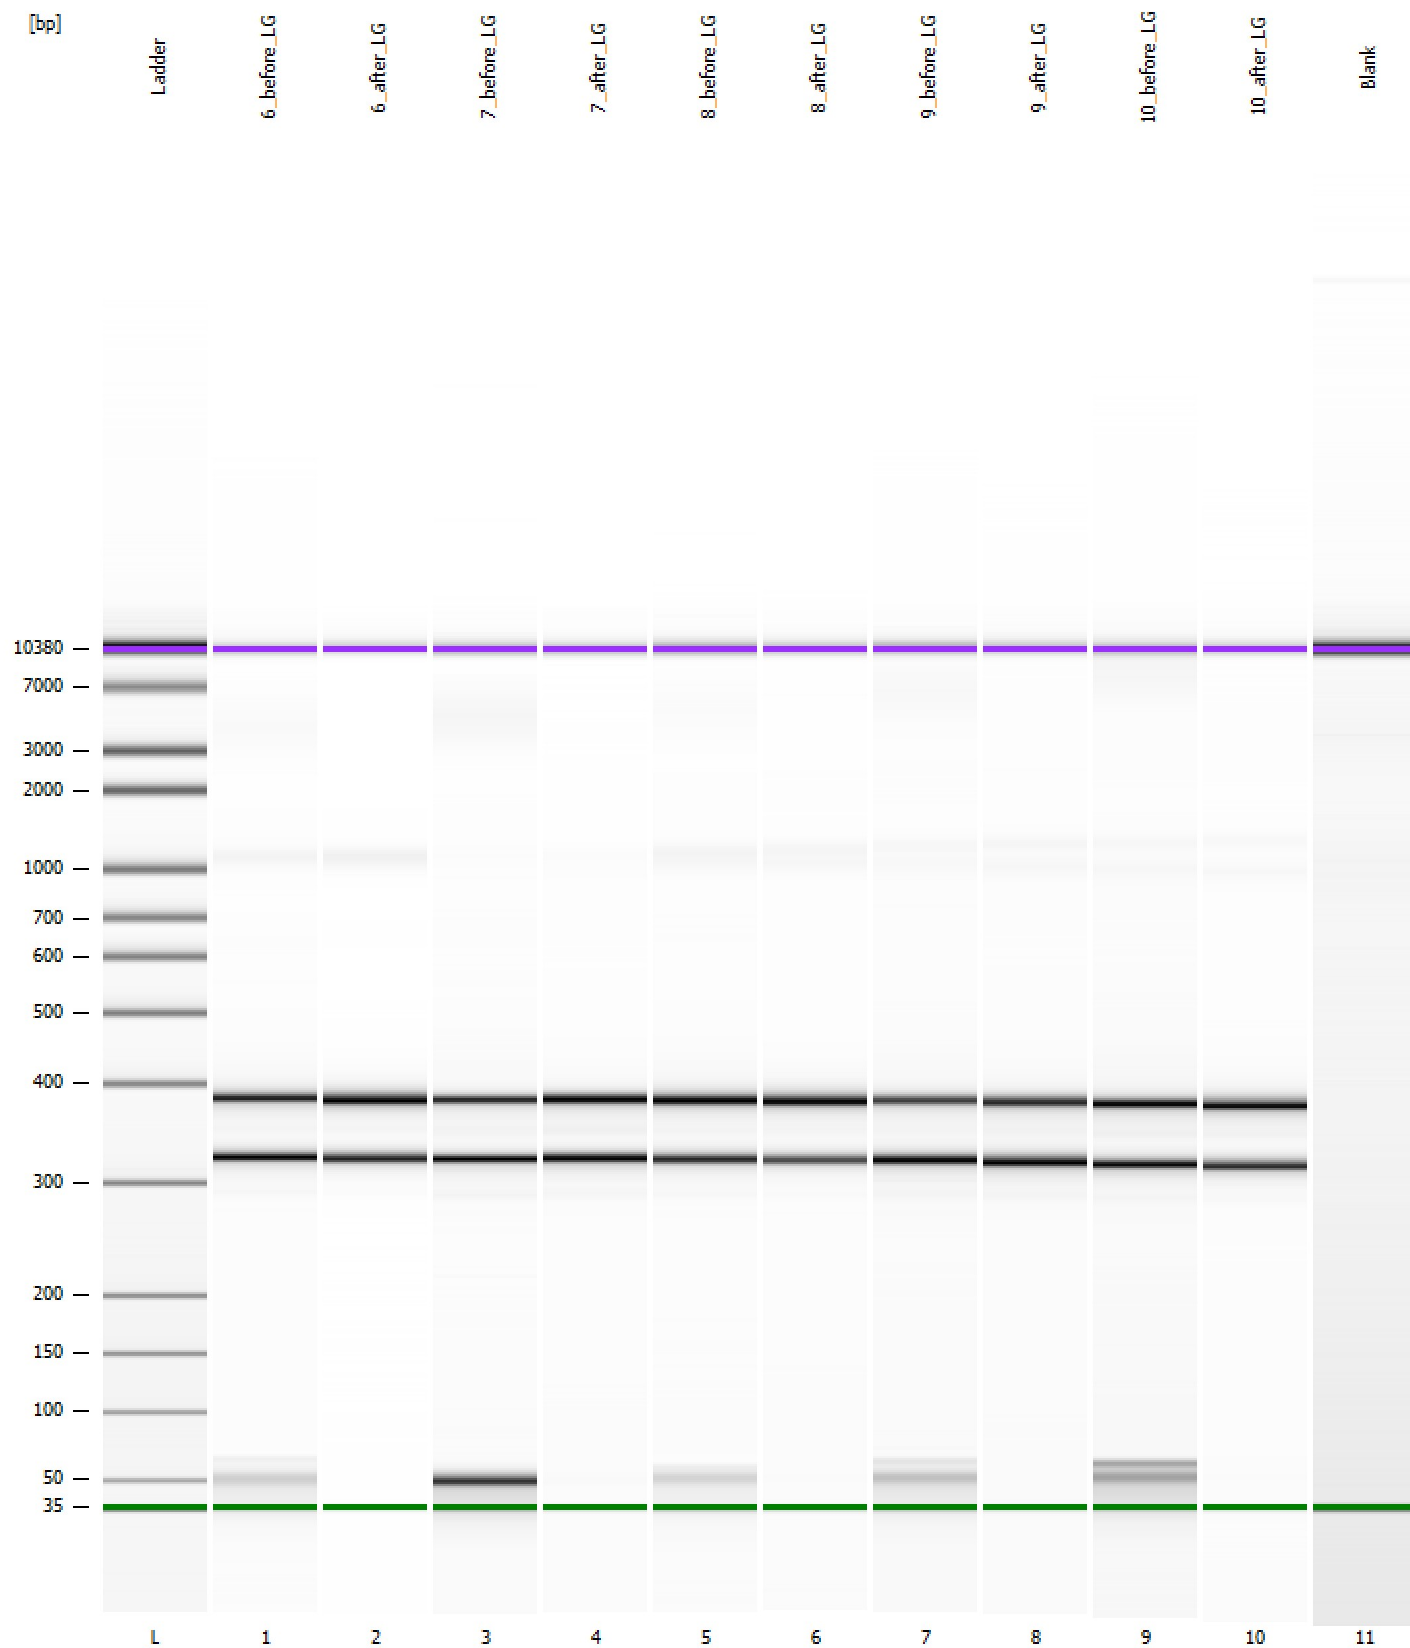
Number of peaks found: 0 Corr. Area 1: 0.6
Noise: 0.4

Region table for sample 11 : Blank

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	0.6	7	1,043	6.4	0.47	0.7	200	2,000

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
Modified: 4/27/2026 3:44:28 PM

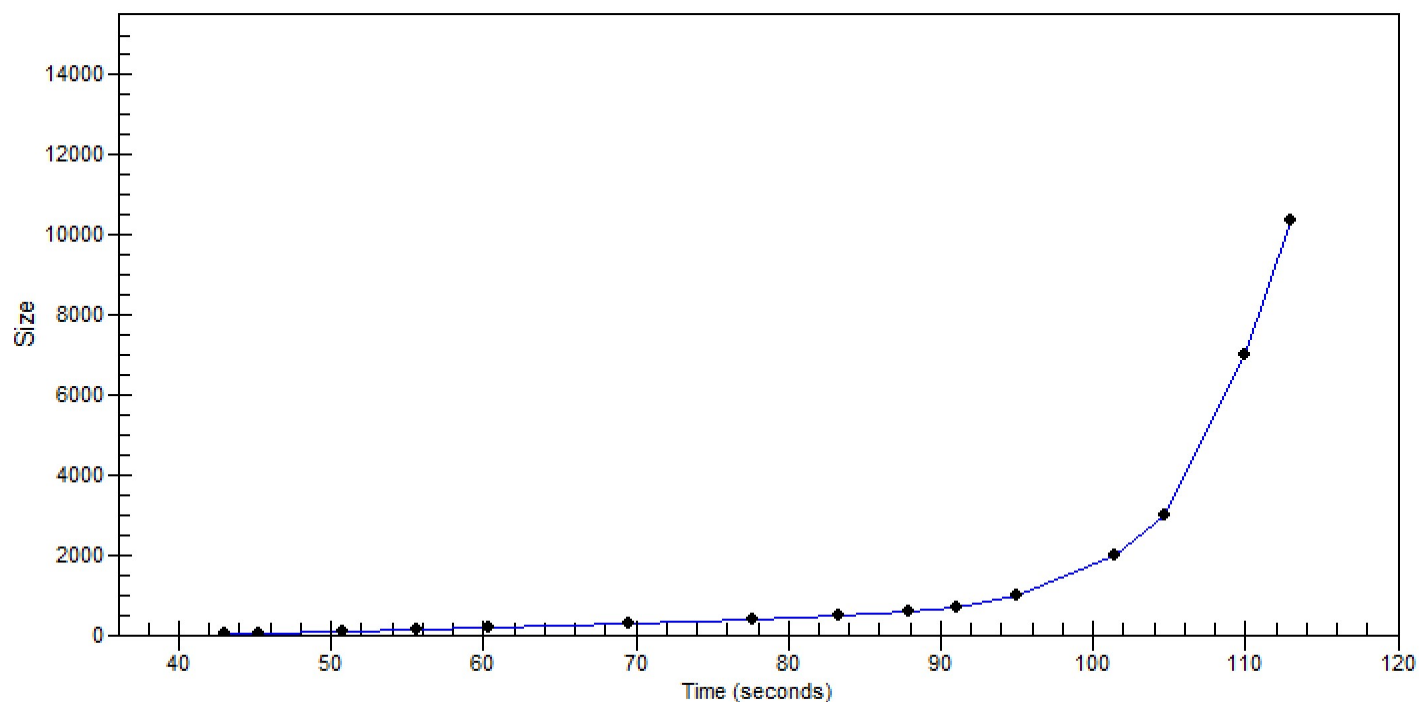
Gel Image

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
Modified: 4/27/2026 3:44:28 PM

Curves

Standard Curve



Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad

Created: 4/27/2026 3:00:11 PM
 Modified: 4/27/2026 3:44:28 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		4/27/2026 3:41:31 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\Data\2026-04-27\2100 expert_High Sensitivity DNA Assay_DE54107817_2026-04-27_15-00-11.xad)		Instrument	Run		4/27/2026 3:00:17 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Product Number : G2939A		Instrument	Run		4/27/2026 3:00:17 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Name :		Instrument	Run		4/27/2026 3:00:17 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Vendor : Agilent Technologies		Instrument	Run		4/27/2026 3:00:17 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Serial# : DE54107817		Instrument	Run		4/27/2026 3:00:17 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Firmware : C.01.069		Instrument	Run		4/27/2026 3:00:17 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Cartridge : Electrode		Instrument	Run		4/27/2026 3:00:17 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC