


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
Modified: 4/28/2026 2:01:44 PM

Electrophoresis File Run Summary

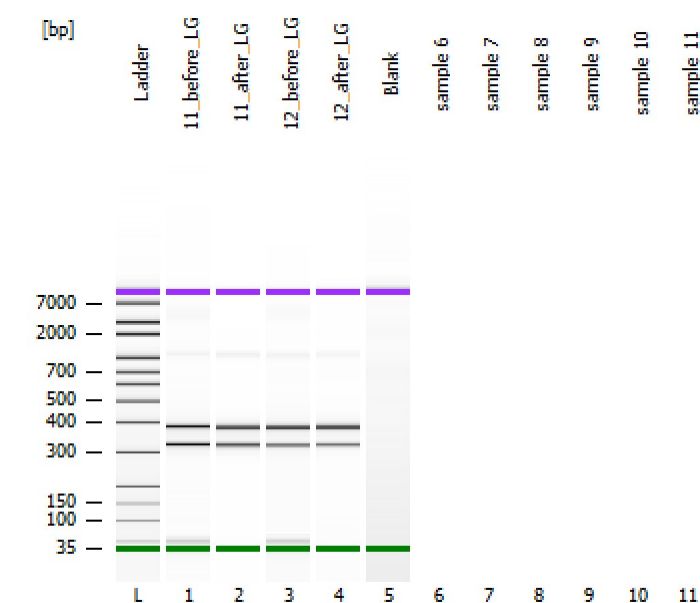

Instrument Information:


Instrument Name: DE54107817
Serial#: DE54107817
Firmware: C.01.069
Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

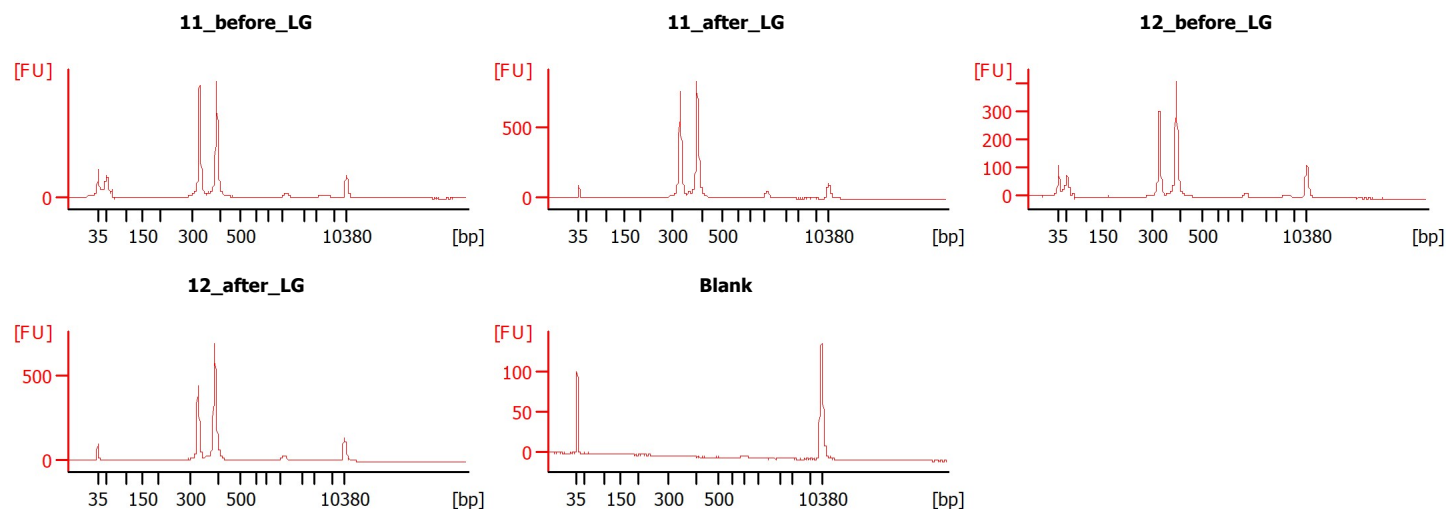

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
Modified: 4/28/2026 2:01:44 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
11_before_LG		☐	✓			
11_after_LG		☐	✓			
12_before_LG		☐	✓			
12_after_LG		☐	✓			
Blank		☐	✓			
sample 6		☐				
sample 7		☐				
sample 8		☐				
sample 9		☐				
sample 10		☐				
sample 11		☐				
Ladder		☐	✓			
Chip Lot #			Reagent Kit Lot #			

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
Modified: 4/28/2026 2:01:44 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
 Modified: 4/28/2026 2:01:44 PM

Electropherogram Summary

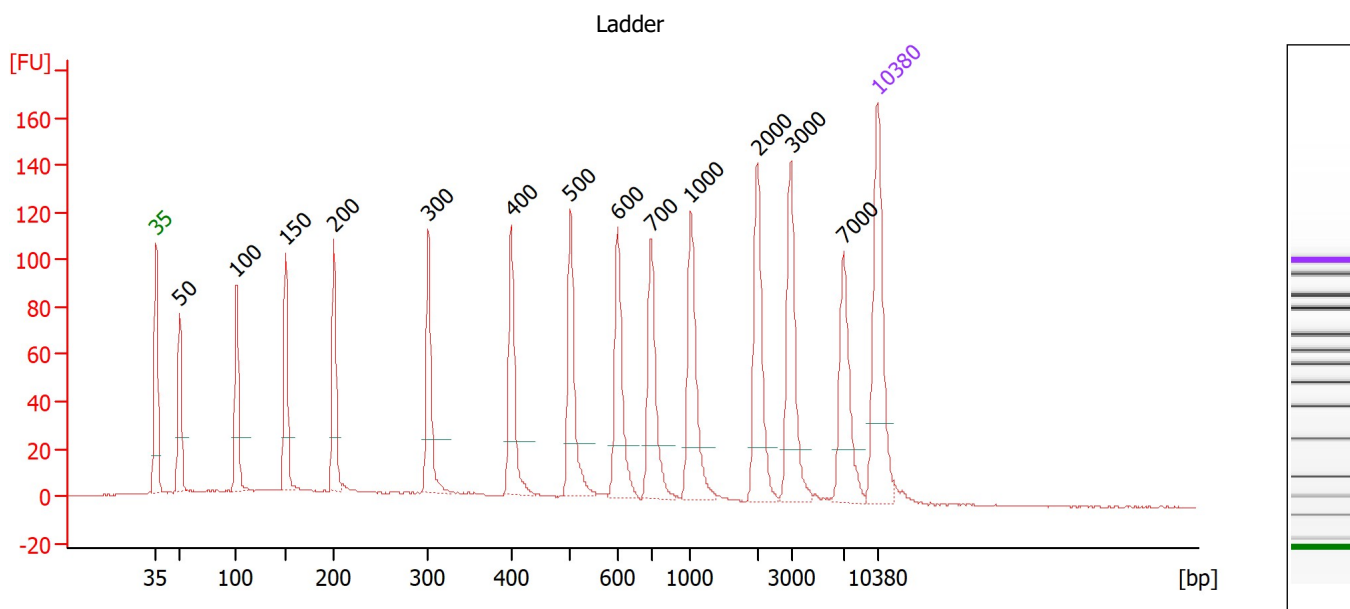

Overall Results for Ladder


Noise: 0.3

Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
 Modified: 4/28/2026 2:01:44 PM

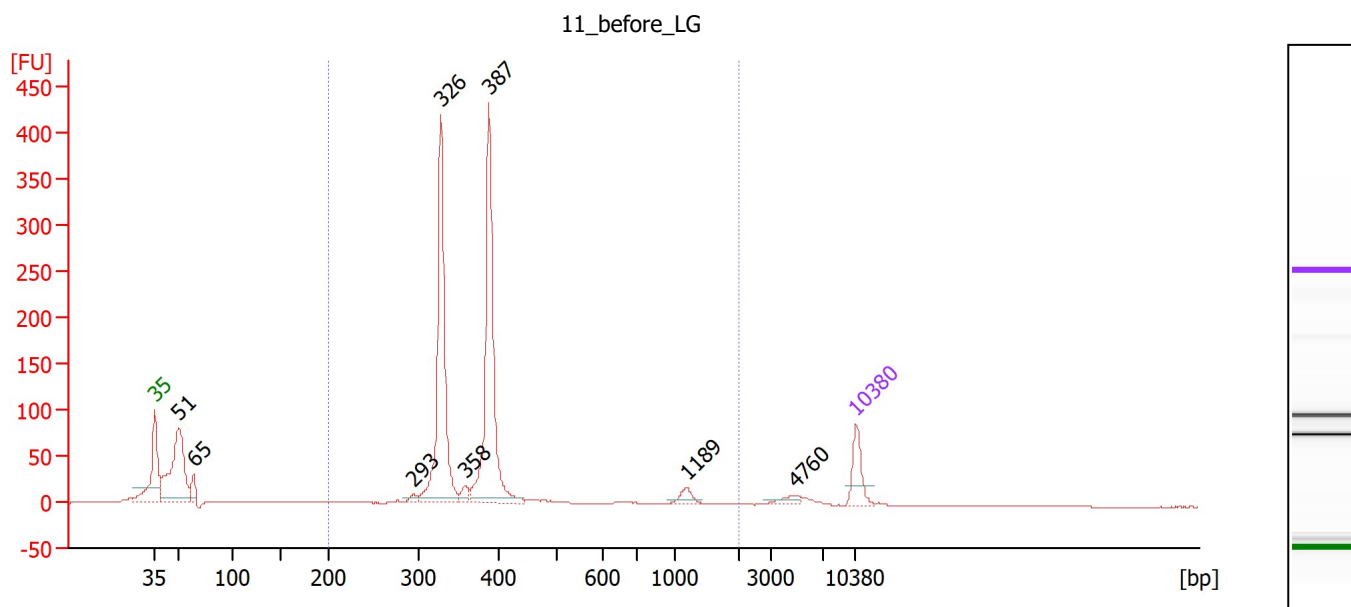Electropherogram Summary Continued ...**Overall Results for sample 1 : 11_before_LG**

Number of peaks found: 8 Corr. Area 1: 1,134.2
 Noise: 0.3

Peak table for sample 1 : 11_before_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	51	533.91	15,833.7	
3	65	63.18	1,482.7	
4	293	17.66	91.2	
5	326	714.74	3,318.0	
6	358	29.48	124.9	
7	387	707.81	2,772.3	
8	1,189	26.83	34.2	
9	4,760	19.02	6.1	


Region table for sample 1 : 11_before_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,134.2	74	397	45.3	1,590.47	6,604.6	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
 Modified: 4/28/2026 2:01:44 PM

Electropherogram Summary Continued ...

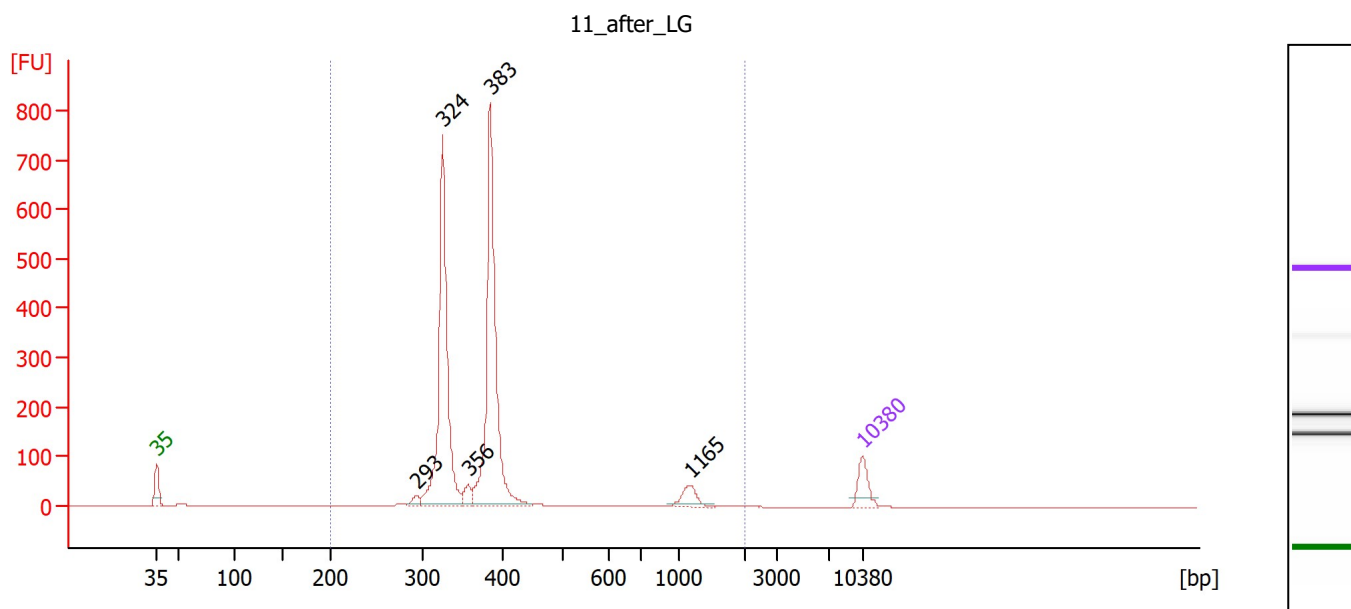

Overall Results for sample 2 : 11_after_LG

Number of peaks found: 5 Corr. Area 1: 2,290.3
 Noise: 0.4

Peak table for sample 2 : 11_after_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	293	31.23	161.7	
3	324	1,064.54	4,978.7	
4	356	52.75	224.7	
5	383	1,078.02	4,260.8	
6	1,165	63.48	82.5	

Region table for sample 2 : 11_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	2,290.3	98	399	47.0	2,337.43	9,733.8	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
 Modified: 4/28/2026 2:01:44 PM

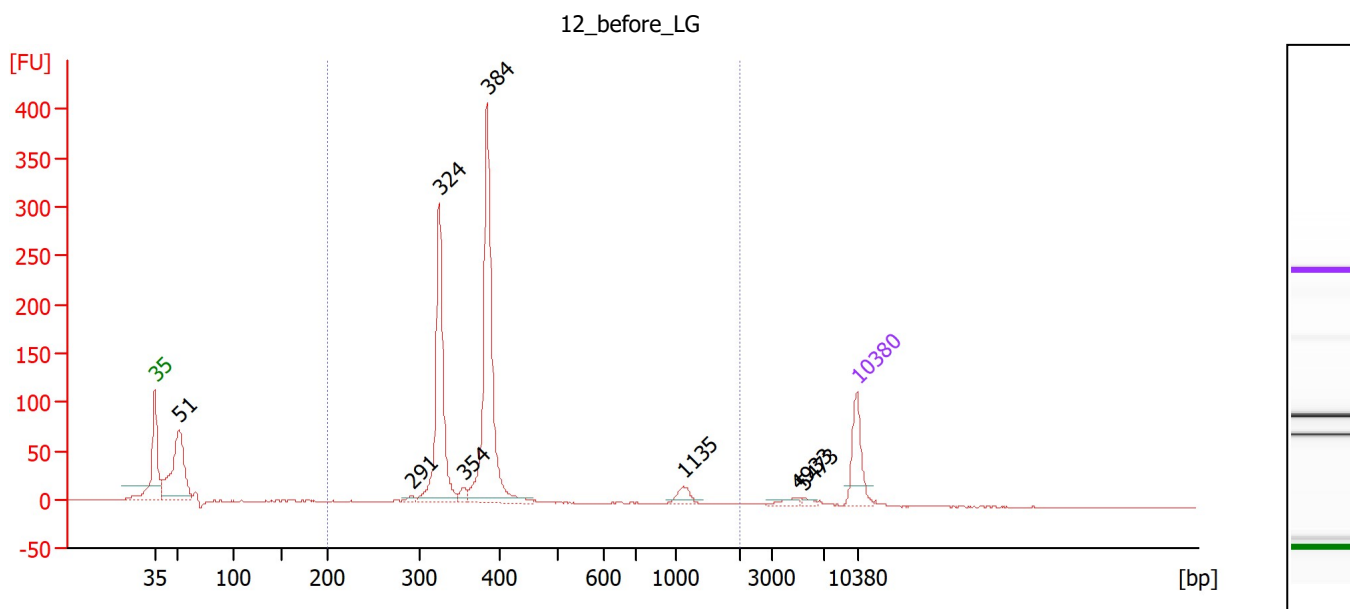Electropherogram Summary Continued ...**Overall Results for sample 3 : 12_before_LG**

Number of peaks found: 8 Corr. Area 1: 967.8
 Noise: 0.3

Peak table for sample 3 : 12_before_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	51	334.29	9,920.0	
3	291	9.23	48.1	
4	324	388.13	1,815.9	
5	354	18.09	77.4	
6	384	519.88	2,053.7	
7	1,135	24.00	32.0	
8	4,933	10.54	3.2	
9	5,473	6.43	1.8	

Region table for sample 3 : 12_before_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	967.8	77	396	42.7	973.70	4,019.5	200	2,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
 Modified: 4/28/2026 2:01:44 PM

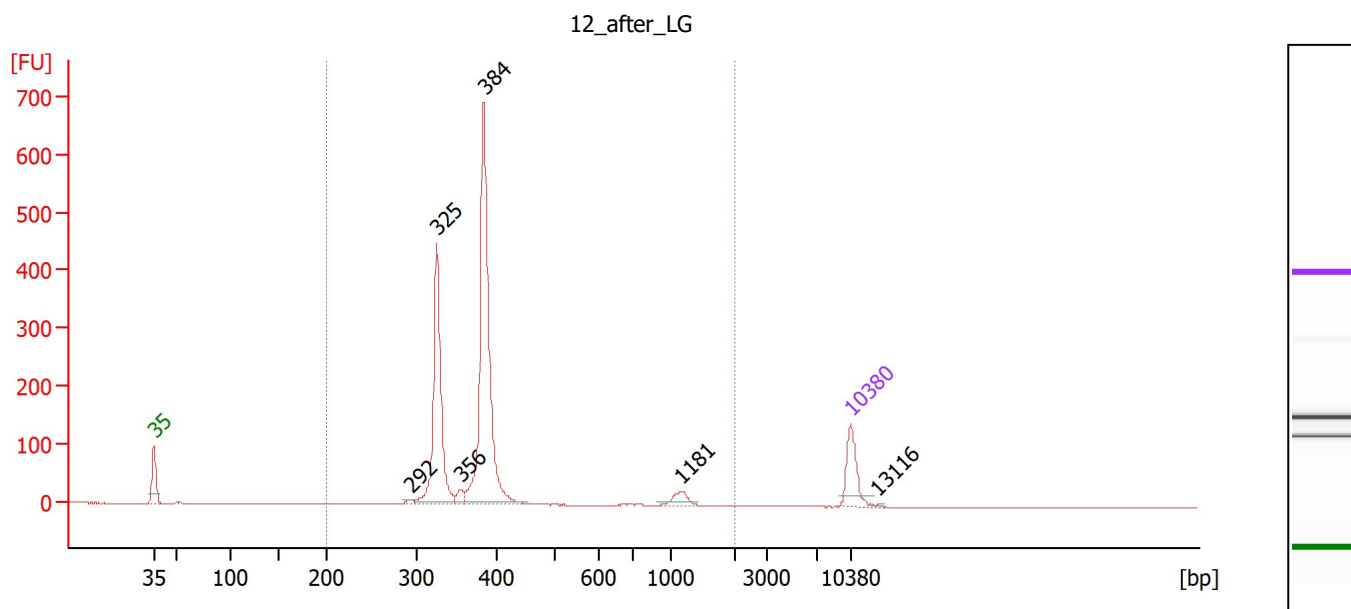Electropherogram Summary Continued ...**Overall Results for sample 4 : 12_after_LG**

Number of peaks found: 6 Corr. Area 1: 1,584.5
 Noise: 0.3

Peak table for sample 4 : 12_after_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	292	6.49	33.6	
3	325	436.90	2,035.4	
4	356	22.52	95.8	
5	384	688.84	2,717.7	
6	1,181	24.46	31.4	
8	13,116	0.00	0.0	

Region table for sample 4 : 12_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,584.4	100	394	39.7	1,190.27	4,877.6	200	2,000

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
Modified: 4/28/2026 2:01:44 PM

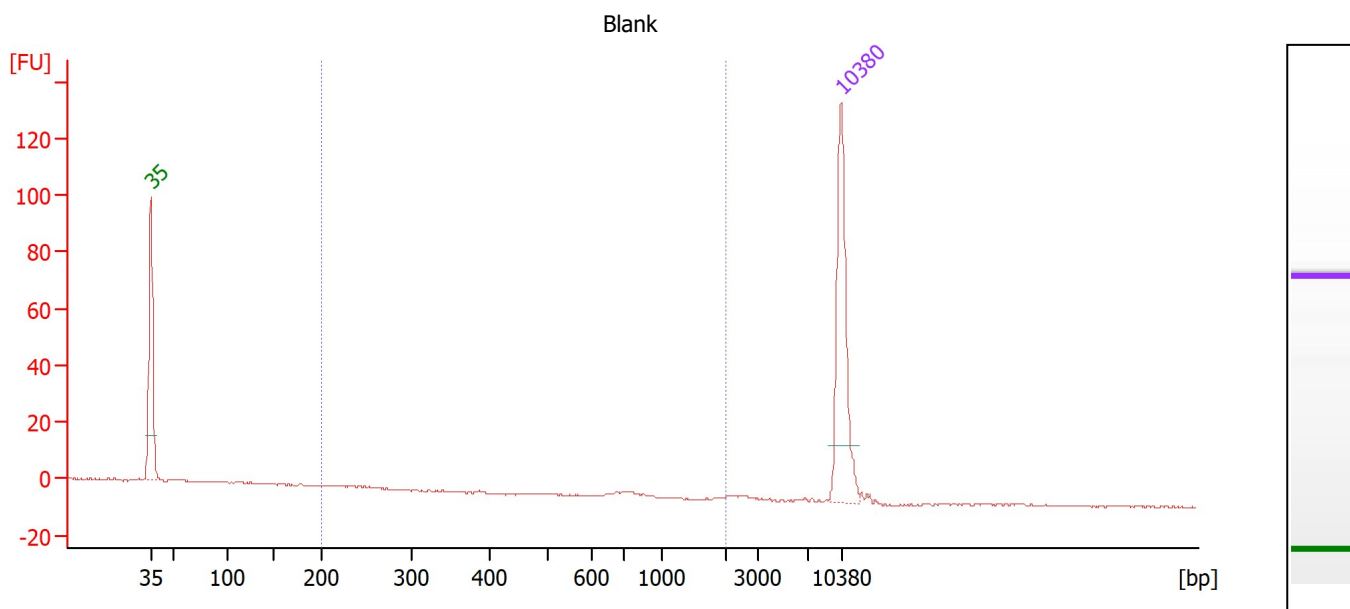Electropherogram Summary Continued ...**Overall Results for sample 5 : Blank**

Number of peaks found: 0 Corr. Area 1: 0.7
Noise: 0.3

Region table for sample 5 : Blank

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	0.7	8	723	6.4	0.51	1.1	200	2,000


Assay Class: High Sensitivity DNA Assay

Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM

Modified: 4/28/2026 2:01:44 PM

Gel Image

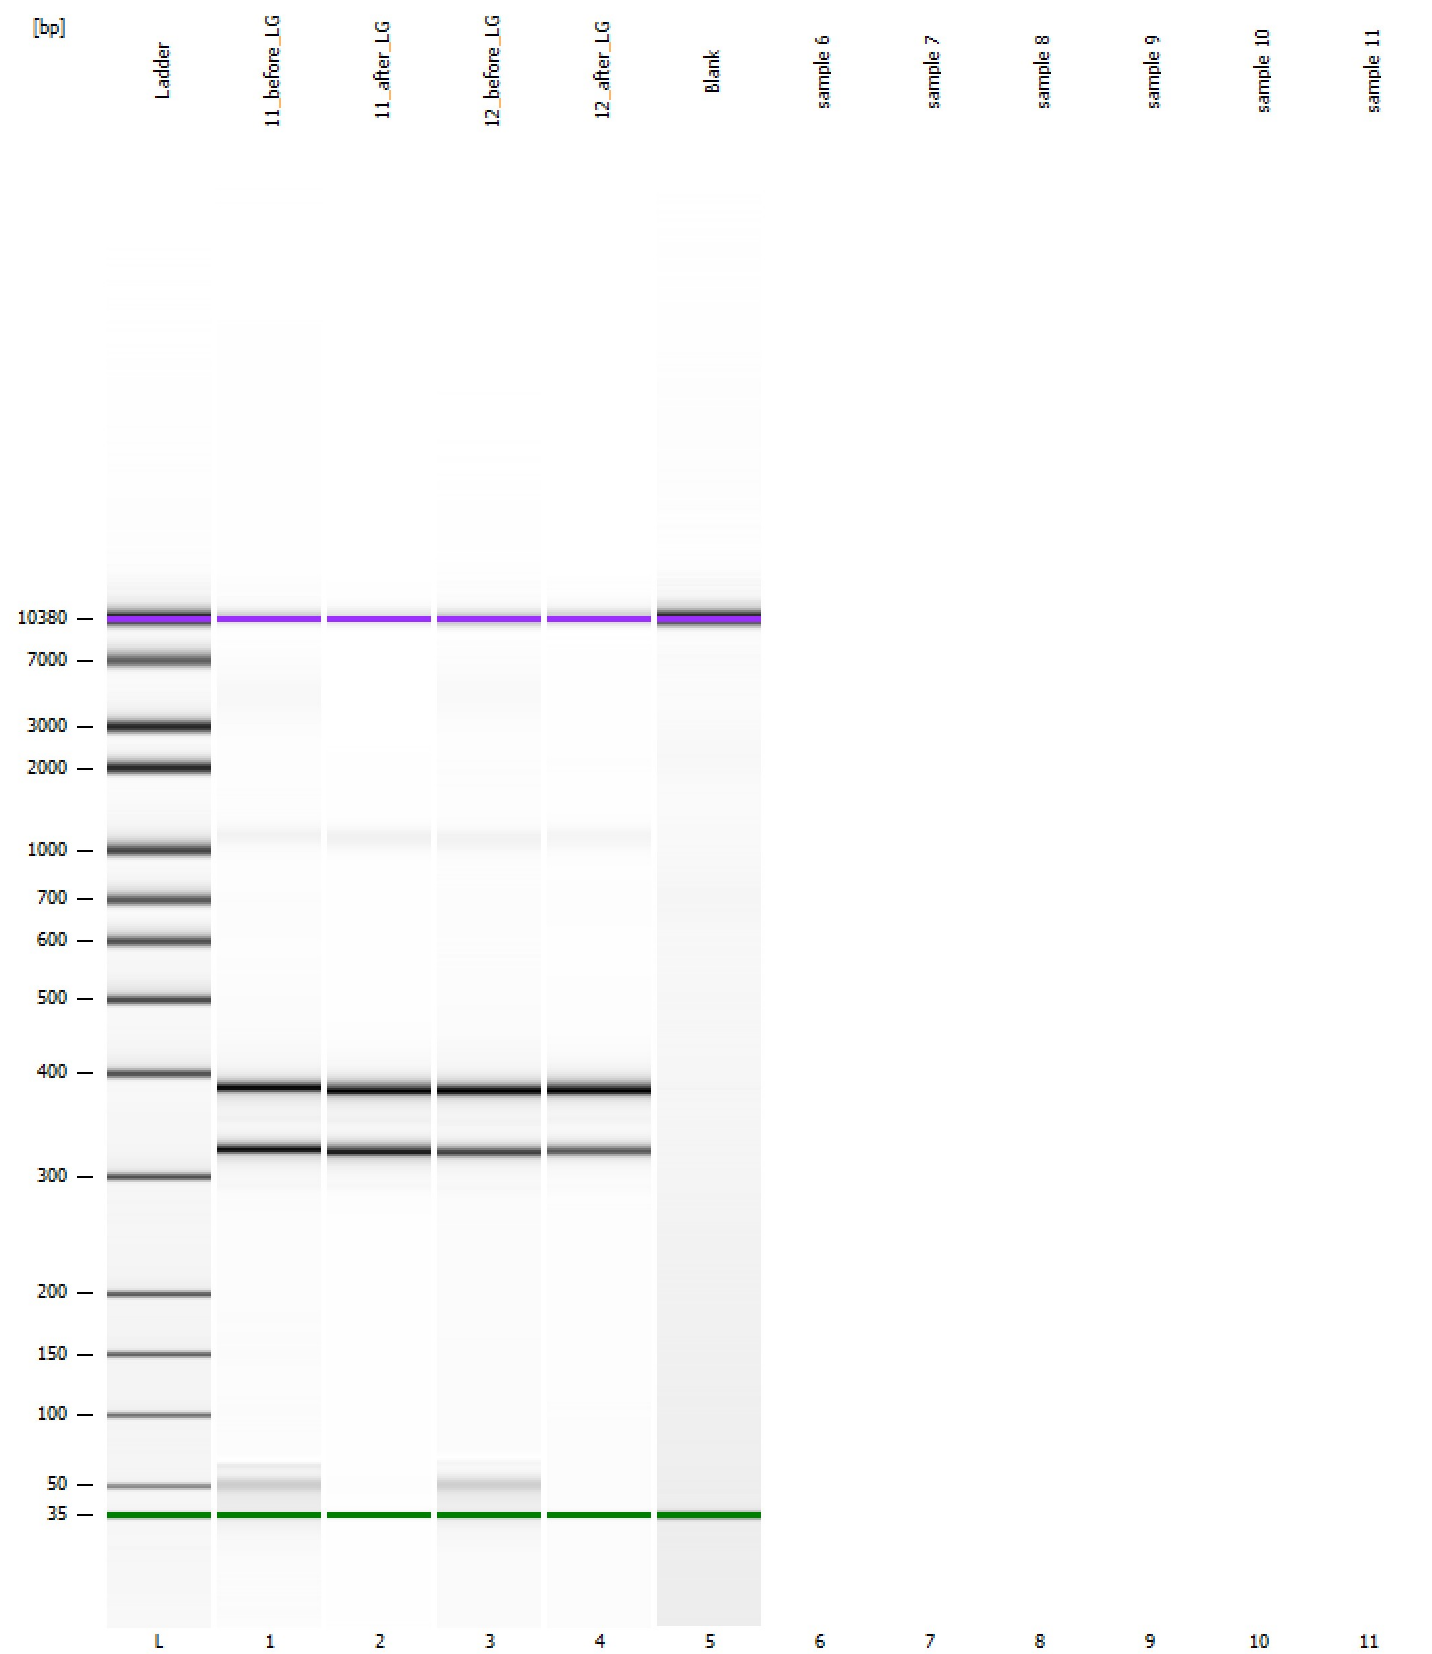


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
Modified: 4/28/2026 2:01:44 PM

Curves

Standard Curve

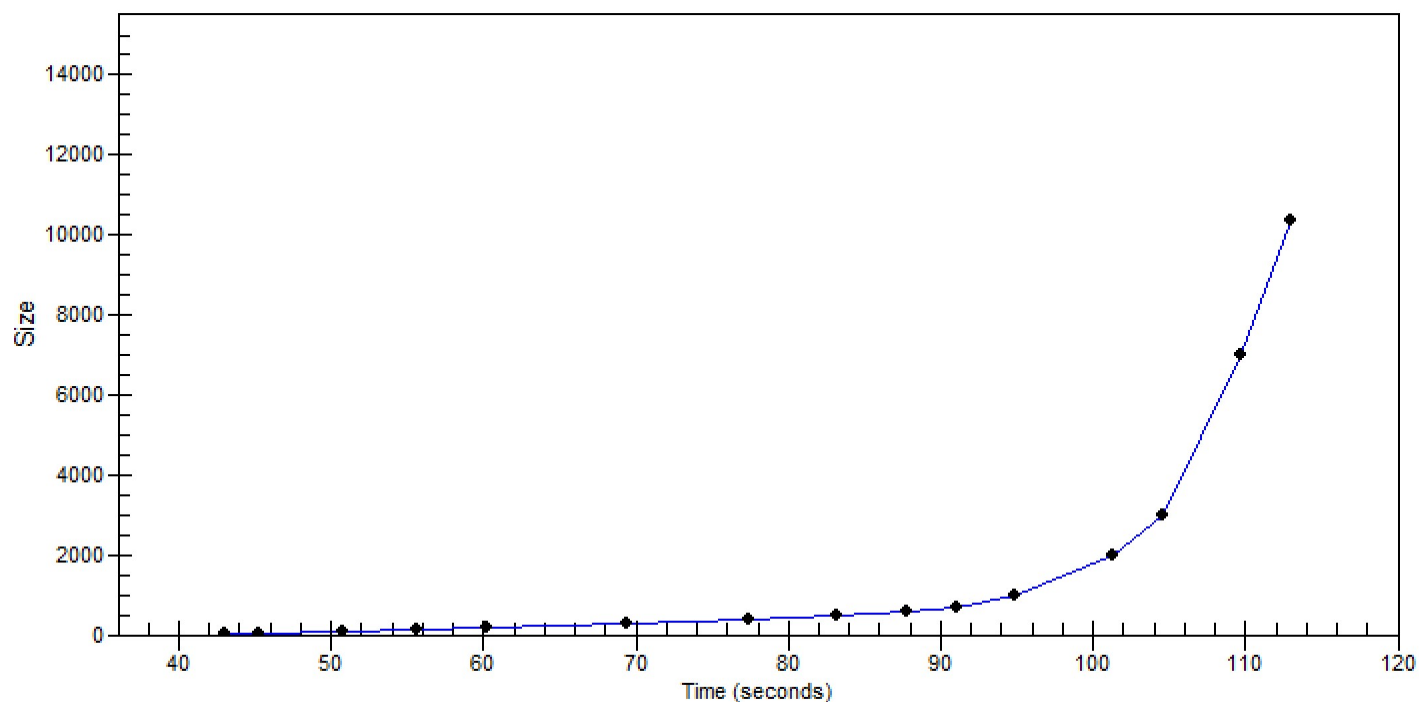

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
Modified: 4/28/2026 2:01:44 PM

Invalid Samples

Sample 6 has not been run, no results available.

Sample 7 has not been run, no results available.

Sample 8 has not been run, no results available.

Sample 9 has not been run, no results available.

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad

Created: 4/28/2026 1:29:27 PM
 Modified: 4/28/2026 2:01:44 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 6)		Instrument	Run		4/28/2026 1:53:37 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\Data\2026-04-28\2100 expert_High Sensitivity DNA Assay_DE54107817_2026-04-28_13-29-27.xad)		Instrument	Run		4/28/2026 1:29:33 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Product Number : G2939A		Instrument	Run		4/28/2026 1:29:33 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Name :		Instrument	Run		4/28/2026 1:29:33 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Vendor : Agilent Technologies		Instrument	Run		4/28/2026 1:29:33 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Serial# : DE54107817		Instrument	Run		4/28/2026 1:29:33 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Firmware : C.01.069		Instrument	Run		4/28/2026 1:29:33 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Cartridge : Electrode		Instrument	Run		4/28/2026 1:29:33 PM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC