


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
Modified: 7/17/2026 10:09:40 AM

Electrophoresis File Run Summary

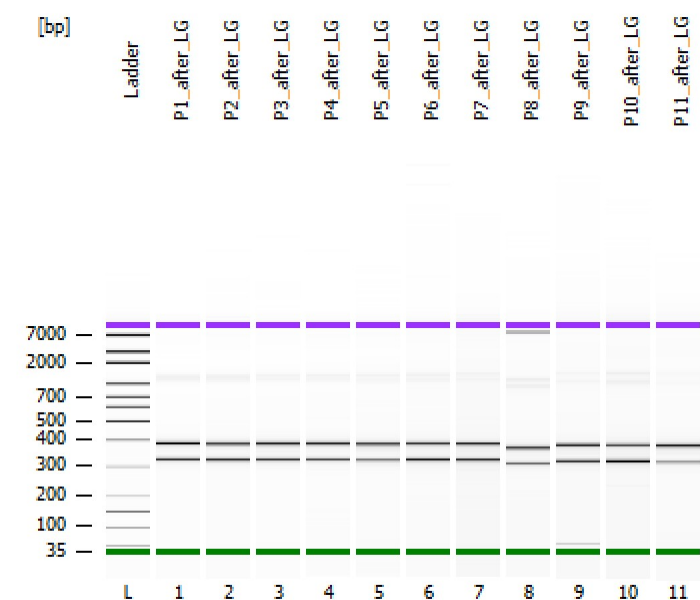

Instrument Information:


Instrument Name: DE54107817 Firmware: C.01.069
Serial#: DE54107817 Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

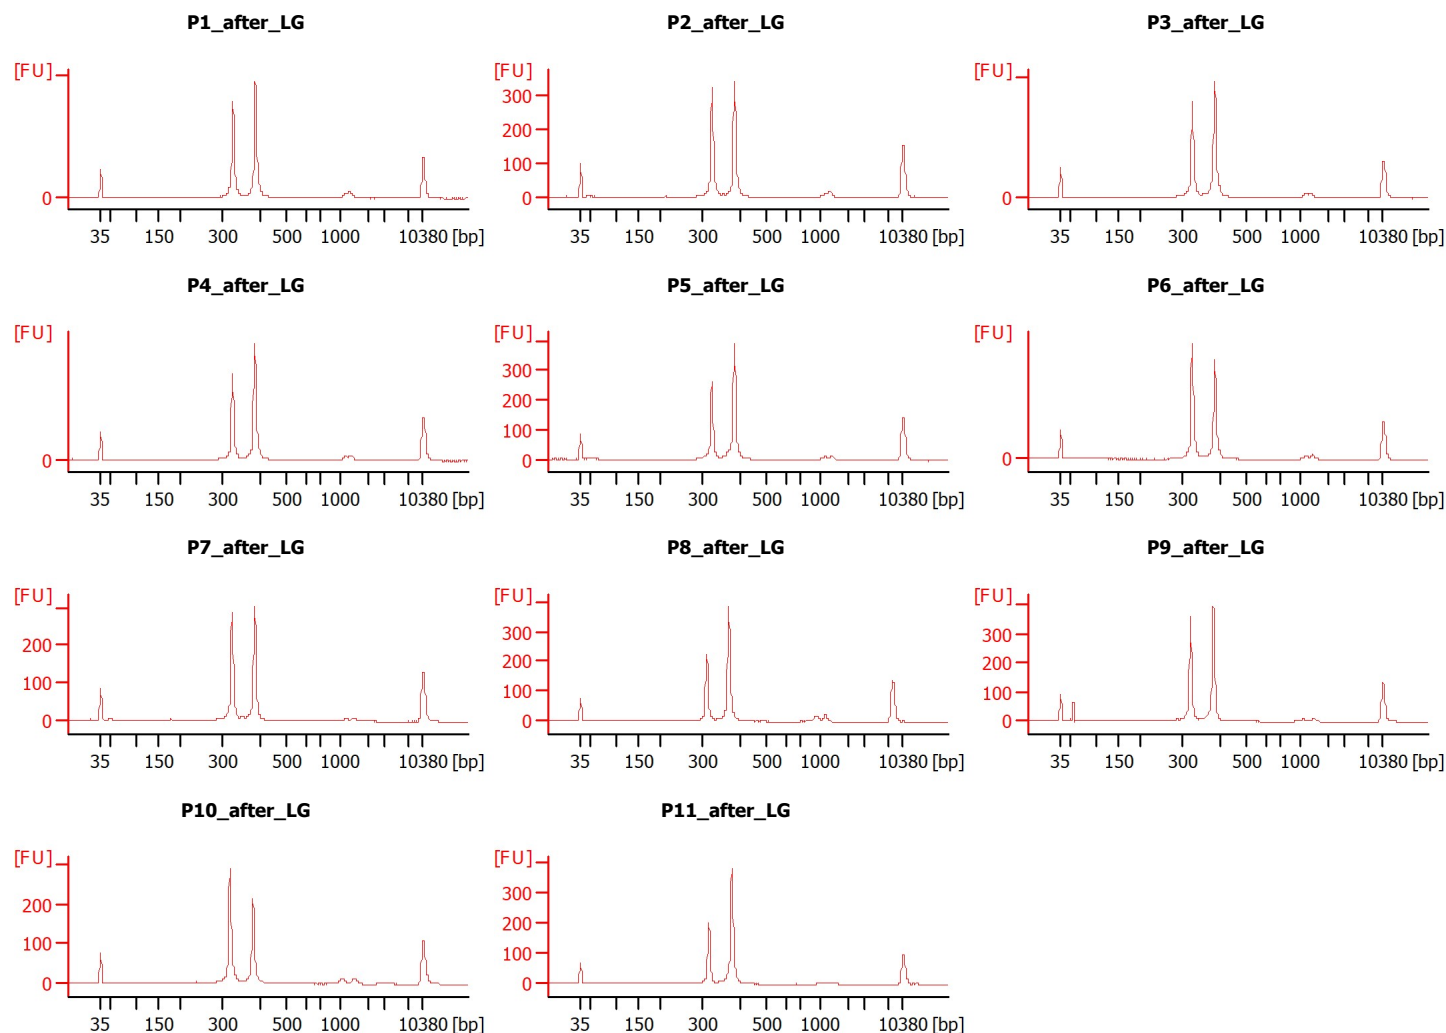

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
Modified: 7/17/2026 10:09:40 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
P1_after_LG		☐	✓			
P2_after_LG		☐	✓			
P3_after_LG		☐	✓			
P4_after_LG		☐	✓			
P5_after_LG		☐	✓			
P6_after_LG		☐	✓			
P7_after_LG		☐	✓			
P8_after_LG		☐	✓			
P9_after_LG		☐	✓			
P10_after_LG		☐	✓			
P11_after_LG		☐	✓			
Ladder		☐	✓			
Chip Lot #			Reagent Kit Lot #			

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
Modified: 7/17/2026 10:09:40 AM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary

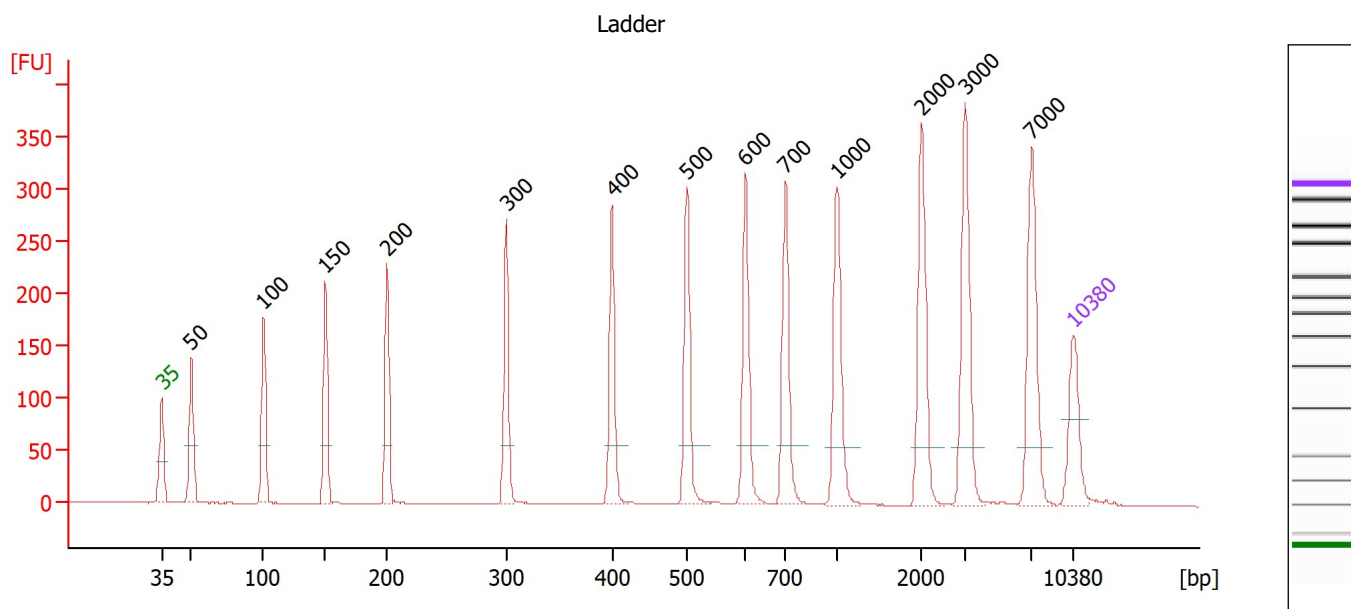

Overall Results for Ladder

Noise: 0.3


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

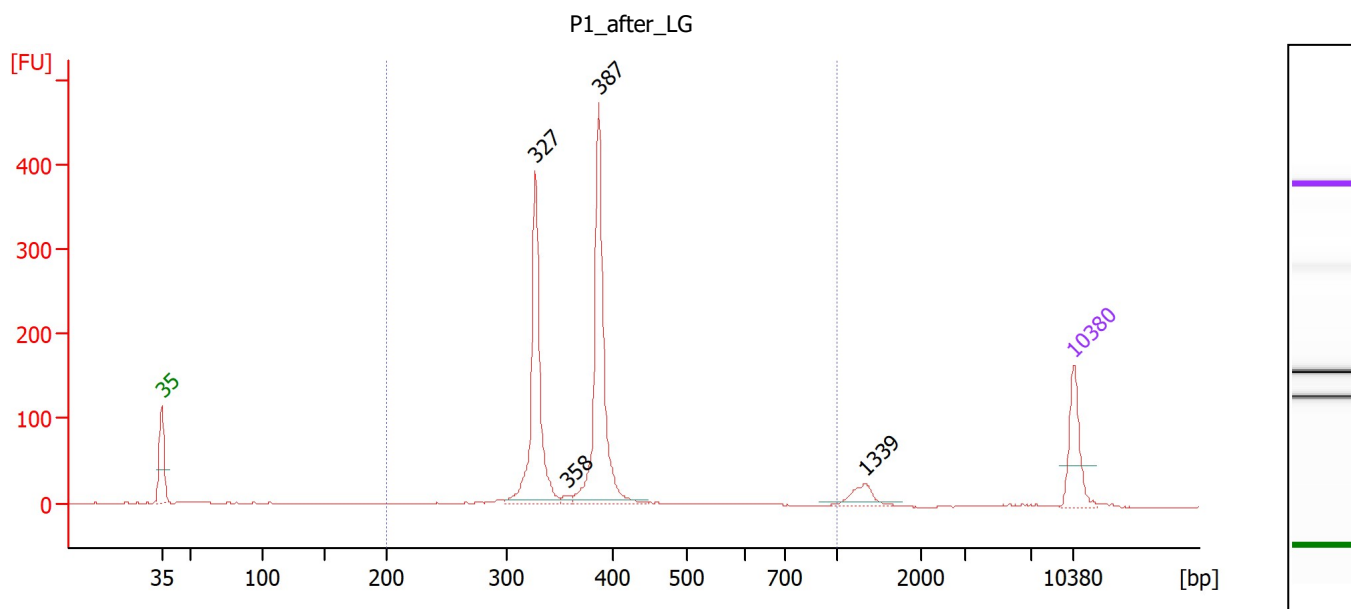

Overall Results for sample 1 : P1_after_LG

Number of peaks found: 4 Corr. Area 1: 978.4
 Noise: 0.3

Peak table for sample 1 : P1_after_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	327	353.15	1,633.9	
3	358	8.65	36.7	
4	387	392.93	1,537.5	
5	1,339	33.70	38.1	


Region table for sample 1 : P1_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	978.4	92	364	13.0	804.38	3,387.5	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

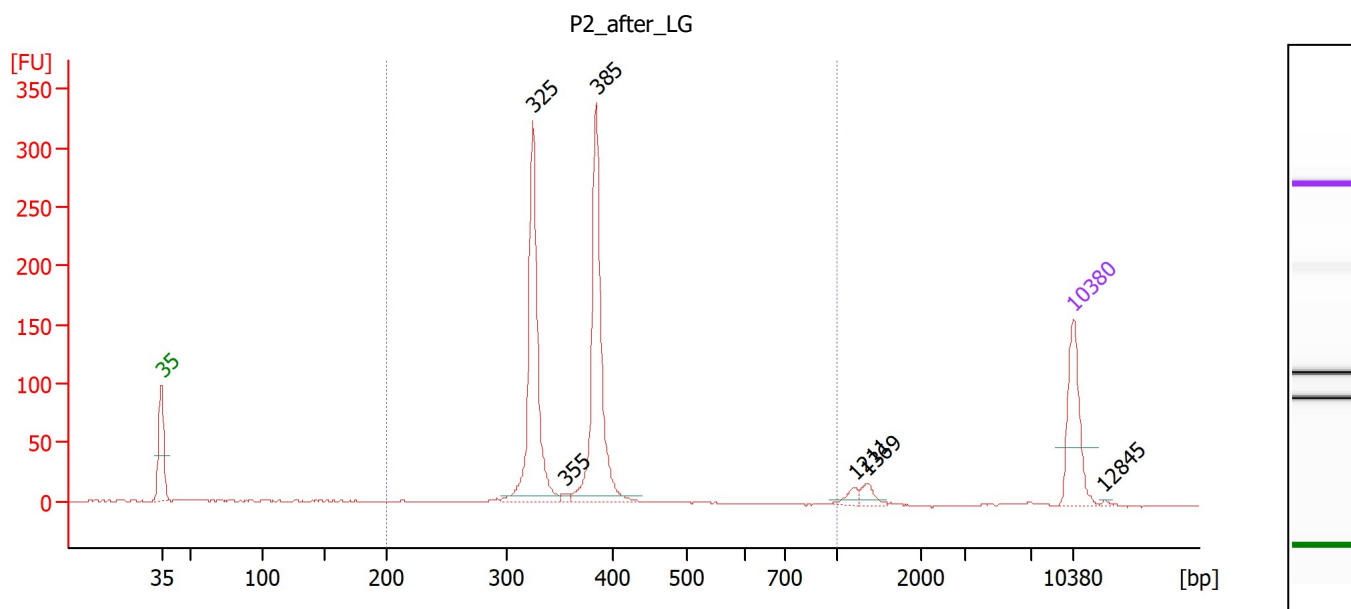

Overall Results for sample 2 : P2_after_LG

Number of peaks found: 6 Corr. Area 1: 784.9
 Noise: 0.4

Peak table for sample 2 : P2_after_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	325	286.07	1,335.4	
3	355	5.10	21.8	
4	385	272.33	1,072.8	
5	1,211	10.23	12.8	
6	1,369	12.84	14.2	
8	12,845	0.00	0.0	

Region table for sample 2 : P2_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	784.9	89	359	13.8	600.95	2,565.0	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

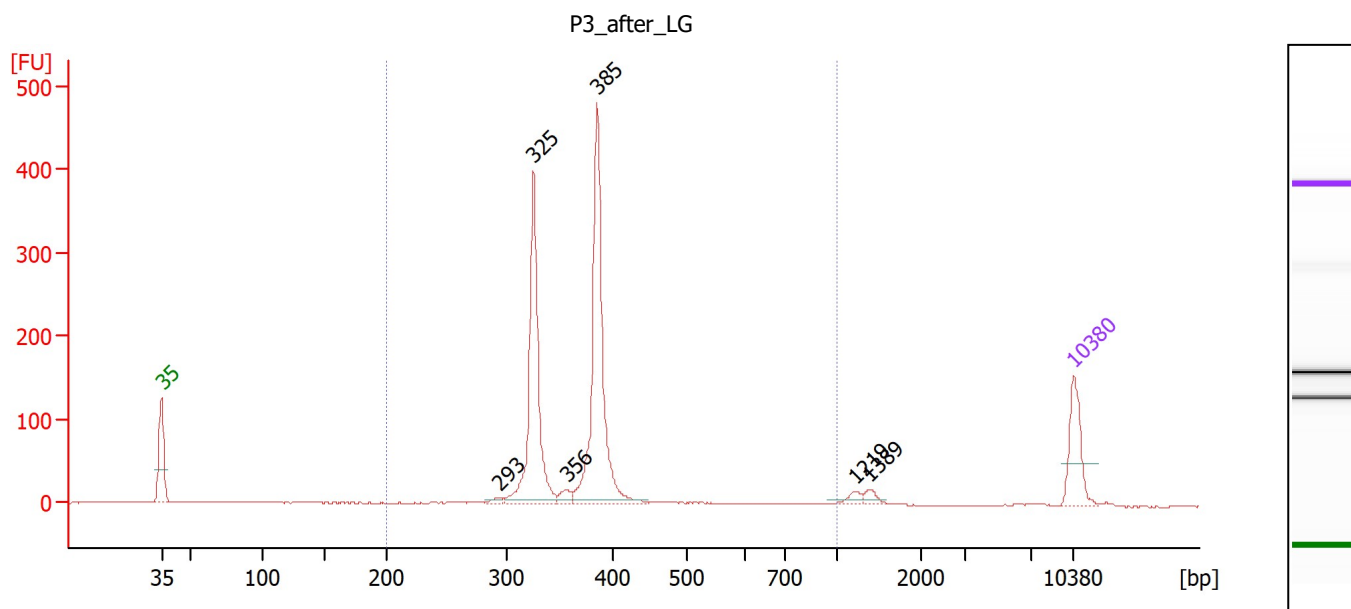Electropherogram Summary Continued ...**Overall Results for sample 3 : P3_after_LG**

Number of peaks found: 6 Corr. Area 1: 1,082.3
 Noise: 0.4

Peak table for sample 3 : P3_after_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	293	6.71	34.8	
3	325	369.80	1,722.8	
4	356	16.31	69.4	
5	385	432.80	1,701.4	
6	1,219	12.57	15.6	
7	1,389	12.65	13.8	


Region table for sample 3 : P3_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,082.3	92	368	17.8	883.08	3,706.9	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

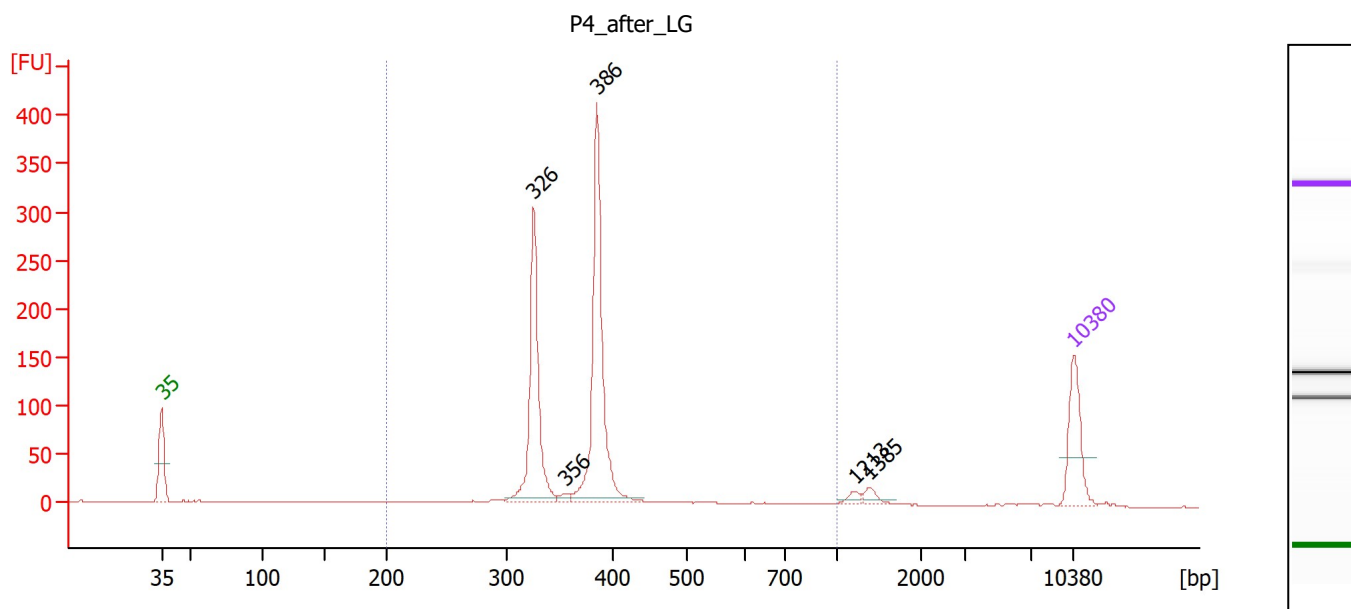

Overall Results for sample 4 : P4_after_LG

Number of peaks found: 5 Corr. Area 1: 842.6
 Noise: 0.4

Peak table for sample 4 : P4_after_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	326	267.05	1,242.8	
3	356	9.14	38.9	
4	386	346.17	1,360.2	
5	1,213	8.74	10.9	
6	1,385	11.49	12.6	


Region table for sample 4 : P4_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	842.6	92	368	15.4	669.51	2,799.8	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

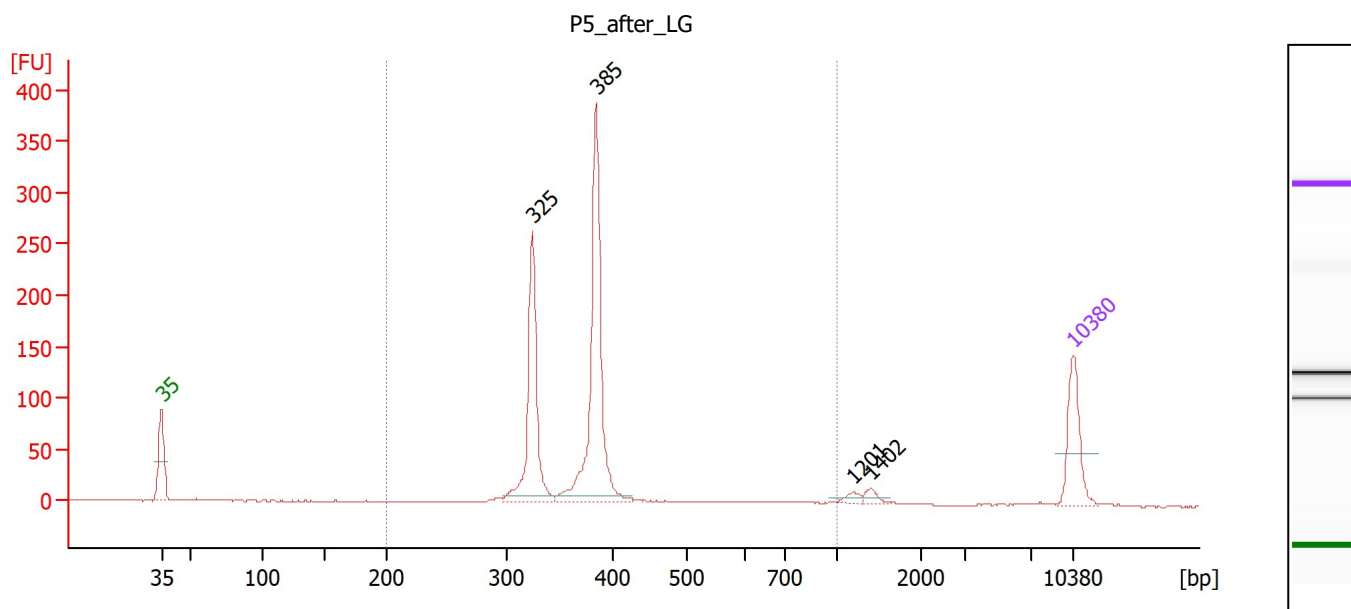

Overall Results for sample 5 : P5_after_LG

Number of peaks found: 4 Corr. Area 1: 784.7
 Noise: 0.3

Peak table for sample 5 : P5_after_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	325	242.00	1,129.5	
3	385	352.81	1,389.8	
4	1,201	9.17	11.6	
5	1,402	10.08	10.9	


Region table for sample 5 : P5_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	784.7	92	370	17.9	651.18	2,721.5	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

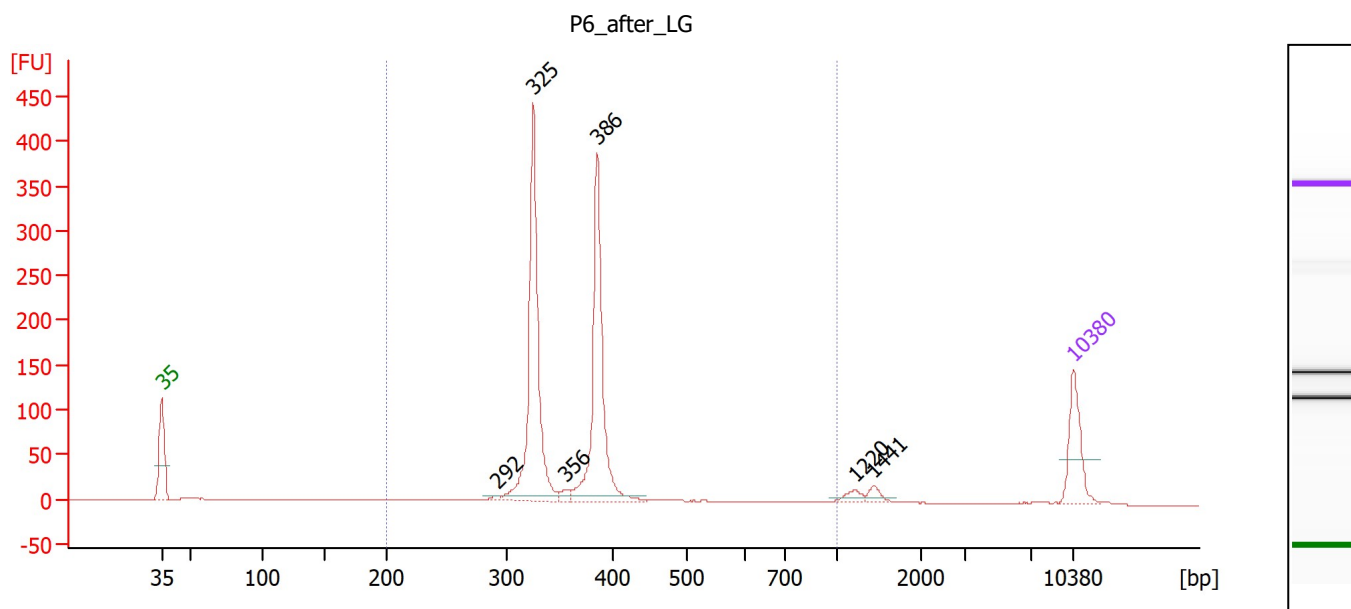

Overall Results for sample 6 : P6_after_LG

Number of peaks found: 6 Corr. Area 1: 983.5
 Noise: 0.4

Peak table for sample 6 : P6_after_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	292	5.98	31.0	
3	325	429.43	2,000.2	
4	356	11.63	49.6	
5	386	347.54	1,364.5	
6	1,220	12.63	15.7	
7	1,441	12.70	13.3	


Region table for sample 6 : P6_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	983.5	93	362	17.7	834.37	3,553.0	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

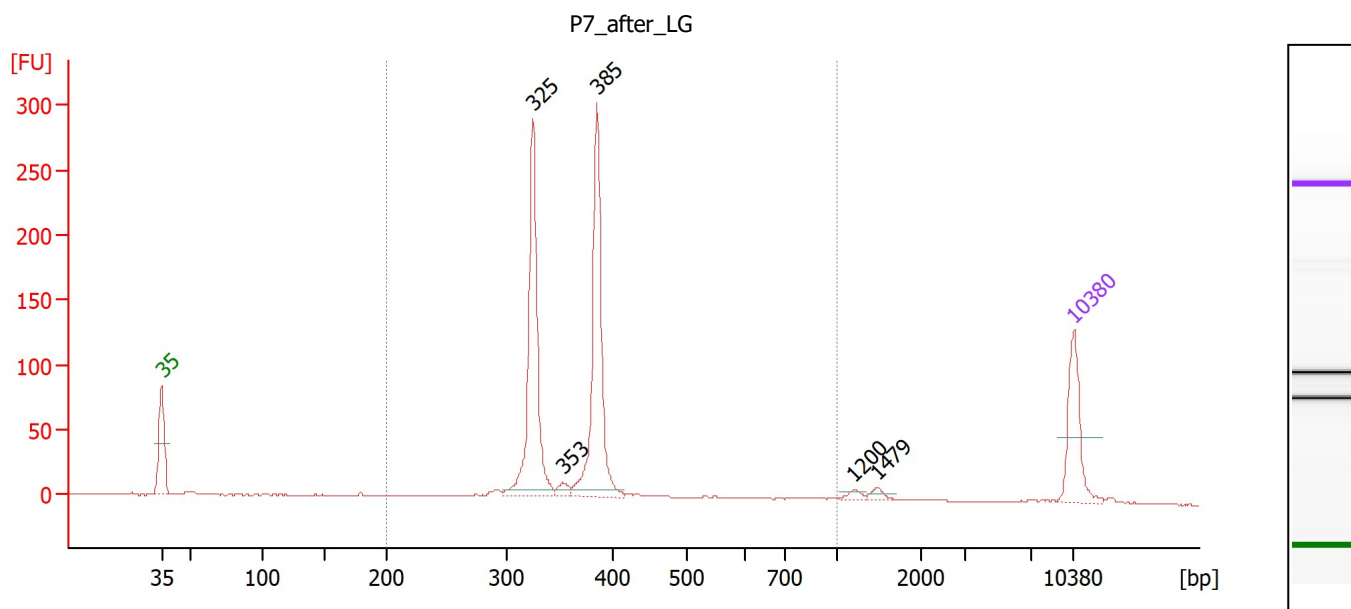

Overall Results for sample 7 : P7_after_LG

Number of peaks found: 5 Corr. Area 1: 701.9
 Noise: 0.3

Peak table for sample 7 : P7_after_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	325	295.35	1,376.8	
3	353	12.31	52.9	
4	385	274.19	1,078.0	
5	1,200	6.28	7.9	
6	1,479	6.81	7.0	

Region table for sample 7 : P7_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	701.9	90	367	20.7	656.26	2,789.2	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

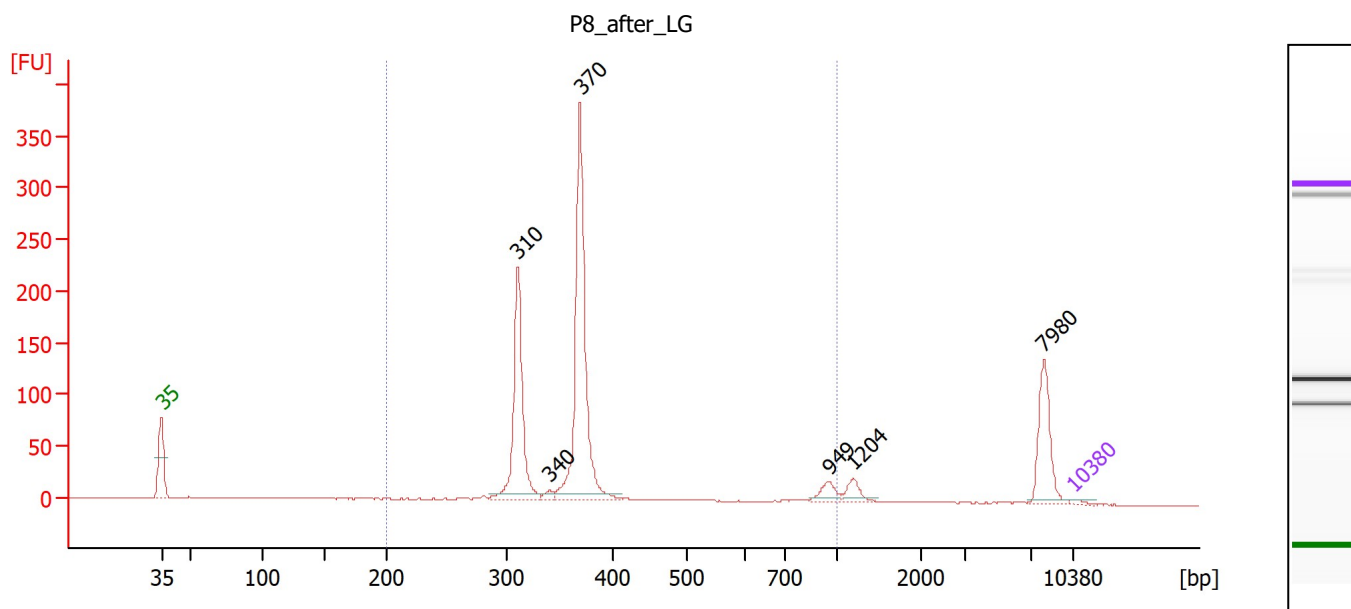Electropherogram Summary Continued ...**Overall Results for sample 8 : P8_after_LG**

Number of peaks found: 6 Corr. Area 1: 756.3
 Noise: 0.4

Peak table for sample 8 : P8_after_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	310	5,470.61	26,704.9	
3	340	206.49	920.1	
4	370	8,792.51	36,035.0	
5	949	486.03	775.9	
6	1,204	445.91	561.2	
7	7,980	1,897.76	360.3	


Region table for sample 8 : P8_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	756.3	81	380	34.1	15,686.69	66,743.8	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

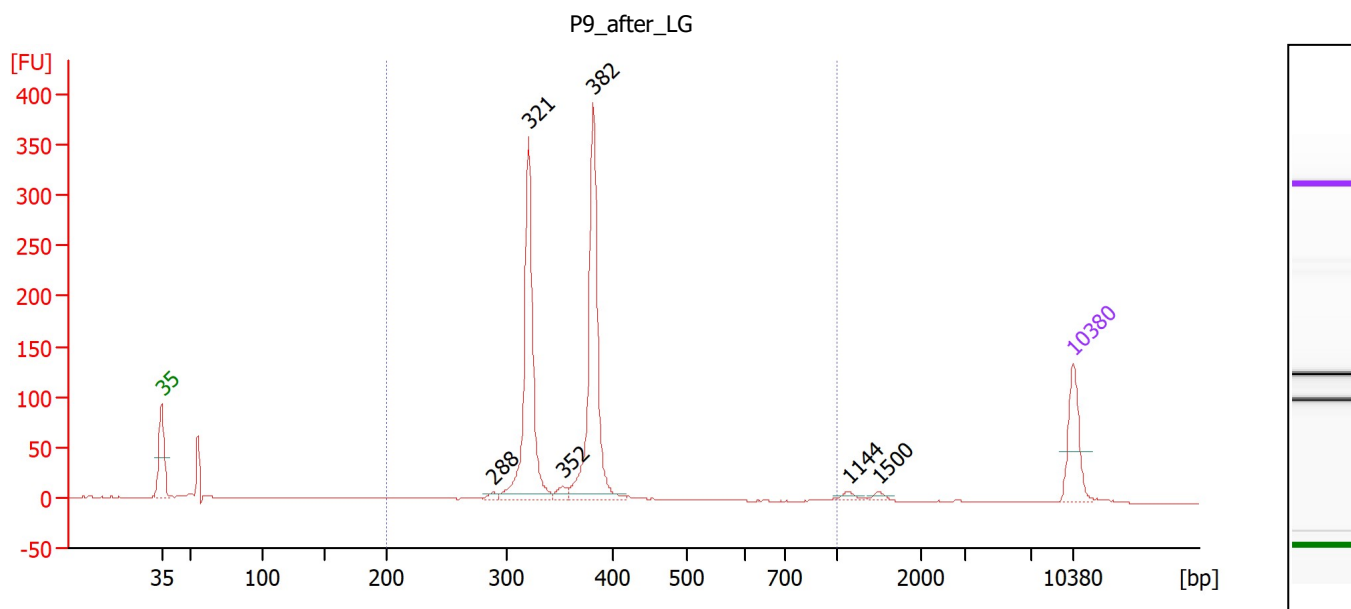

Overall Results for sample 9 : P9_after_LG

Number of peaks found: 6 Corr. Area 1: 839.6
 Noise: 0.4

Peak table for sample 9 : P9_after_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	288	8.25	43.4	
3	321	388.71	1,836.3	
4	352	15.80	68.0	
5	382	384.92	1,528.7	
6	1,144	8.65	11.4	
7	1,500	6.93	7.0	


Region table for sample 9 : P9_after_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	839.6	89	358	16.7	833.67	3,582.8	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

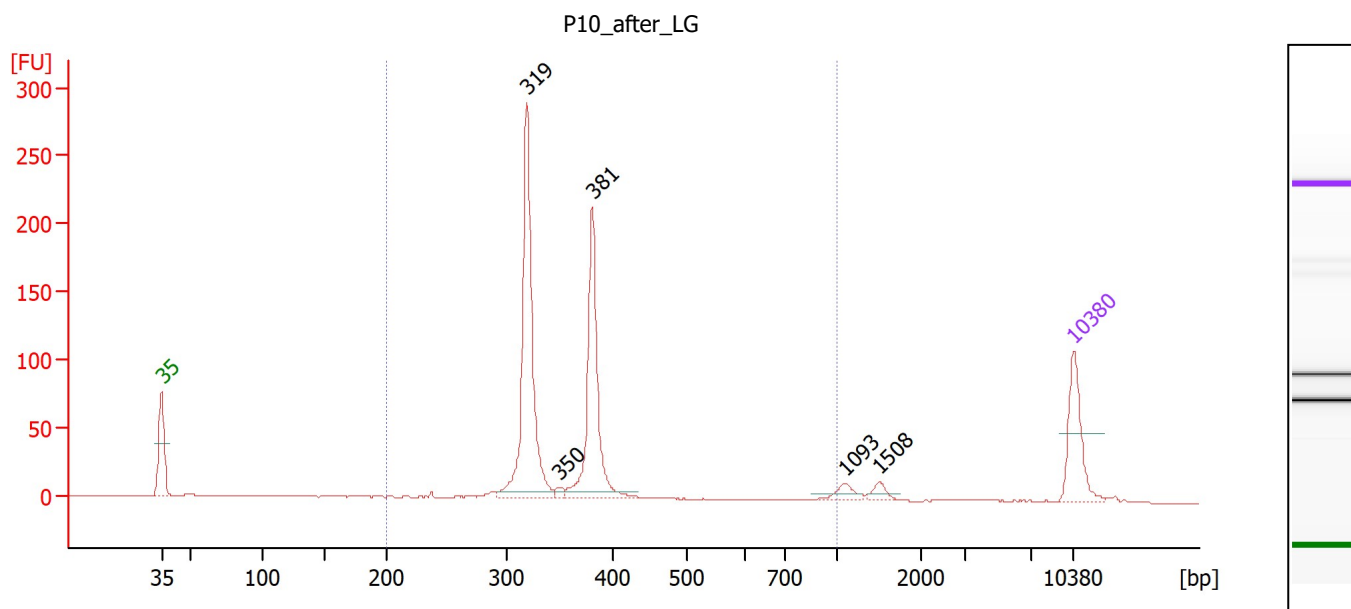

Overall Results for sample 10 : P10_after LG

Number of peaks found: 5 Corr. Area 1: 632.2
 Noise: 0.3

Peak table for sample 10 : P10_after LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	319	371.52	1,763.3	
3	350	7.53	32.7	
4	381	241.71	960.5	
5	1,093	16.58	23.0	
6	1,508	12.27	12.3	


Region table for sample 10 : P10_after LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	632.2	87	356	22.3	672.56	2,945.0	200	1,000

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Electropherogram Summary Continued ...

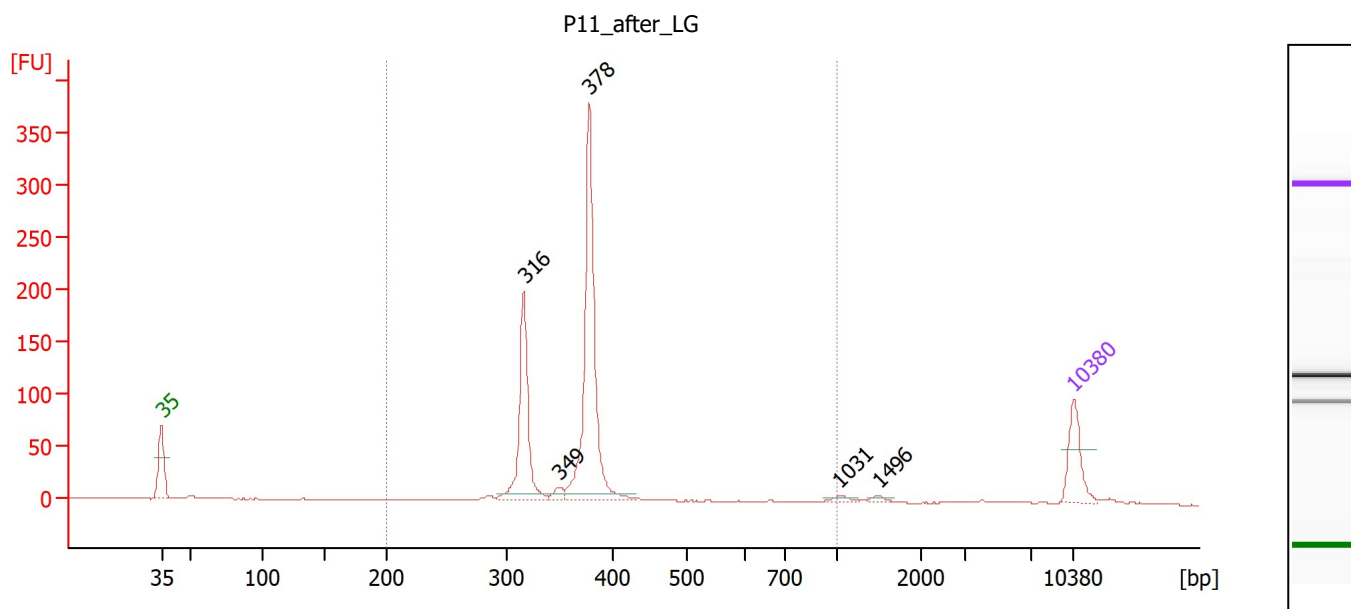

Overall Results for sample 11 : P11 after LG

Number of peaks found: 5 Corr. Area 1: 693.0
 Noise: 0.2

Peak table for sample 11 : P11 after LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	316	272.81	1,306.0	
3	349	17.82	77.3	
4	378	505.19	2,024.3	
5	1,031	9.60	14.1	
6	1,496	7.79	7.9	

Region table for sample 11 : P11 after LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	693.0	91	366	19.3	861.92	3,645.6	200	1,000


Assay Class: High Sensitivity DNA Assay

Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM

Modified: 7/17/2026 10:09:40 AM

Gel Image

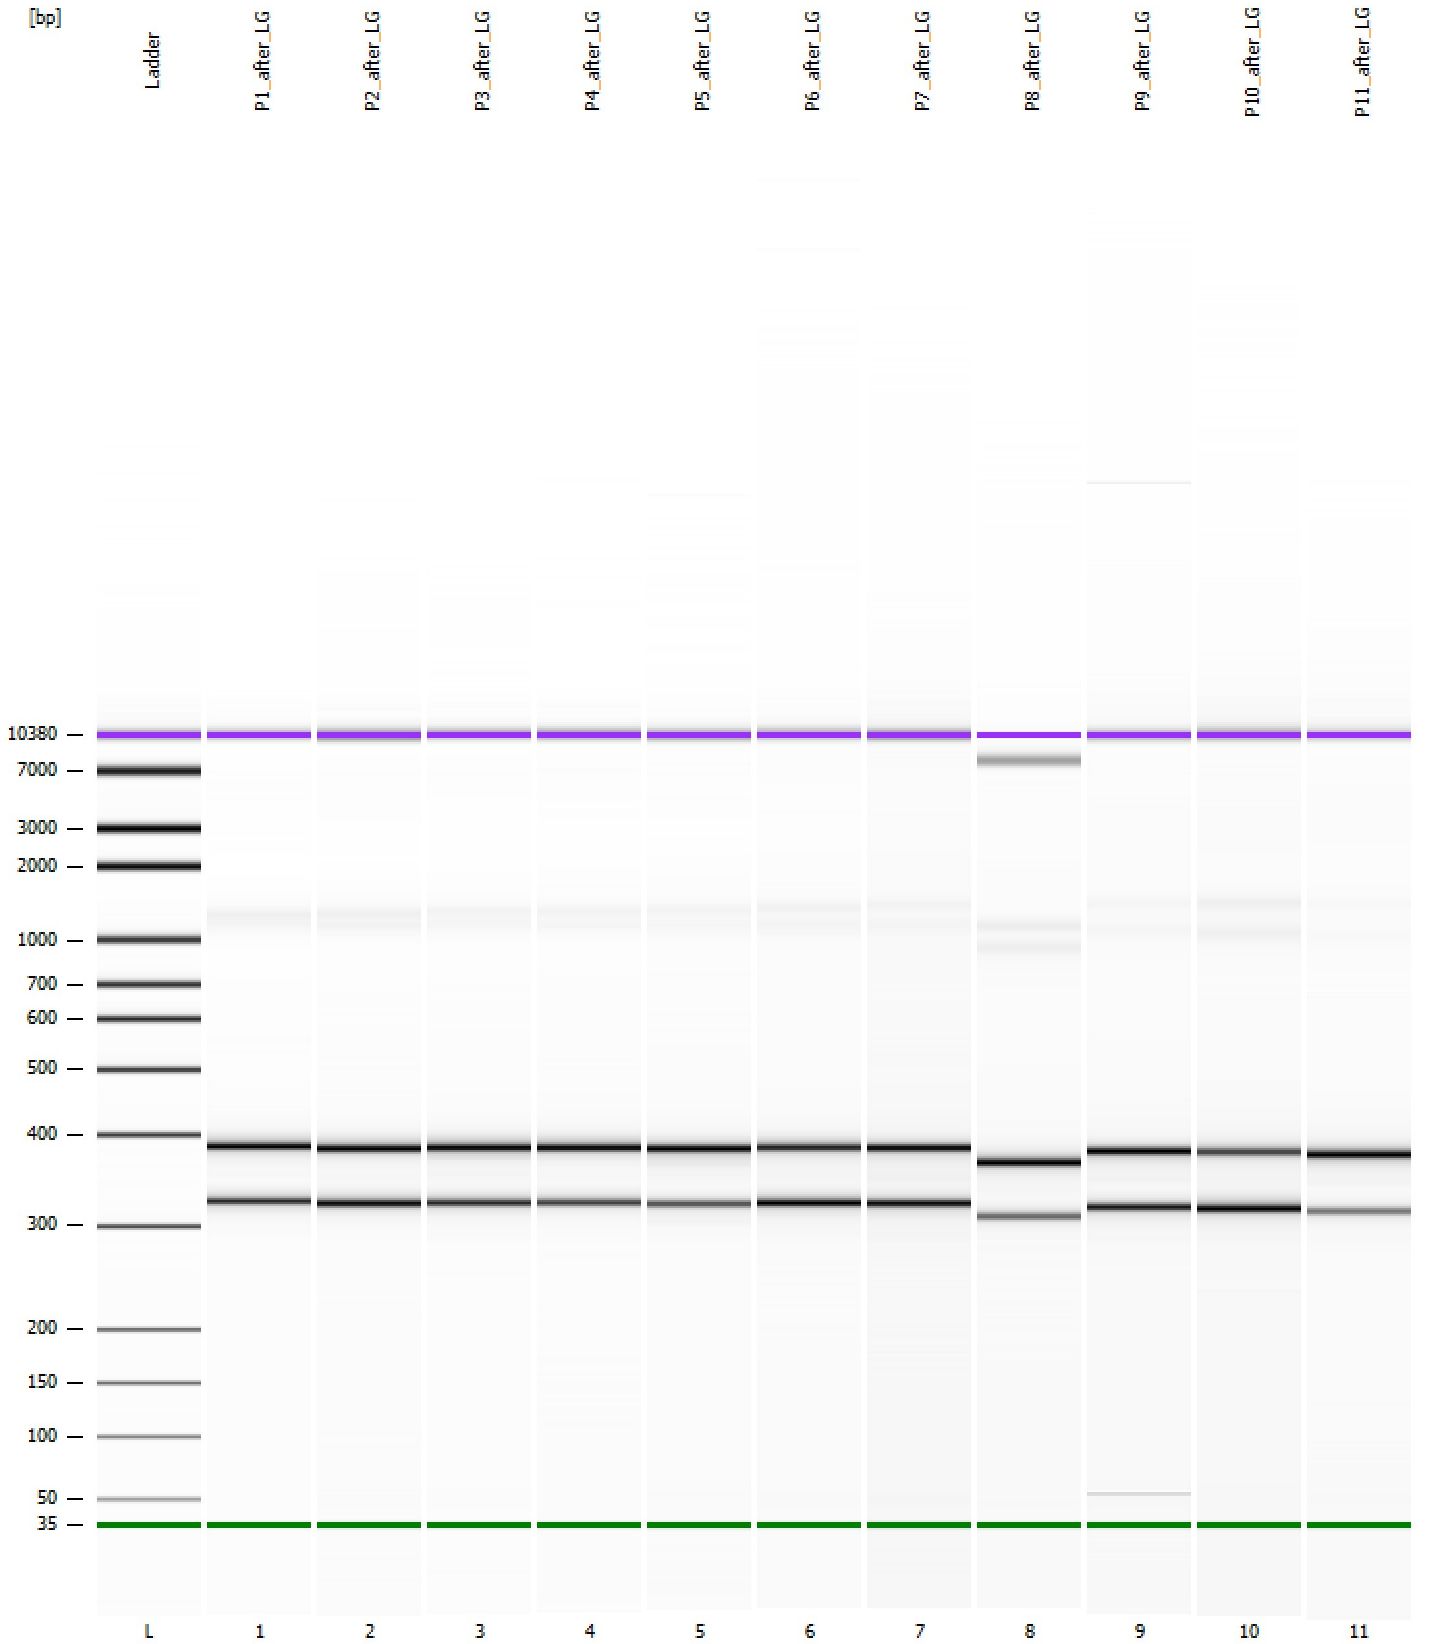


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
Modified: 7/17/2026 10:09:40 AM

Curves

Standard Curve

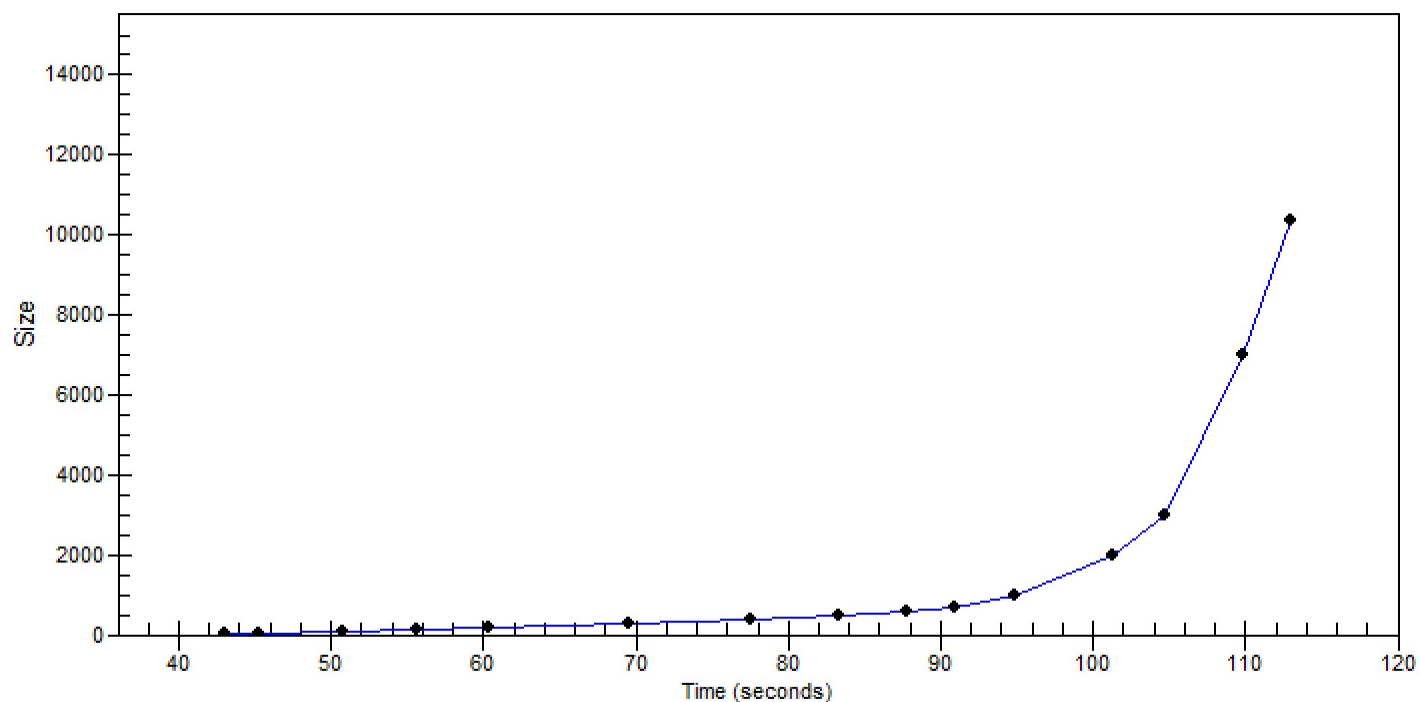

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad

Created: 7/17/2026 9:15:09 AM
 Modified: 7/17/2026 10:09:40 AM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		7/17/2026 9:56:29 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\Data\2026-07-17\2100 expert_High Sensitivity DNA Assay_DE54107817_2026-07-17_09-15-10.xad)		Instrument	Run		7/17/2026 9:15:15 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Product Number : G2939A		Instrument	Run		7/17/2026 9:15:15 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Name :		Instrument	Run		7/17/2026 9:15:15 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Vendor : Agilent Technologies		Instrument	Run		7/17/2026 9:15:15 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Serial# : DE54107817		Instrument	Run		7/17/2026 9:15:15 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Firmware : C.01.069		Instrument	Run		7/17/2026 9:15:15 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Cartridge : Electrode		Instrument	Run		7/17/2026 9:15:15 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC