


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
Modified: 4/22/2026 9:05:52 AM

Electrophoresis File Run Summary

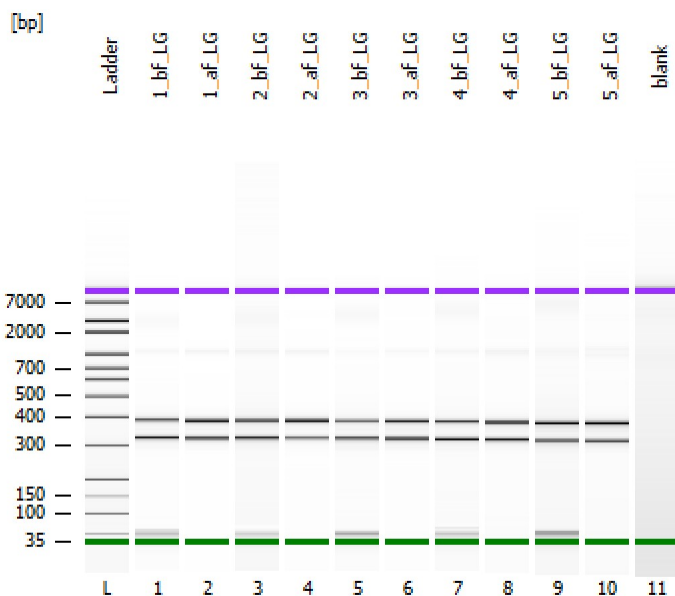

Instrument Information:

Instrument Name: DE54107817 Firmware: C.01.069
Serial#: DE54107817 Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy

Assay Class: High Sensitivity DNA Assay

Version: 1.03


Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:

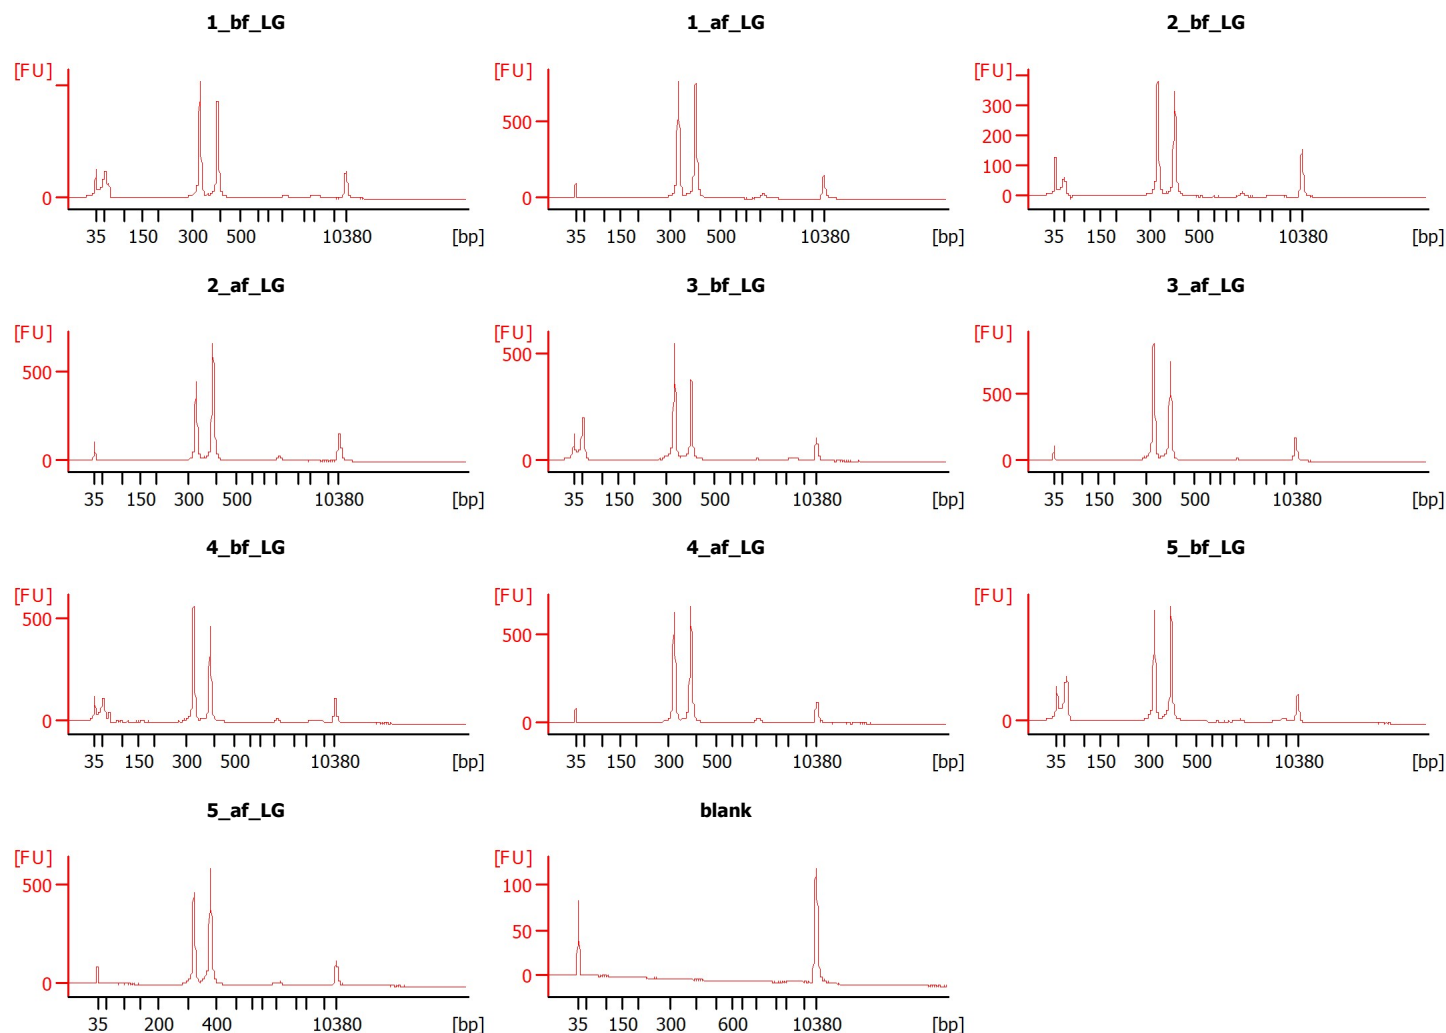

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
Modified: 4/22/2026 9:05:52 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
1_bf_LG		☐	✓			
1_af_LG		☐	✓			
2_bf_LG		☐	✓			
2_af_LG		☐	✓			
3_bf_LG		☐	✓			
3_af_LG		☐	✓			
4_bf_LG		☐	✓			
4_af_LG		☐	✓			
5_bf_LG		☐	✓			
5_af_LG		☐	✓			
blank		☐	✓			
Ladder		☐	✓			
Chip Lot #			Reagent Kit Lot #			

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
Modified: 4/22/2026 9:05:52 AM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

Electropherogram Summary

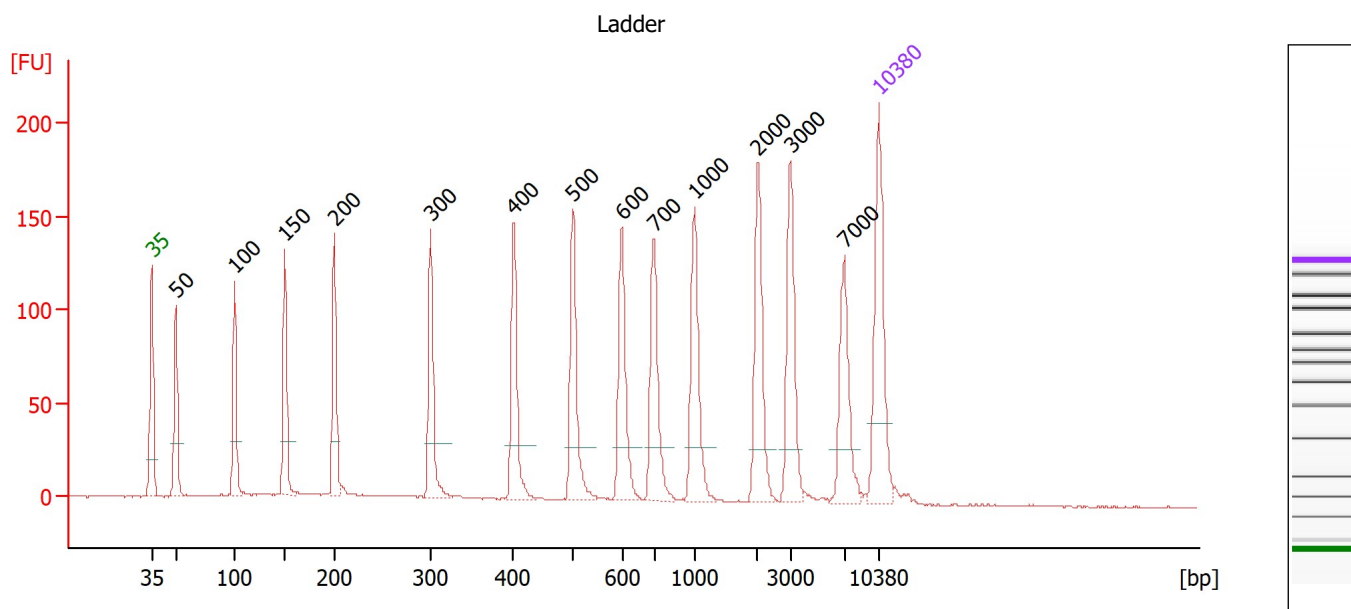

Overall Results for Ladder

Noise: 0.4


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

Electropherogram Summary Continued ...

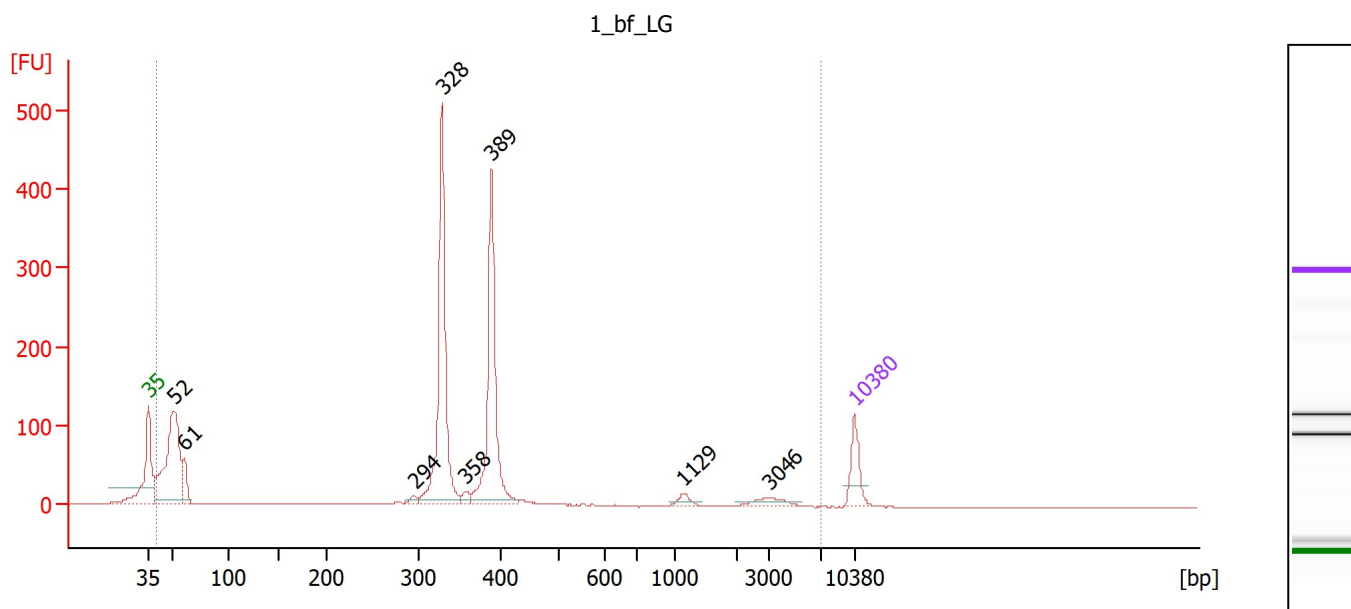

Overall Results for sample 1 : 1_bf_LG

Number of peaks found: 8 Corr. Area 1: 1,675.1
 Noise: 0.3

Peak table for sample 1 : 1_bf_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	52	690.71	20,305.1	
3	61	95.19	2,353.4	
4	294	17.44	89.7	
5	328	671.94	3,104.3	
6	358	21.89	92.7	
7	389	538.61	2,095.8	
8	1,129	18.83	25.3	
9	3,046	29.91	14.9	

Region table for sample 1 : 1_bf_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,675.1	98	419	100.0	2,117.17	28,206.5	41	6,981

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

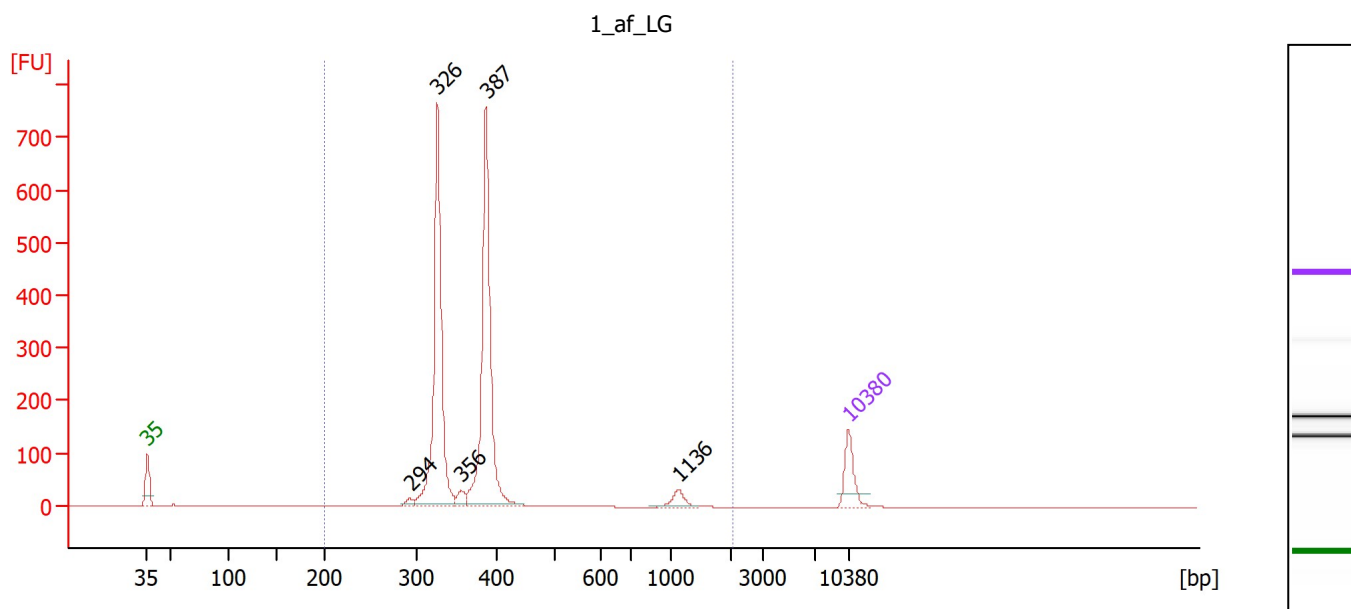Electropherogram Summary Continued ...**Overall Results for sample 2 : 1_af_LG**

Number of peaks found: 5 Corr. Area 1: 2,013.7
 Noise: 0.4

Peak table for sample 2 : 1_af_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	294	15.42	79.6	
3	326	768.62	3,567.3	
4	356	29.06	123.5	
5	387	739.16	2,894.2	
6	1,136	32.98	44.0	

Region table for sample 2 : 1_af_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	2,013.7	99	382	36.0	1,571.93	6,576.3	200	2,011

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

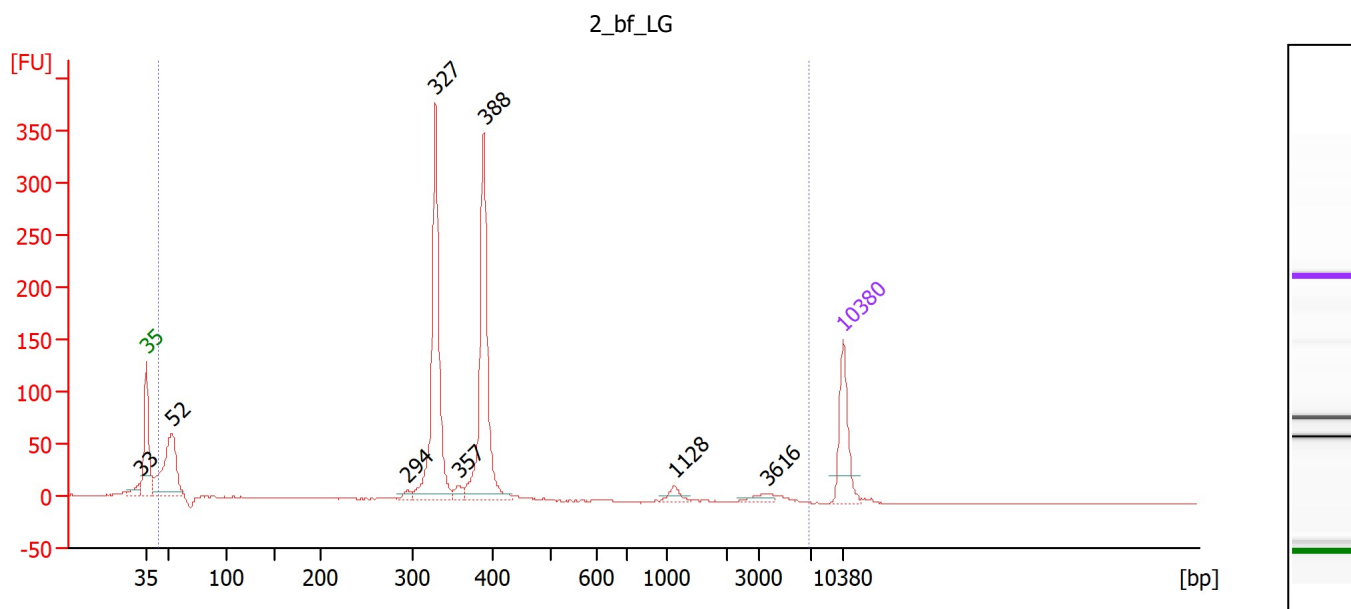Electropherogram Summary Continued ...**Overall Results for sample 3 : 2_bf_LG**

Number of peaks found: 8 Corr. Area 1: 1,096.5
 Noise: 0.3

Peak table for sample 3 : 2_bf_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	33	0.00	0.0	
3	52	233.56	6,767.0	
4	294	8.98	46.4	
5	327	369.50	1,710.3	
6	357	13.92	59.1	
7	388	323.67	1,263.3	
8	1,128	13.26	17.8	
9	3,616	11.17	4.7	


Region table for sample 3 : 2_bf_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,096.5	95	418	100.0	924.49	9,259.0	43	6,854

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

Electropherogram Summary Continued ...

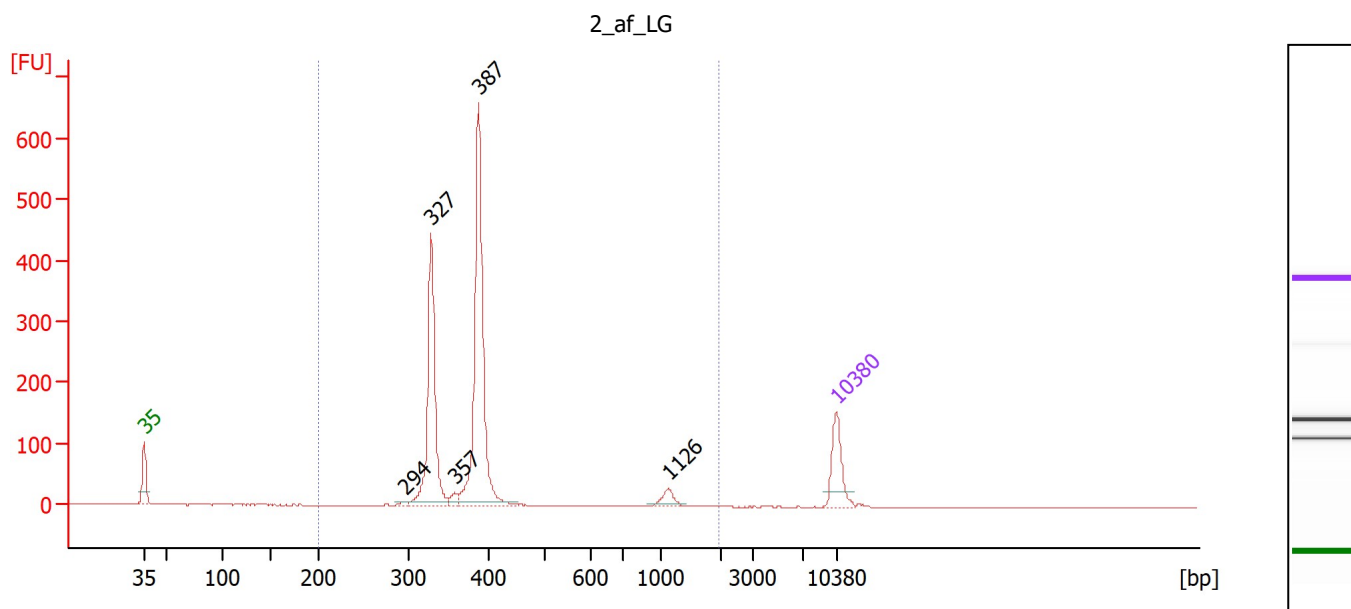

Overall Results for sample 4 : 2_af_LG

Number of peaks found: 5 Corr. Area 1: 1,474.3
 Noise: 0.3

Peak table for sample 4 : 2_af_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	294	6.15	31.6	
3	327	393.15	1,820.8	
4	357	17.79	75.6	
5	387	573.55	2,244.9	
6	1,126	23.28	31.3	

Region table for sample 4 : 2_af_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,474.3	98	397	40.7	1,017.72	4,157.5	200	1,978

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

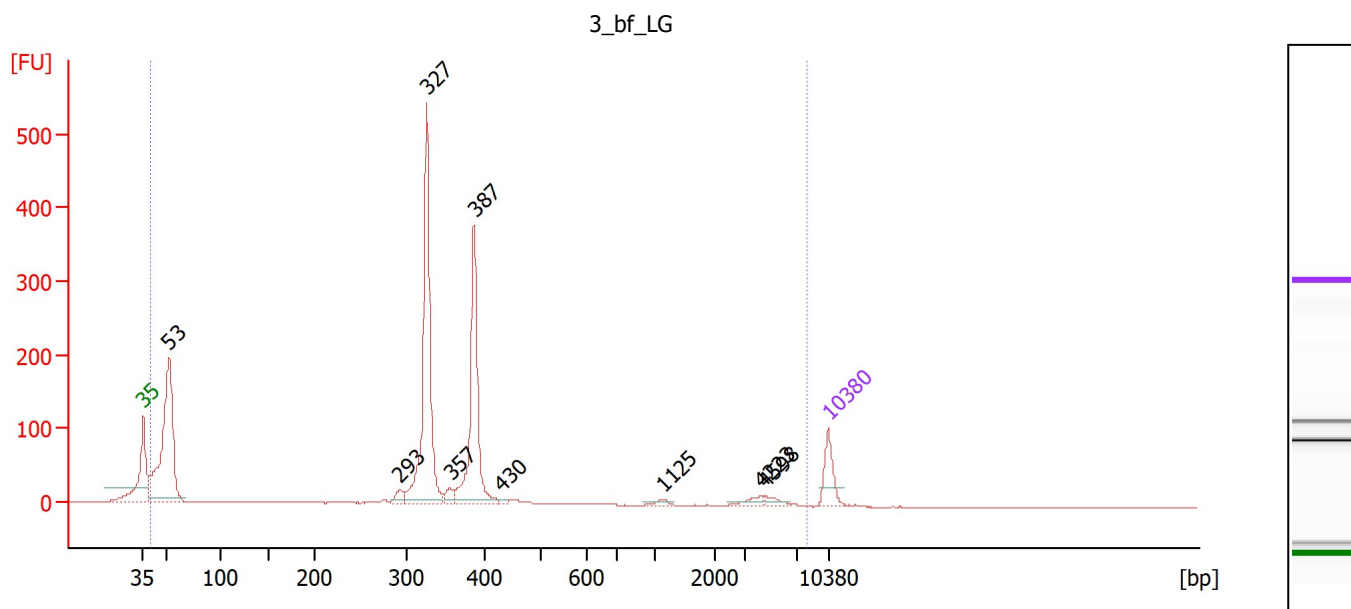Electropherogram Summary Continued ...**Overall Results for sample 5 : 3_bf_LG**

Number of peaks found: 9 Corr. Area 1: 1,785.5
 Noise: 0.2

Peak table for sample 5 : 3_bf_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	53	924.52	26,351.1	
3	293	32.46	167.8	
4	327	760.84	3,528.2	
5	357	31.47	133.7	
6	387	492.14	1,925.3	
7	430	5.92	20.9	
8	1,125	11.42	15.4	
9	4,223	20.58	7.4	
10	4,598	18.19	6.0	


Region table for sample 5 : 3_bf_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,785.5	98	465	100.0	2,379.57	33,630.8	41	8,111

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

Electropherogram Summary Continued ...

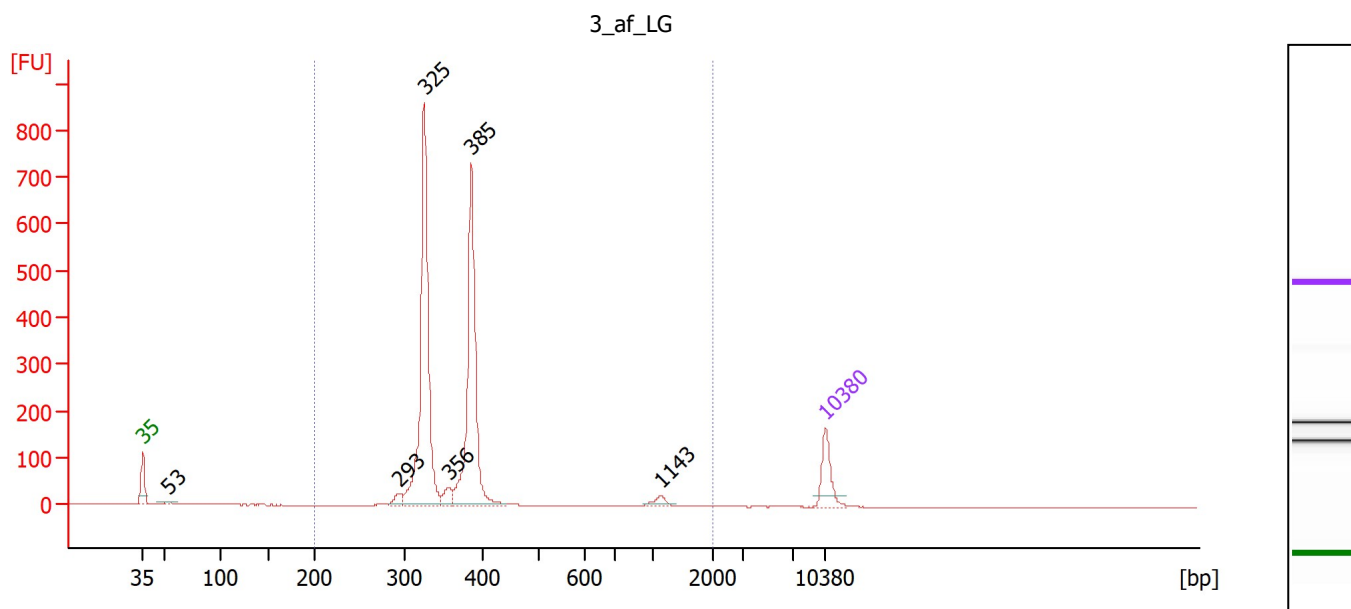

Overall Results for sample 6 : 3_af_LG

Number of peaks found: 6 Corr. Area 1: 2,149.1
 Noise: 0.3

Peak table for sample 6 : 3_af_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	53	12.59	358.5	
3	293	27.00	139.4	
4	325	801.15	3,733.4	
5	356	40.00	170.3	
6	385	631.82	2,485.2	
7	1,143	17.26	22.9	

Region table for sample 6 : 3_af_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	2,149.1	99	371	33.2	1,530.13	6,515.1	200	2,038

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

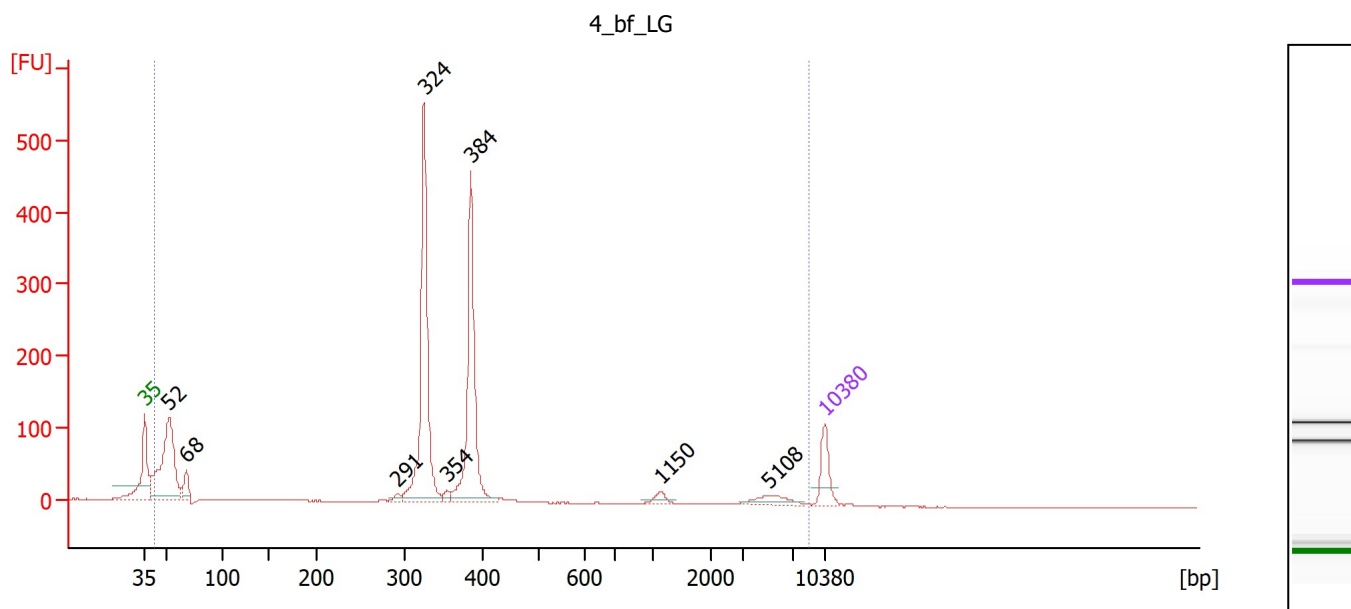Electropherogram Summary Continued ...**Overall Results for sample 7 : 4_bf_LG**

Number of peaks found: 8 Corr. Area 1: 1,656.8
 Noise: 0.3

Peak table for sample 7 : 4_bf_LG

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	52	614.02	17,932.7	
3	68	75.37	1,685.0	
4	291	15.48	80.6	
5	324	701.67	3,283.2	
6	354	18.31	78.4	
7	384	544.59	2,148.2	
8	1,150	22.10	29.1	
9	5,108	41.79	12.4	


Region table for sample 7 : 4_bf_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,656.8	98	547	100.0	2,023.82	24,711.7	41	8,636

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

Electropherogram Summary Continued ...

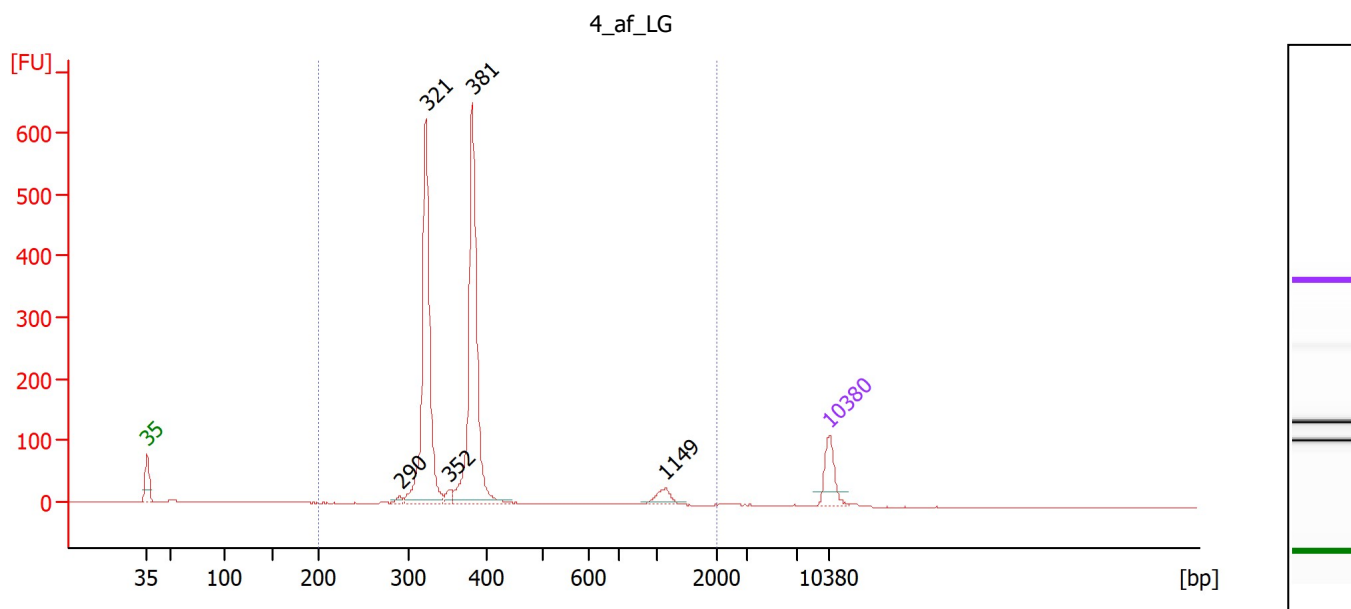

Overall Results for sample 8 : 4_af_LG

Number of peaks found: 5 Corr. Area 1: 1,699.5
 Noise: 0.3

Peak table for sample 8 : 4_af_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	290	12.56	65.6	
3	321	729.84	3,441.5	
4	352	23.98	103.2	
5	381	731.41	2,910.6	
6	1,149	34.51	45.5	

Region table for sample 8 : 4_af_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,699.5	99	385	40.4	1,536.79	6,475.7	200	2,020

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

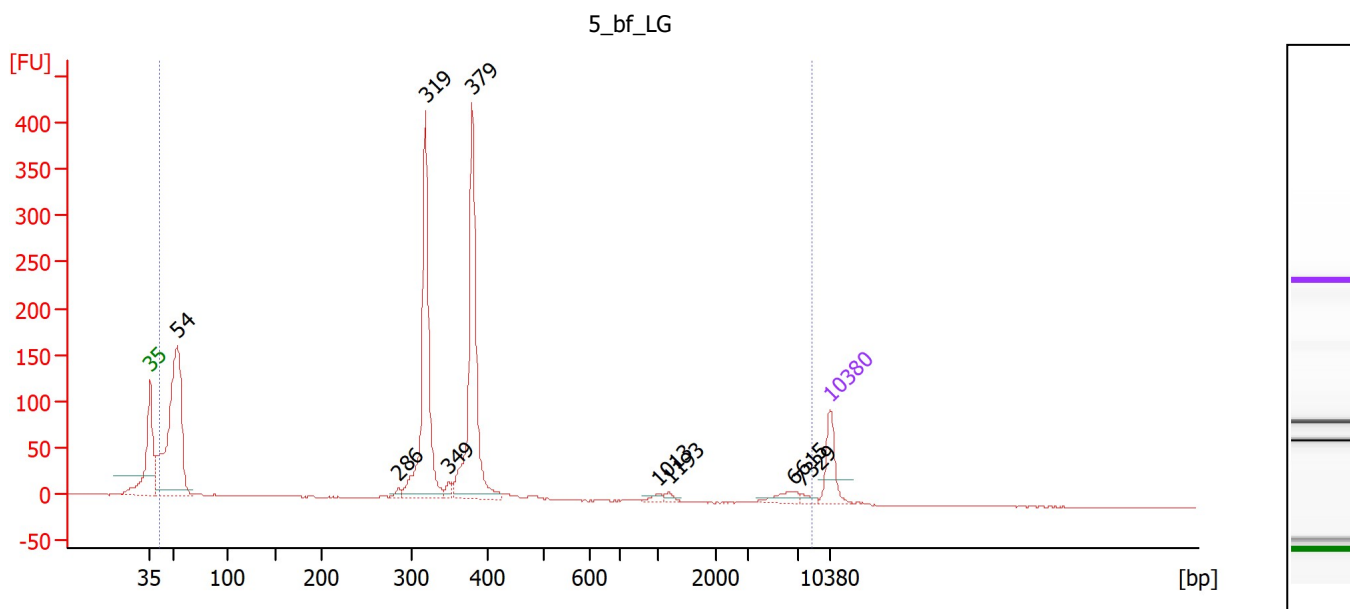Electropherogram Summary Continued ...**Overall Results for sample 9 : 5_bf_LG**

Number of peaks found: 9 Corr. Area 1: 1,633.7
 Noise: 0.4

Peak table for sample 9 : 5_bf_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	54	894.09	24,945.1	
3	286	13.65	72.2	
4	319	575.68	2,737.7	
5	349	21.22	92.2	
6	379	561.81	2,246.3	
7	1,013	10.01	15.0	
8	1,193	9.87	12.5	
9	6,615	26.00	6.0	
10	7,329	11.01	2.3	

Region table for sample 9 : 5_bf_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,633.7	97	553	100.0	2,122.41	30,199.8	42	8,520

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

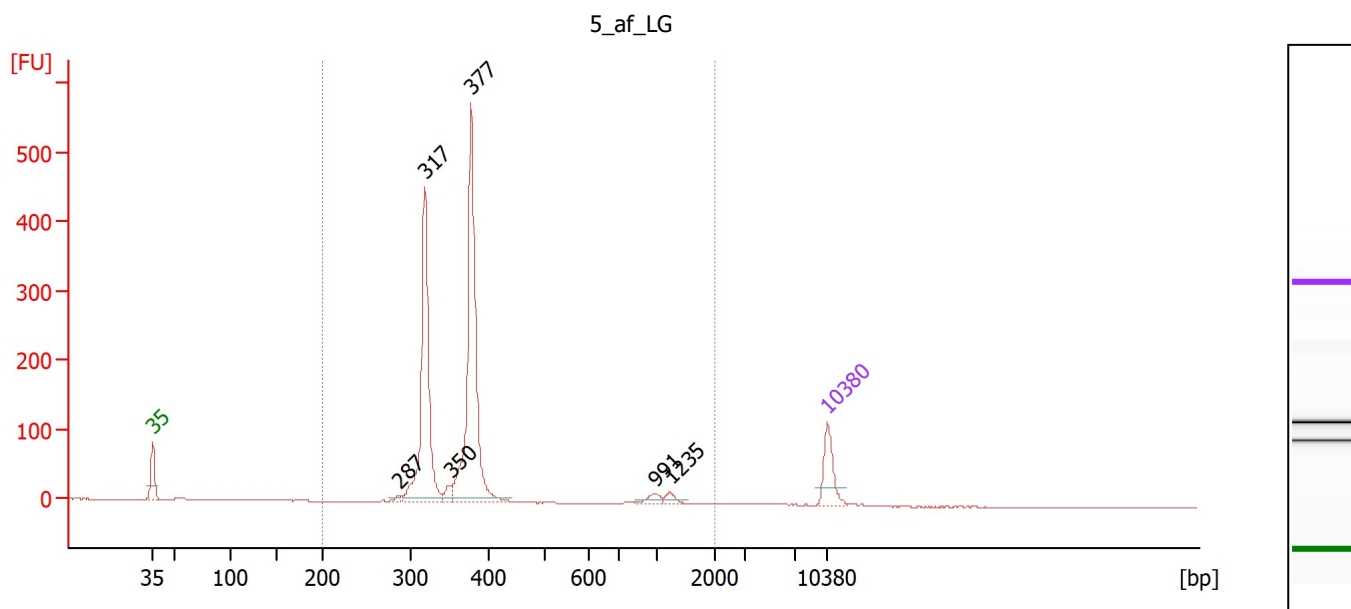Electropherogram Summary Continued ...**Overall Results for sample 10 : 5_af_LG**

Number of peaks found: 6 Corr. Area 1: 1,389.6
 Noise: 0.3

Peak table for sample 10 : 5_af_LG


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
2	287	8.12	42.9	
3	317	564.68	2,696.8	
4	350	24.12	104.3	
5	377	691.99	2,778.2	
6	991	19.08	29.2	
7	1,235	16.28	20.0	

Region table for sample 10 : 5_af_LG

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	1,389.6	99	384	40.7	1,323.78	5,598.7	200	1,985

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
Modified: 4/22/2026 9:05:52 AM

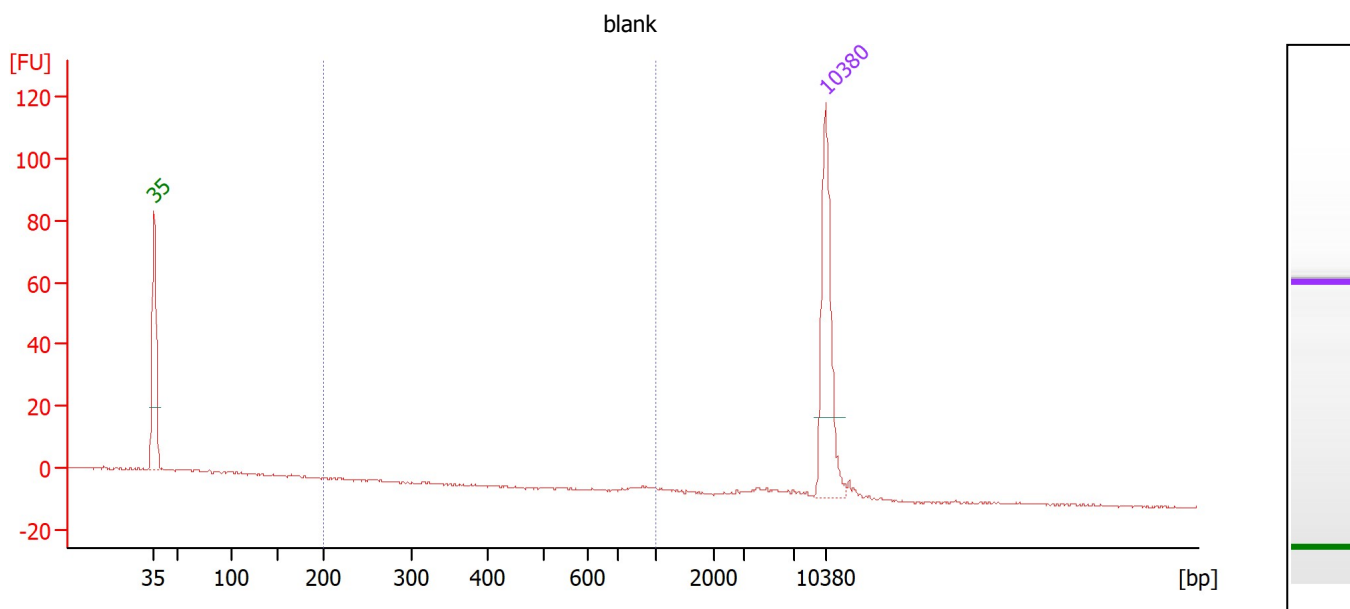Electropherogram Summary Continued ...**Overall Results for sample 11 : blank**


Number of peaks found: 0 Corr. Area 1: 0.5
Noise: 0.4

Region table for sample 11 : blank

Name	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Co From lo [bp]	To [bp]
Region 1	0.5	2	905	8.8	0.39	0.7	200	1,000

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
Modified: 4/22/2026 9:05:52 AM

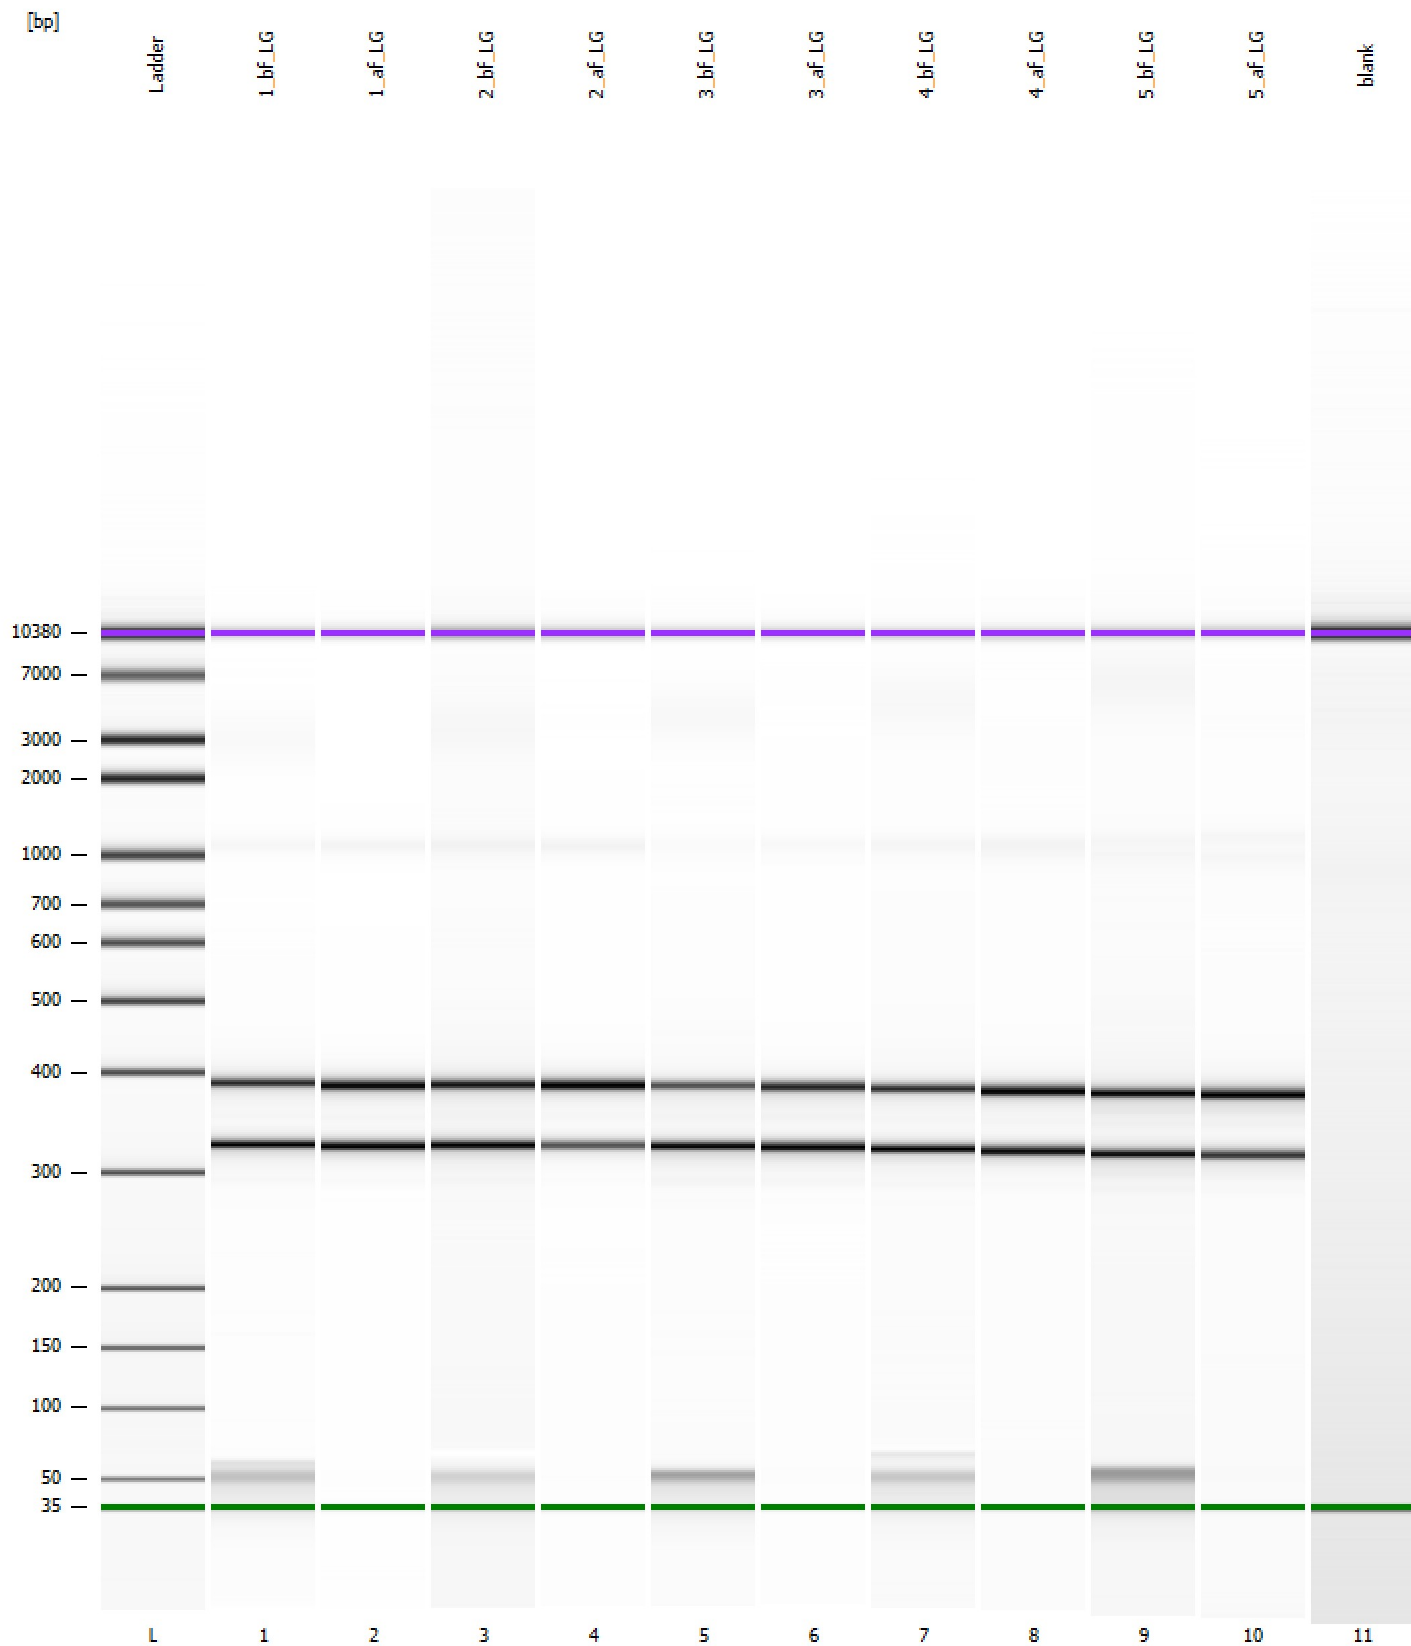
Gel Image

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
Modified: 4/22/2026 9:05:52 AM

Curves

Standard Curve

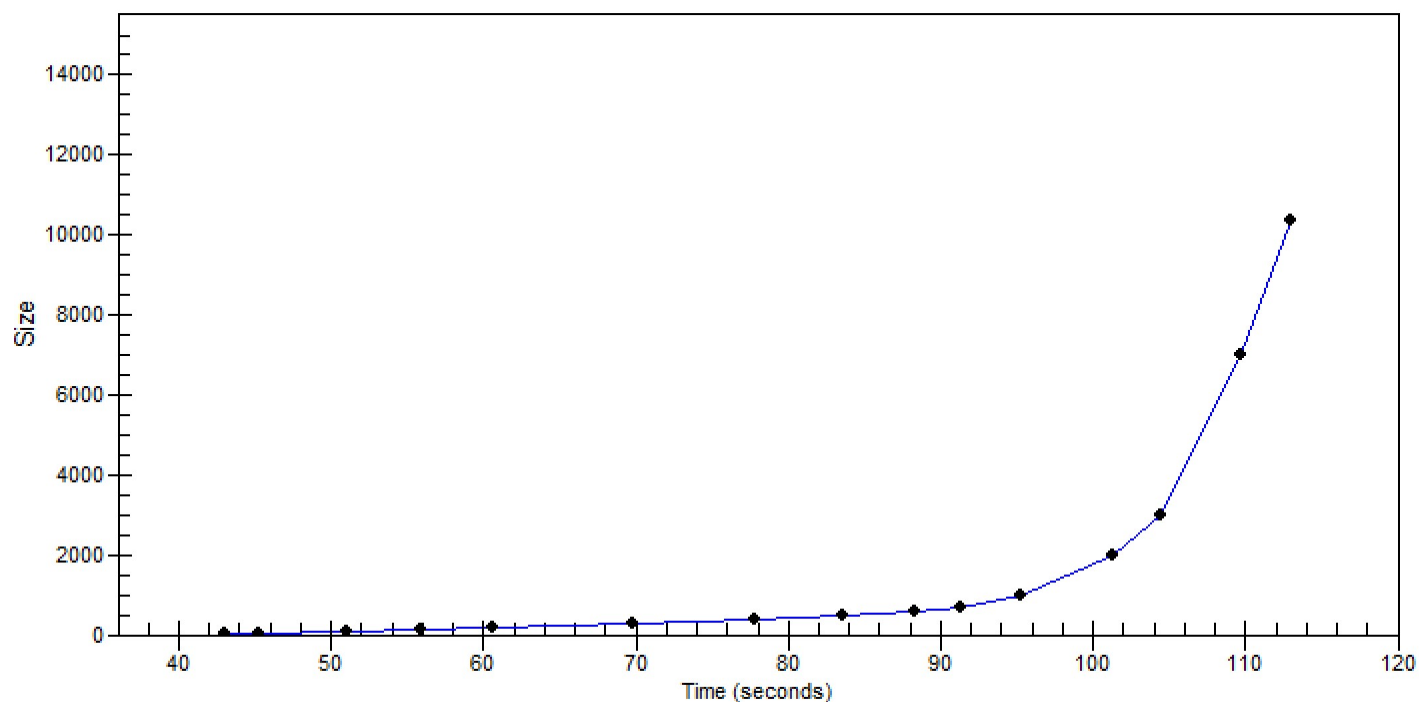

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad

Created: 4/22/2026 8:00:05 AM
 Modified: 4/22/2026 9:05:52 AM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		4/22/2026 8:41:27 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\Data\2026-04-22\2100 expert_High Sensitivity DNA Assay_DE54107817_2026-04-22_08-00-06.xad)		Instrument	Run		4/22/2026 8:00:11 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Product Number : G2939A		Instrument	Run		4/22/2026 8:00:11 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Name :		Instrument	Run		4/22/2026 8:00:11 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Vendor : Agilent Technologies		Instrument	Run		4/22/2026 8:00:11 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Serial# : DE54107817		Instrument	Run		4/22/2026 8:00:11 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Firmware : C.01.069		Instrument	Run		4/22/2026 8:00:11 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC
Cartridge : Electrode		Instrument	Run		4/22/2026 8:00:11 AM	(GMT +02:00) W. Europe Standard Time	bioanalyzer	GC-BIOANALYS-PC