
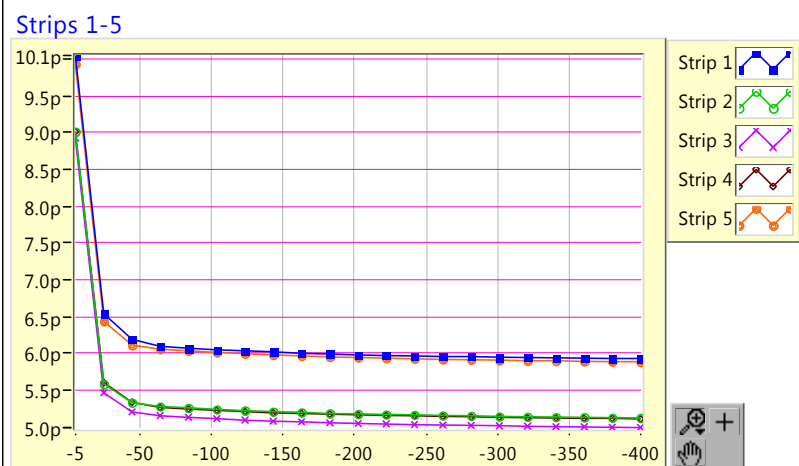


View_measurement.vi
C:\Users\root\Desktop\ProductionDB_040629_INP_modification_Oct_2015\Istrip-measurement\
View_measurement.vi
Last modified on 10/12/2015 at 3:49 PM
Printed on 11/24/2015 at 3:18 PM

CV 33305010000619

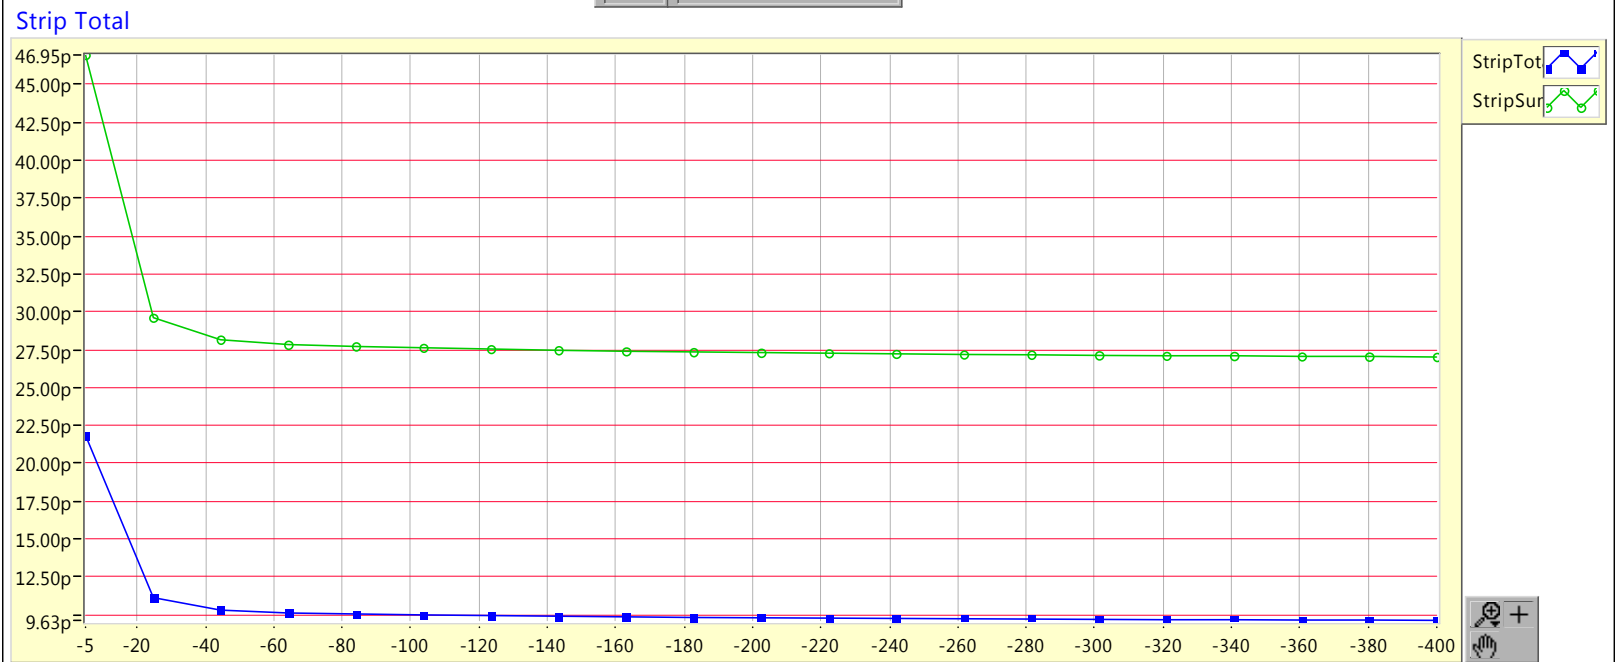

Output Array

0	-5.00E+0	1.01E-11
0	-2.48E+1	6.54E-12
0	-4.45E+1	6.19E-12