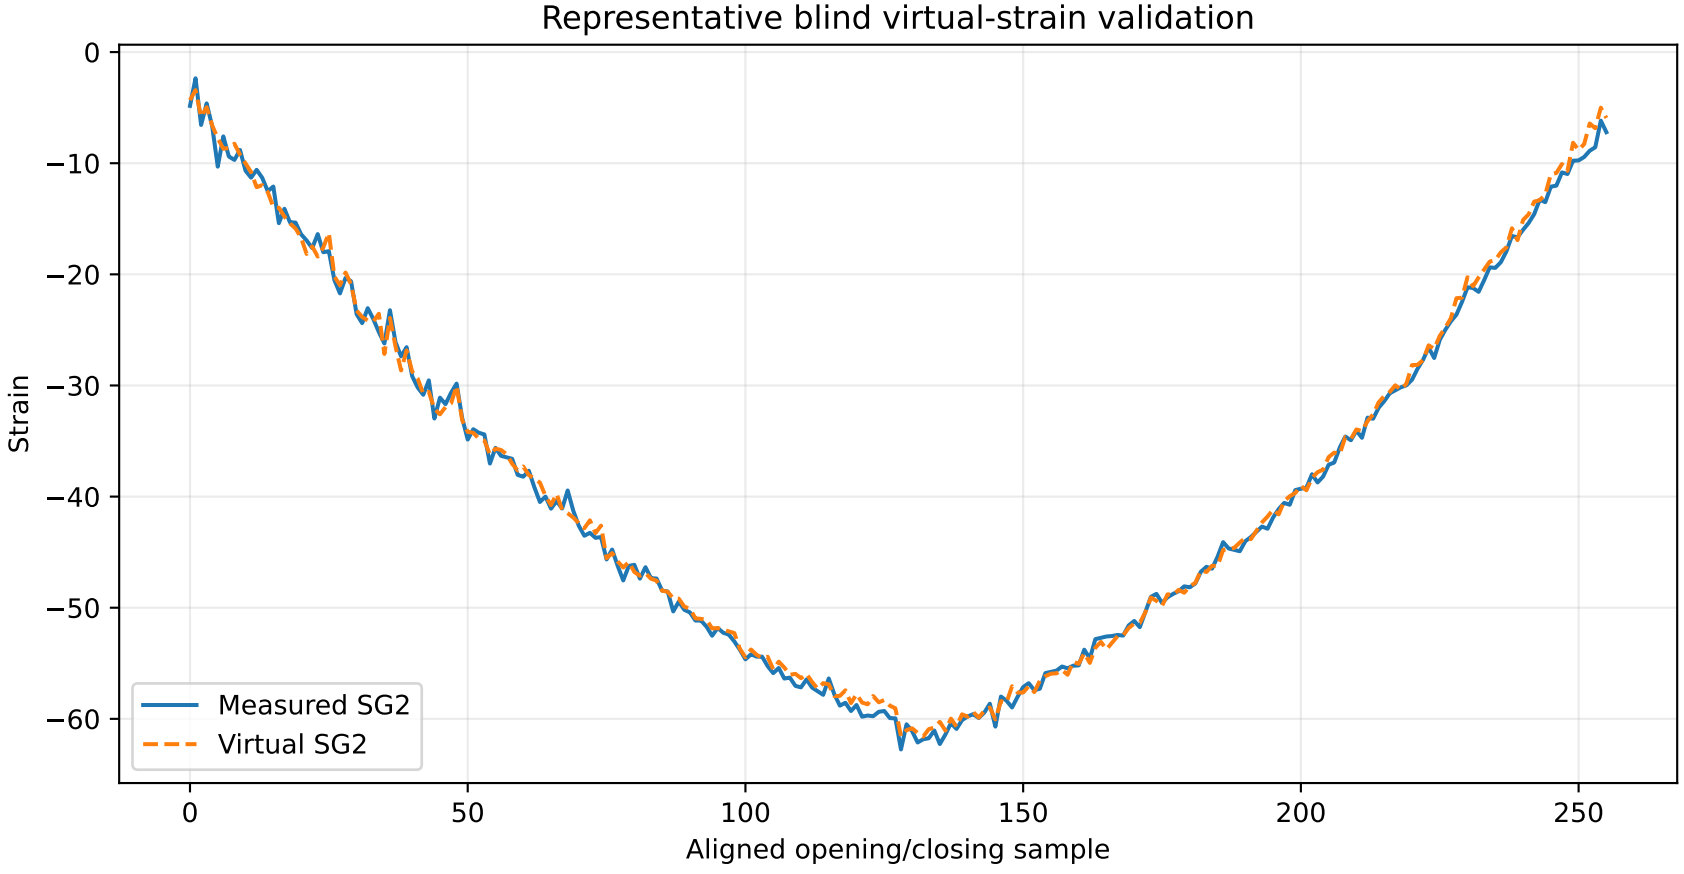
Representative blind virtual-strain validation
Strain
Aligned opening/closing sample
Measured SG2
Virtual SG2
0
−10
−20
−30
−40
−50
−60
0
50
100
150
200
250