

Screen Layout for the Touch screen

JKUAT Ventilator

● ON

Calibration ●

● OFF

AC/CMV/SIMV	CPAP/PEEP	PC	PS	Maintenance
-------------	-----------	----	----	-------------

This could be an area for display of the parmeters that are measured

Tabs for Modes
of control →

Once the ventilator is turned ON,


- It will prompt for calibration
- It will not allow for selection of ventilation mode before calibration is done
- Once the calibration is done, the ventilator displays a message asking for the operator to set the mode of ventilation
- Once the ventilation mode (Tab) is selected, the user will be prompted to set the parameters for the selected mode of ventilation
- When set, the ventilator will open a window to allow for confirmation of ventilation parameters.
- Every time a parameter is set, the operator has to press a next (or back) button or will be promoted by a dialogue box, say, YES or NO
- When selected, each of the ventilation mode will open the respective parameters to be set on the screen

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS SURFACE FINISH: TOLERANCES: LINEAR: ANGULAR:				FINISH:		DEBURR AND BREAK SHARP EDGES		DO NOT SCALE DRAWING		REVISION	
DRAWN	Kabini	SIGNATURE	DATE			TITLE					
CHECK'D											
APP'D											
MFG											
Q.A											
				MATERIAL:		DWG NO. Suggested Screen Layout					
WEIGHT:						SCALE: 1:2				SHEET 1 OF 9	

B	<ol style="list-style-type: none"> Once the calibration is done, the ventilator displays a message asking for the operator to set the mode of ventilation Once the ventilation mode (Tab) is selected, the user will be prompted to set the parameters for the selected mode of ventilation When set, the ventilator will open a window to allow for confirmation of ventilation parameters.
A	<ol style="list-style-type: none"> Every time a parameter is set, the operator has to press a next (or back) button or will be promoted by a dialogue box, say, YES or NO When selected, each of the ventilation mode will open the respective parameters to be set on the screen

1. It will prompt for calibration
2. It will not allow for selection of ventilation mode before calibration is done
3. Once the calibration is done, the ventilator displays a message asking for the operator to set the mode of ventilation
4. Once the ventilation mode (Tab) is selected, the user will be prompted to set the parameters for the selected mode of ventilation
5. When set, the ventilator will open a window to allow for confirmation of ventilation parameters.
6. Every time a parameter is set, the operator has to press a next (or back) button or will be promoted by a dialogue box, say, YES or NO
7. When selected, each of the ventilation mode will open the respective parameters to be set on the screen


UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS SURFACE FINISH: TOLERANCES: LINEAR: ANGULAR:				FINISH:		DEBURR AND BREAK SHARP EDGES		DO NOT SCALE DRAWING		REVISION	
NAME		SIGNATURE		DATE				TITLE			
DRAWN Kabini											
CHK'D											
APPV'D											
MFG											
Q.A						MATERIAL:		DWG NO. Suggested Screen Layout		A3	
						WEIGHT:		SCALE: 1:2		SHEET 1 OF 9	

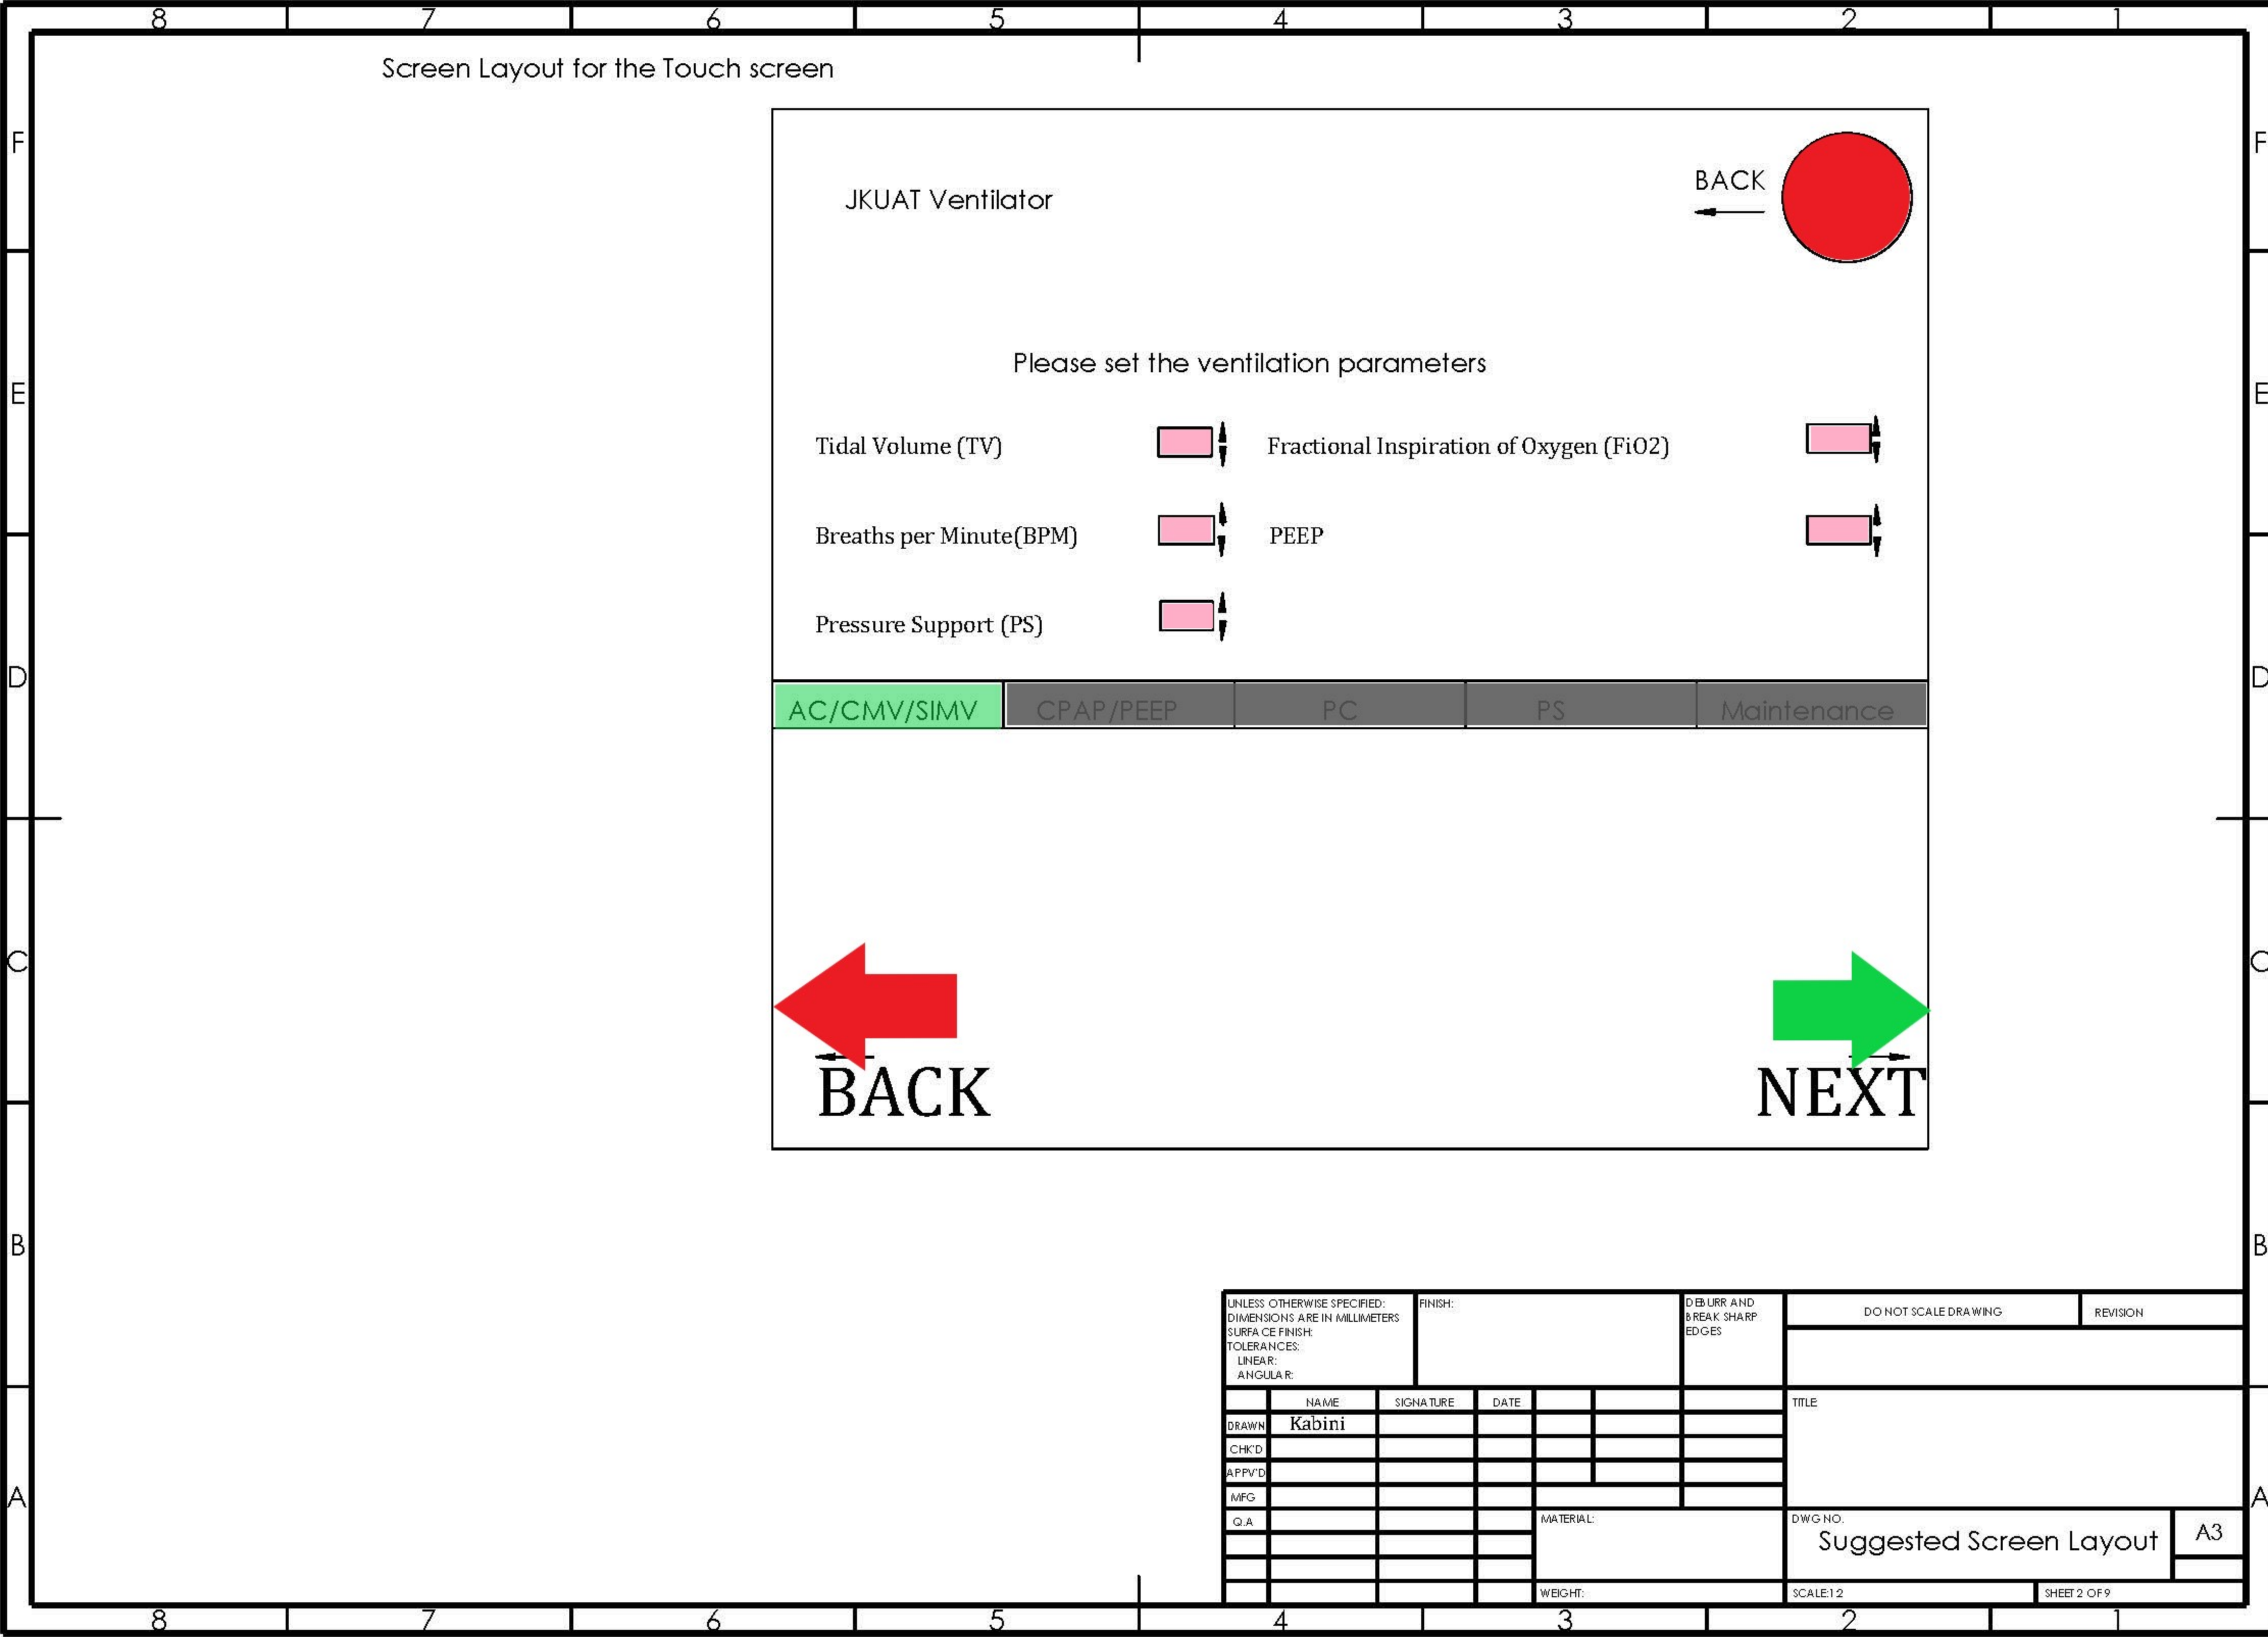

Screen Layout for the Touch screen

JKUAT Ventilator

BACK



Please set the ventilation parameters

Tidal Volume (TV)



Fractional Inspiration of Oxygen (FiO2)



Breaths per Minute (BPM)



PEEP



Pressure Support (PS)



AC/CMV/SIMV

CPAP/PEEP

PC

PS

Maintenance




BACK



NEXT


UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS SURFACE FINISH: TOLERANCES: LINEAR: ANGULAR:				FINISH:			DEBURR AND BREAK SHARP EDGES			DO NOT SCALE DRAWING			REVISION						
	NAME		SIGNATURE		DATE					TITLE									
DRAWN	Kabini																		
CHK'D																			
APPV'D																			
MFG																			
Q.A																			
							MATERIAL:			DWG NO. Suggested Screen Layout					A3				
							WEIGHT:			SCALE:1:2					SHEET 2 OF 9				

Screen Layout for the Touch screen

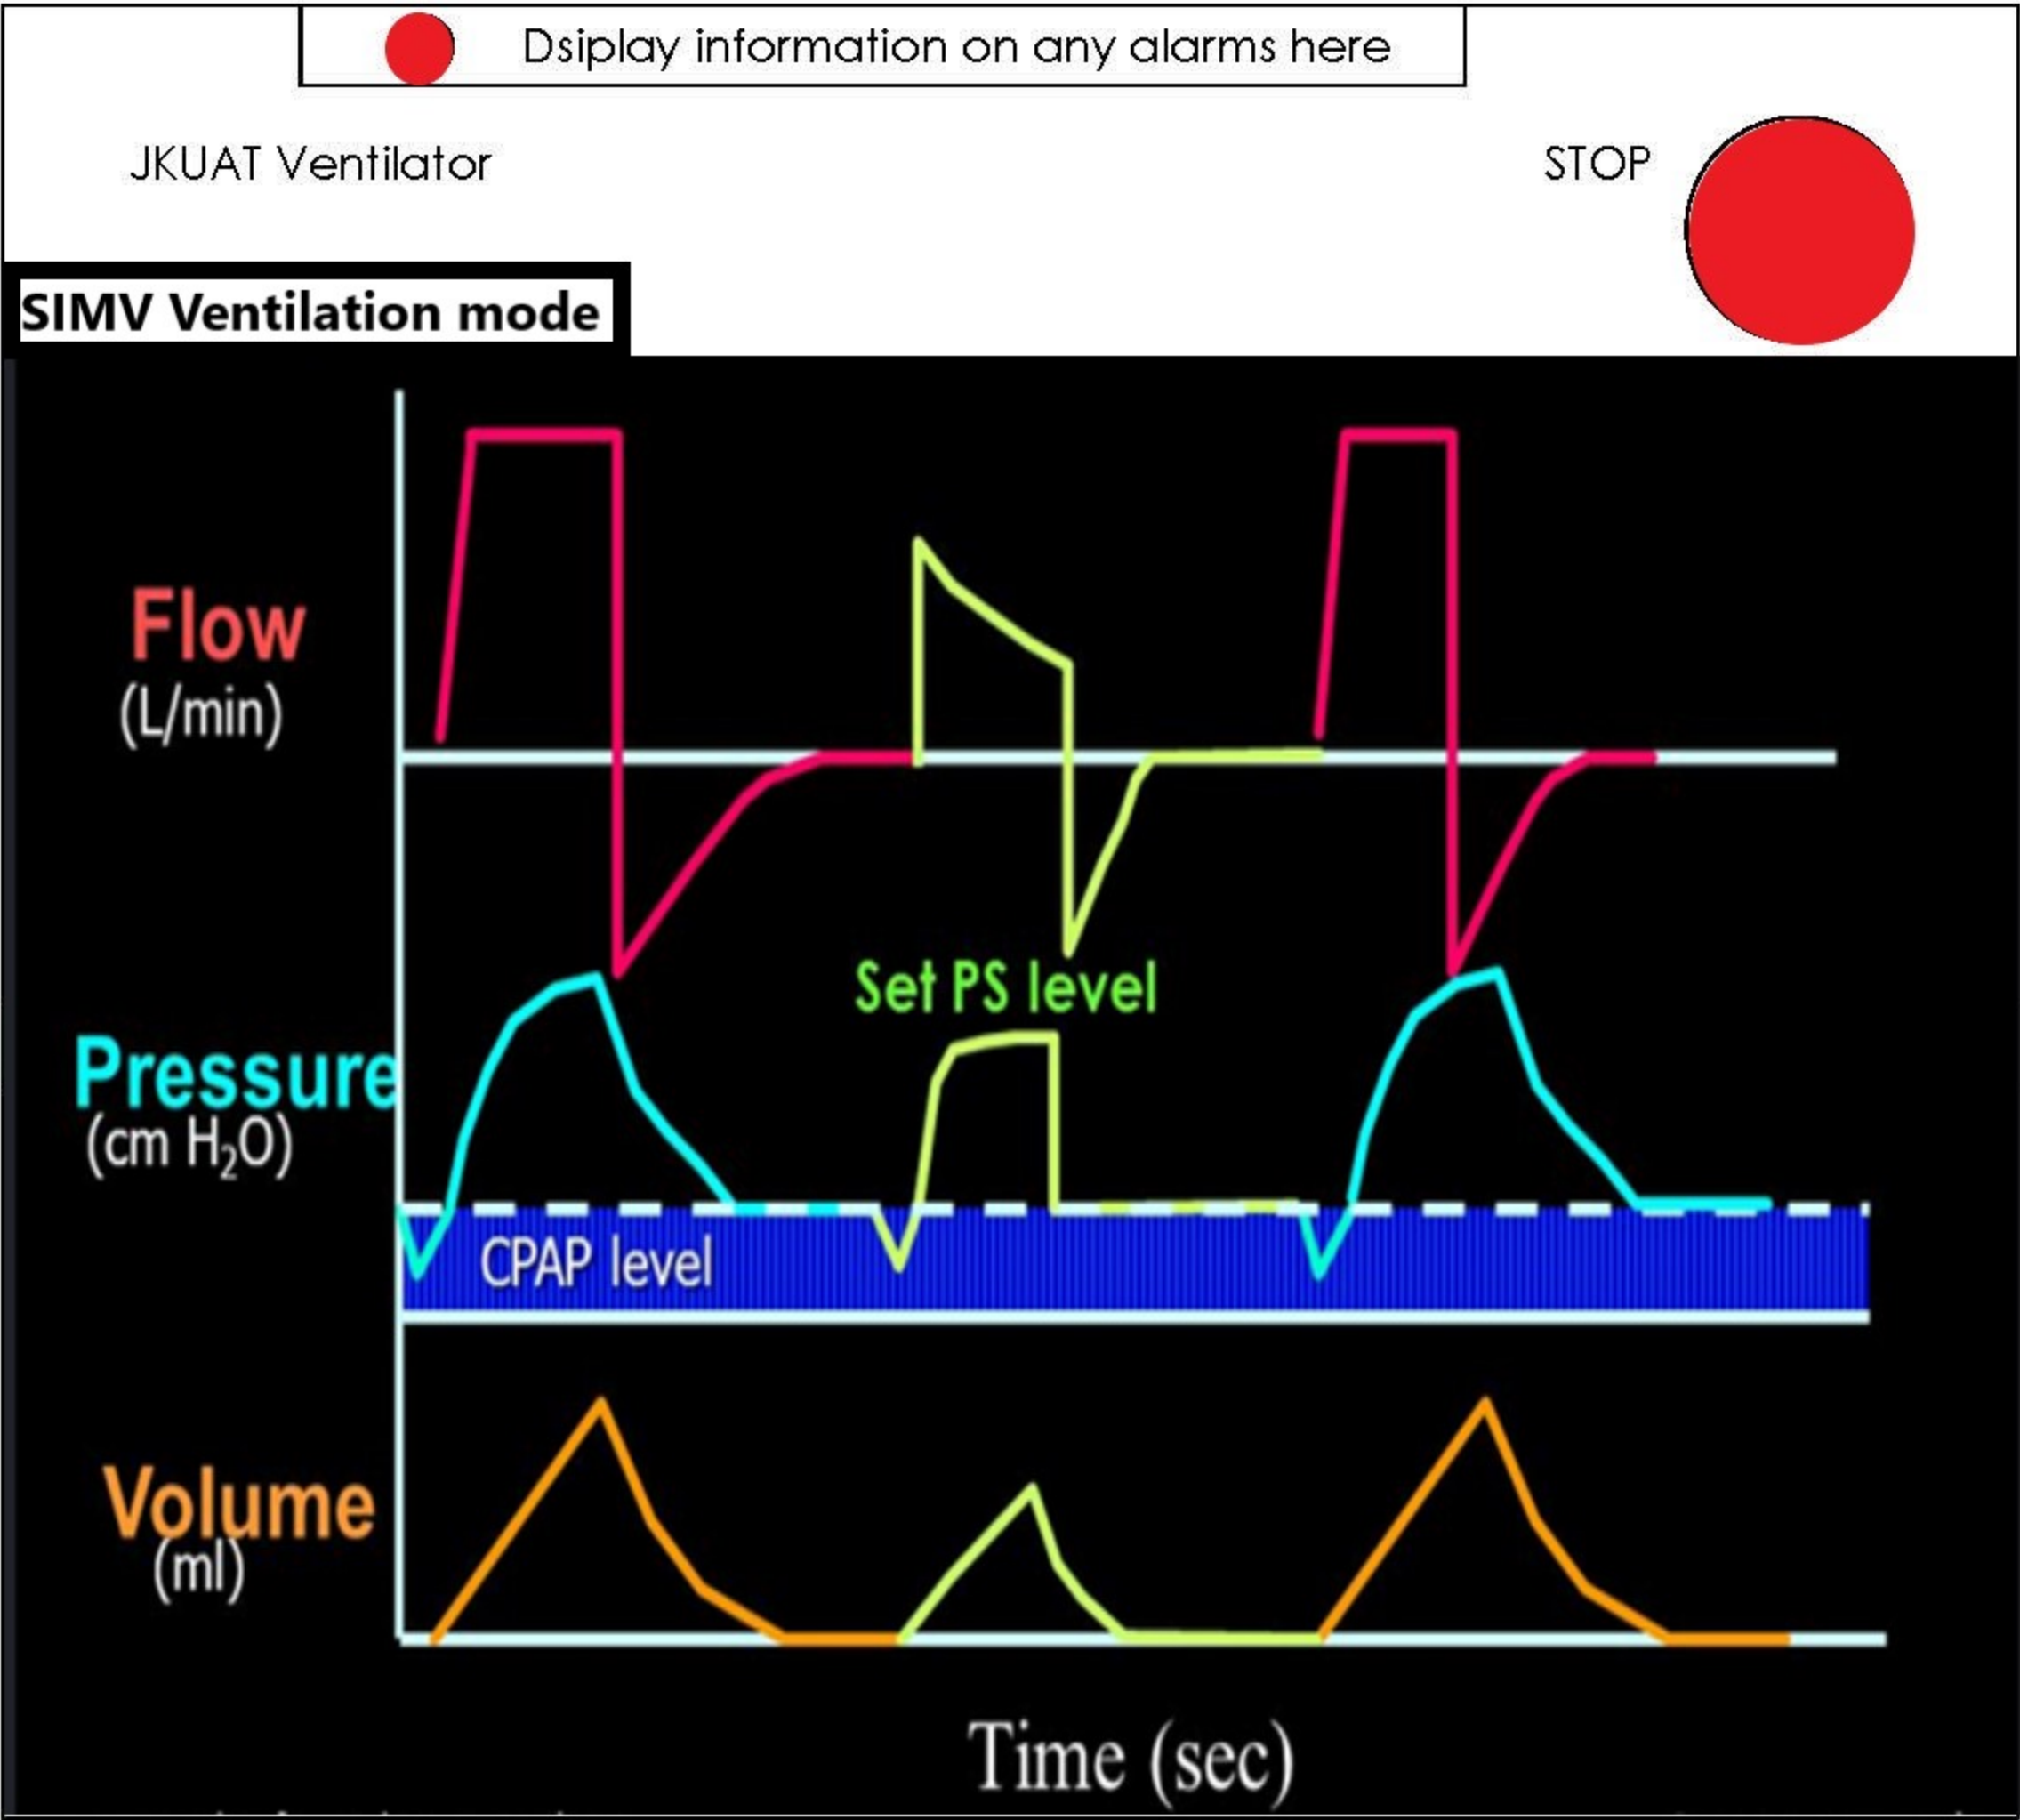

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS SURFACE FINISH: TOLERANCES: LINEAR: ANGULAR:				FINISH:		DEBURR AND BREAK SHARP EDGES	DO NOT SCALE DRAWING		REVISION		
	NAME	SIGNATURE	DATE				TITLE				
DRAWN	Kabini										
CHK'D											
APPV'D											
MFG											
Q.A				MATERIAL:			DWG NO. Suggested Screen Layout				A3
				WEIGHT:			SCALE:1:2			SHEET 4 OF 9	

STOP




Set the parameters for CPAP ventilation mode

Maintenance

Display the set parameters here

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS SURFACE FINISH: TOLERANCES: LINEAR: ANGULAR:				FINISH:		DEBURR AND BREAK SHARP EDGES		DO NOT SCALE DRAWING		REVISION	
		NAME		SIGNATURE		DATE				TITLE	
DRAWN		Kabini									
CHK'D											
APPV'D											
MFG											
Q.A						MATERIAL:		DWG NO.		A3	
								Suggested Screen Layout			
						WEIGHT:		SCALE: 1:2		SHEET 5 OF 9	

Screen Layout for the Touch screen

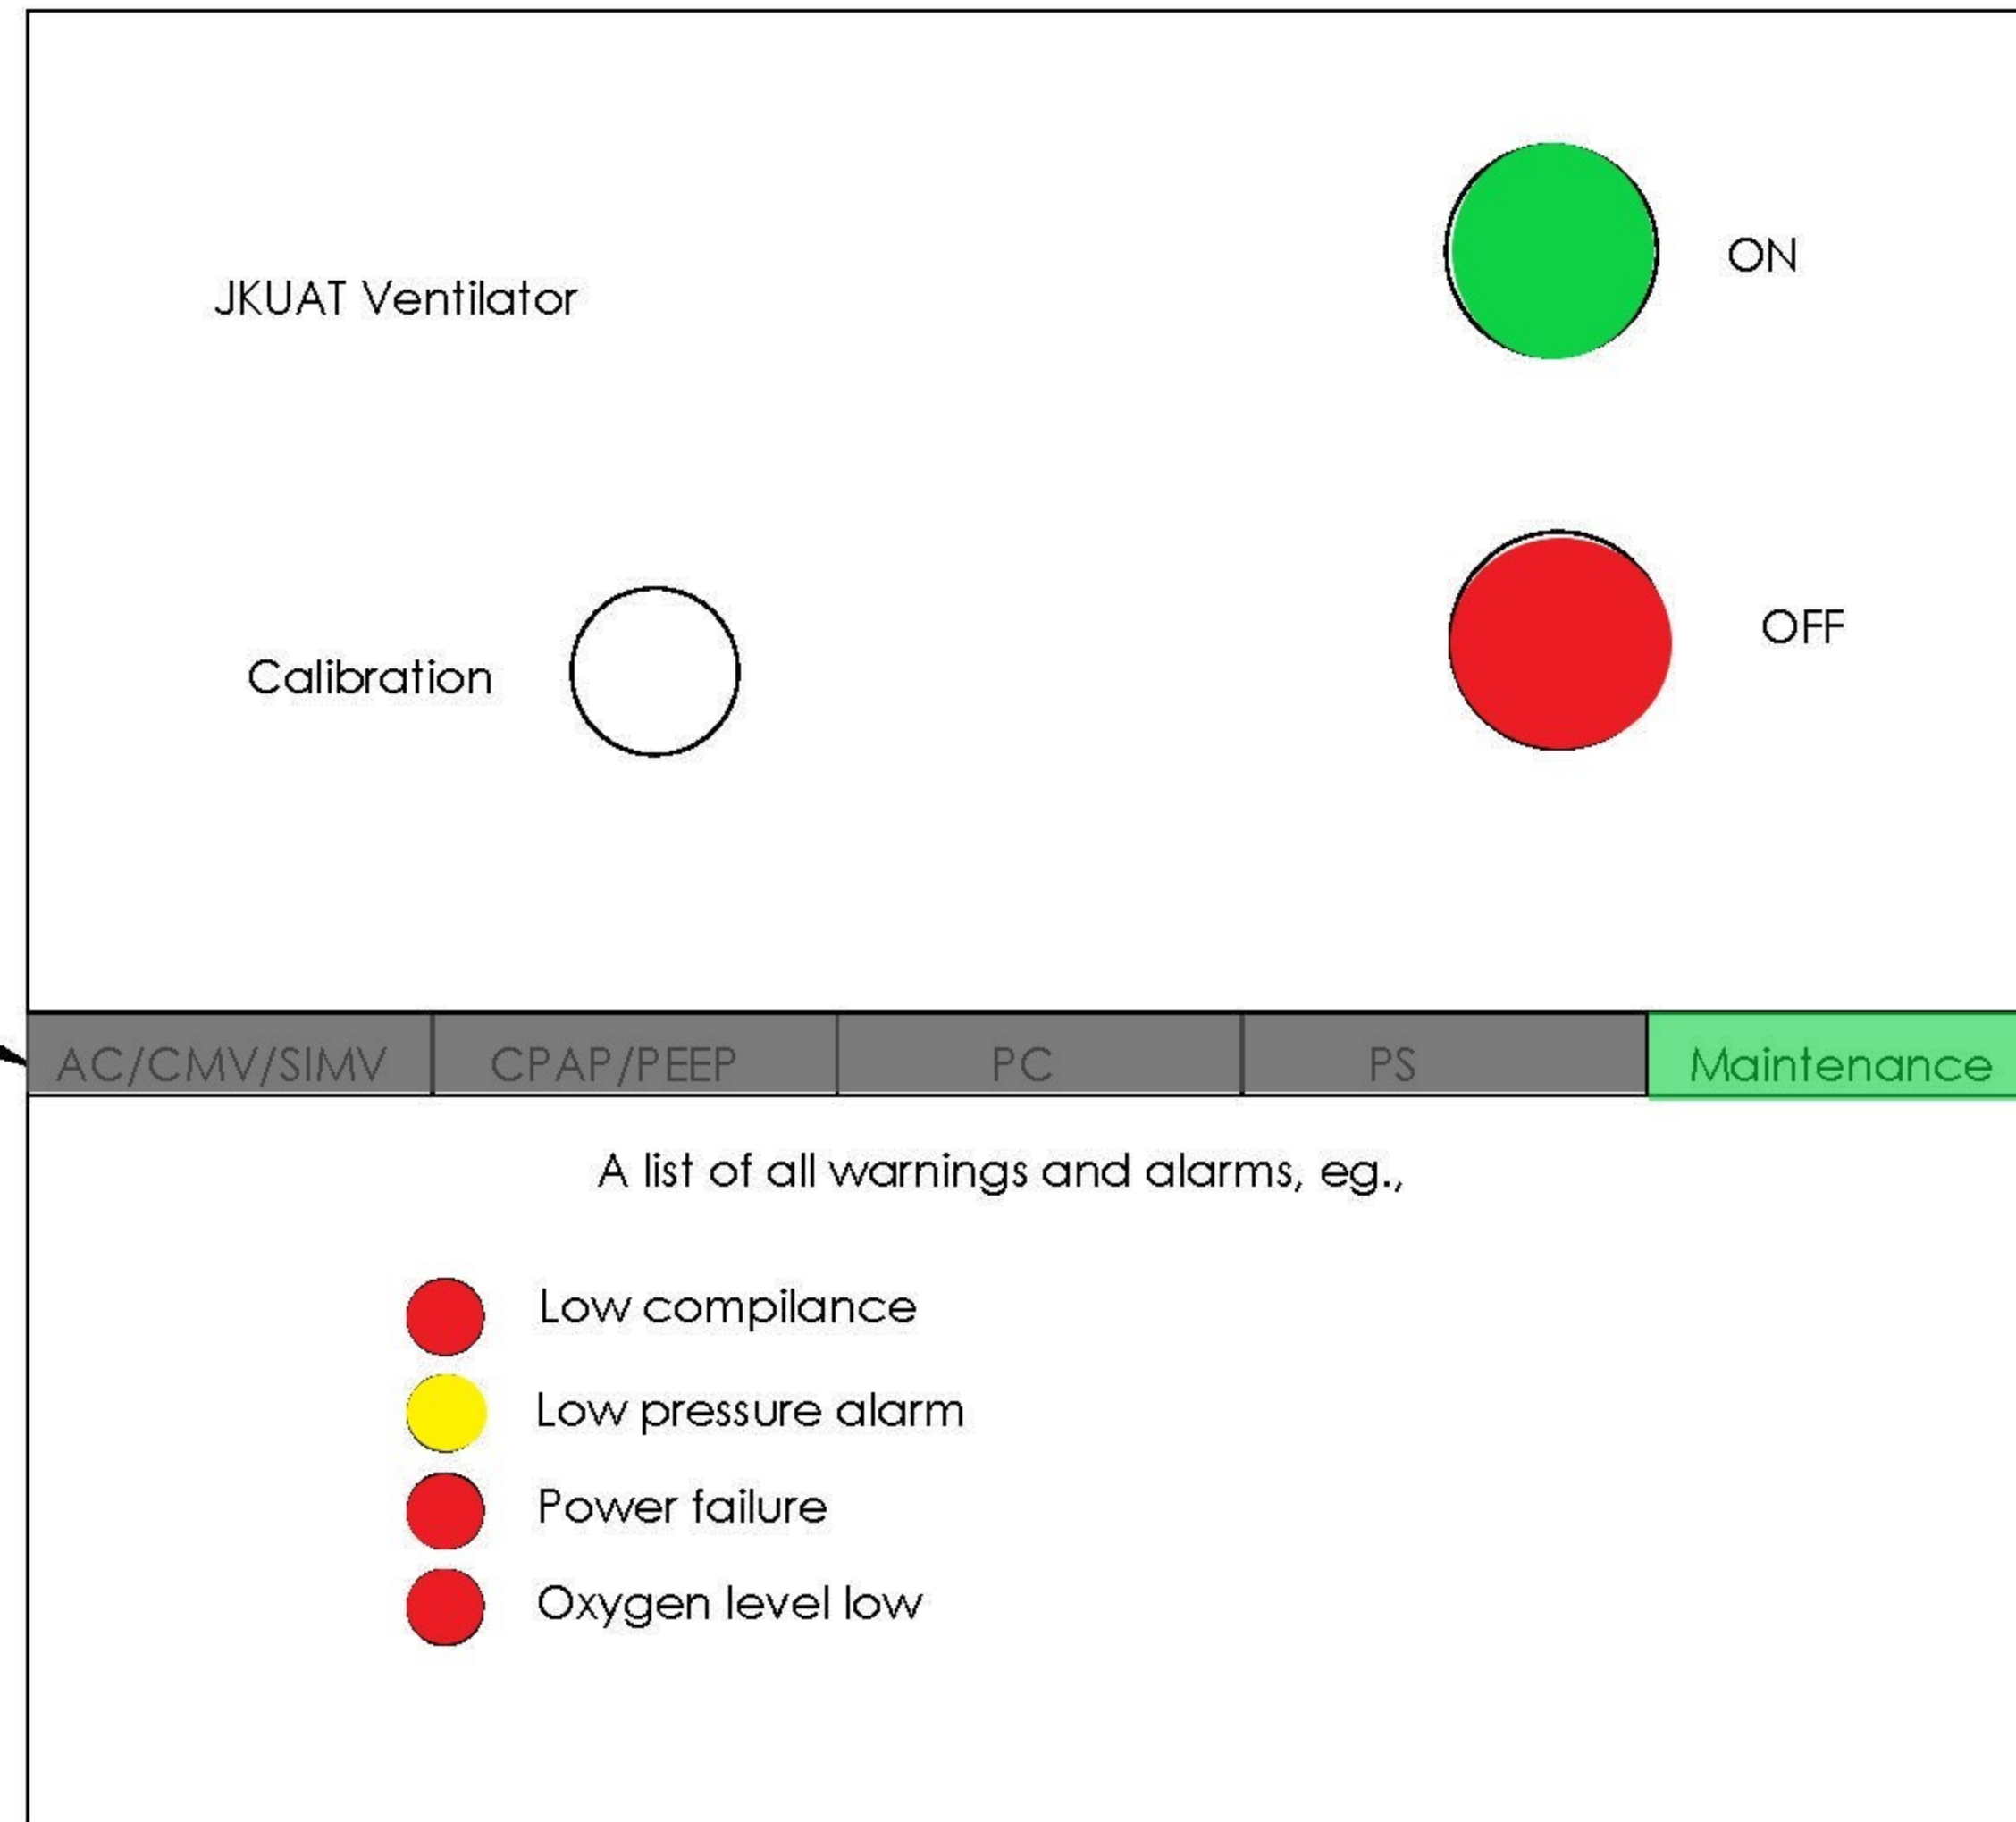

Once the ventilator is turned ON,

1. It will prompt for calibration
2. It will not allow for selection of ventilation mode before calibration is done
3. Once the calibration is done, the ventilator displays a message asking for the operator to set the mode of ventilation
4. Once the ventilation mode (Tab) is selected, the user will be prompted to set the parameters for the selected mode of ventilation
5. When set, the ventilator will open a window to allow for confirmation of ventilation parameters.
6. Every time a parameter is set, the operator has to press a next (or back) button or will be promoted by a dialogue box, say, YES or NO
7. When selected, each of the ventilation mode will open the respective parameters to be set on the screen

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN MILLIMETERS SURFACE FINISH: TOLERANCES: LINEAR: ANGULAR:				FINISH:				DEBURR AND BREAK SHARP EDGES				DO NOT SCALE DRAWING				REVISION							
		NAME		SIGNATURE		DATE								TITLE									
DRAWN		Kabini																					
CHK'D																							
APPV'D																							
MFG																							
Q.A								MATERIAL:				DWG NO. Suggested Screen Layout						A3					
								WEIGHT:				SHEET 10 OF 10											