

Preliminary data 1: 10-day proof-of-concept open continuous cultivation of *Caldimonas thermodepolymerans* in turbidostat


Microbial Bioengineering Laboratory (data collected by Dr. Miguel Silva)

Department of Experimental Biology, Faculty of Science,
Masaryk University, Brno, Czech Republic

MOTIVATION

- The purpose of this 10-day experiment was to verify whether *C. thermodepolymerans* can be cultured in continuous mode (turbidostat) at 50°C in open non-sterile conditions without contamination of the culture with another organism.
- The minimal medium containing 5 g/L xylose was not sterilised prior to cultivation, the glass bioreactor vessel and connecting tubes were briefly rinsed with 70% ethanol prior to cultivation, the Chi.Bio reactor vessel containing the *C. thermodepolymerans* culture was connected to the outside environment via two outlets without air filters for the whole course of the experiment (open culture).

BIOREACTOR SETUP

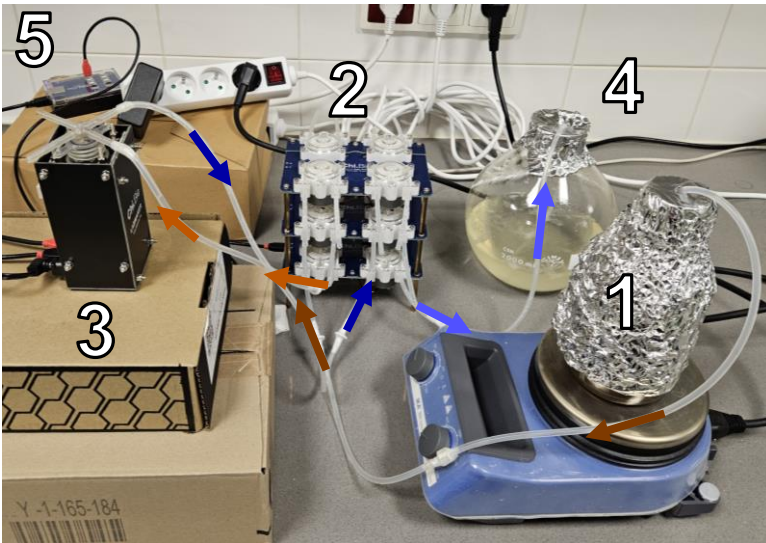

Chi.bio minibioreactor set-up for open continuous *Caldimonas* culture at 50°C.

- 1 – Heating plate keeps the minimal medium with 5 g/L D-xylose at desired temperature (50 °C).
- 2 – Peristaltic pump for turbidostatic mode to regulate OD. Flows the medium from the medium bottle (1) to the reactor (3) and takes excess medium to waste (4). Flow represented by arrows: brown → orange → dark blue → light blue.
- 3 – Chi.bio minireactor that contains heating plate, magnetic stirrer and LED for OD measurement
- 4 – Waste bottle
- 5 – Chi.bio microcontroller controls the reactor and pumps. The microcontroller is connected to a computer with a graphical interface (6).
- 6 – Graphical interface allows to readily set cultivation parameters and monitor them in real-time.

6

Device: M0

M0 M1 M2 M3 M4 M5 M6 M7

Scan Devices

Experiment

Running

Start Stop Reset

Experiment Start Time: 2023-11-17 20:34:57

OD Regulation

Switch Dither OD

OD: Measure Current: 1.625 Target: 1.500 New: 0 Set

OD Zero: Current: 13535 Actual: 0 Measured: 0 Set

Raw: 2126

Volume (ml): Current: 20.000 New: 0 Set

Light Outputs

LED	Current	Default	New	Set	Switch
395nm LED	0.100	0.100	0	Set	Switch
457nm LED	0.100	0.100	0	Set	Switch
500nm LED	0.100	0.100	0	Set	Switch
523nm LED	0.100	0.100	0	Set	Switch
595nm LED	0.100	0.100	0	Set	Switch
623nm LED	0.100	0.100	0	Set	Switch
6500K LED	0.100	0.100	0	Set	Switch
650nm LASER	0.500	0.500	0	Set	Switch
280nm UV	0.500	0.500	0	Set	Switch

Spectrometer

Full Spectral Measurement:

Measure Gain: 1x

410nm = 0 440nm = 0 470nm = 0

510nm = 0 550nm = 0 583nm = 0

620nm = 0 670nm = 0 Clear = 0

Measure Fluorescent Proteins (FPs)

Thermometry

T (air, external): Measure Current: 34.063

T (air, internal): Measure Current: 41.250

T (liquid): Measure Current: 50.210

Thermostat Target: 50.000 New: 0 Set Switch

Stir/Pump

Pump	Current	New Rate	Set	Switch	Direction
P1 (IN)	0.000	0	Set	Switch	Direction
P2 (OUT)	0.000	0	Set	Switch	Direction
P3	0.000	0	Set	Switch	Direction
P4	0.000	0	Set	Switch	Direction
Stirring	1.000	0	Set	Switch	


Optogenetics

Light 395/30 Current: LEDD 0 New: 0 Switch


Custom Program Program C1 Status: 0.000 New: 0 Switch

RESULTS

Real time monitoring of the continuous culture

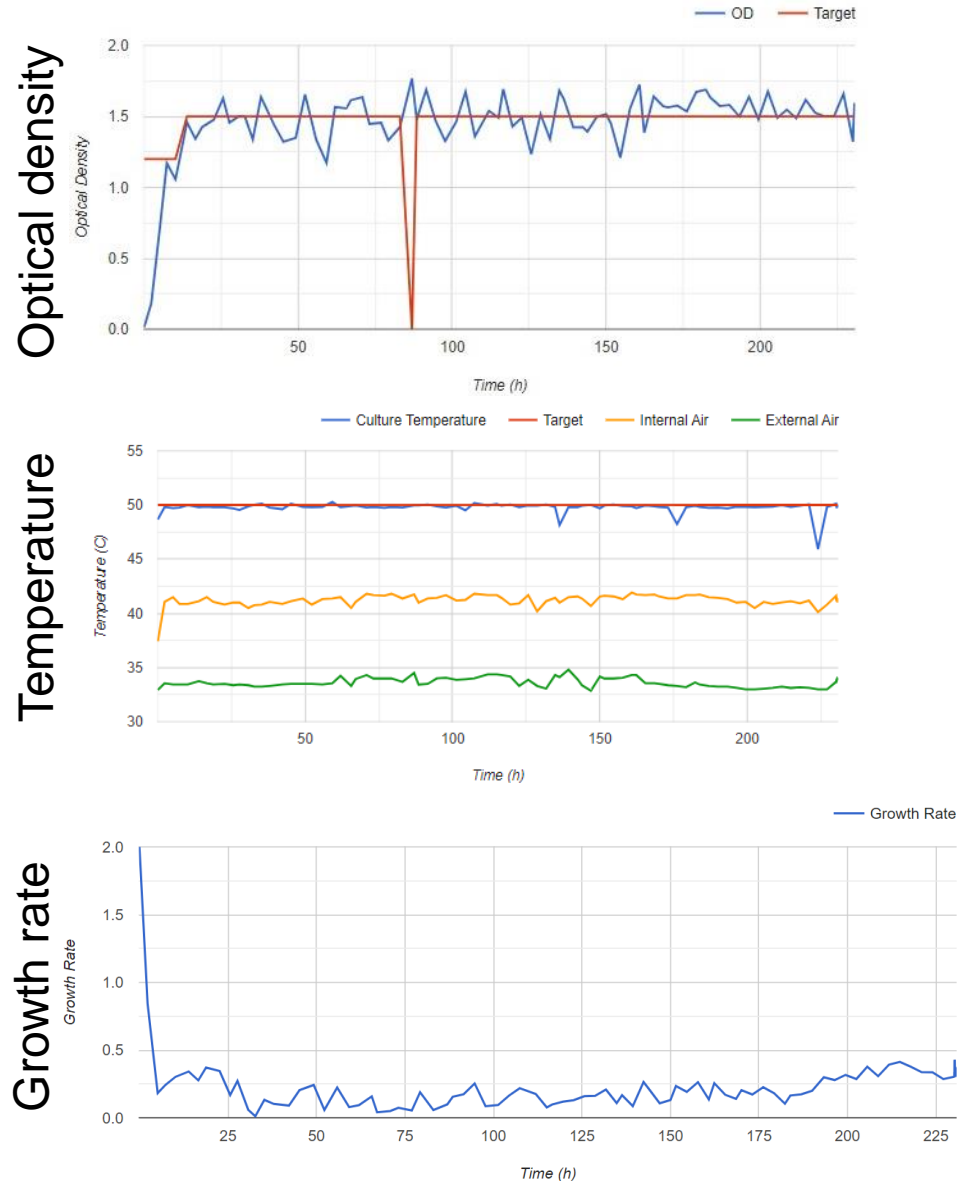


Post cultivation growth data

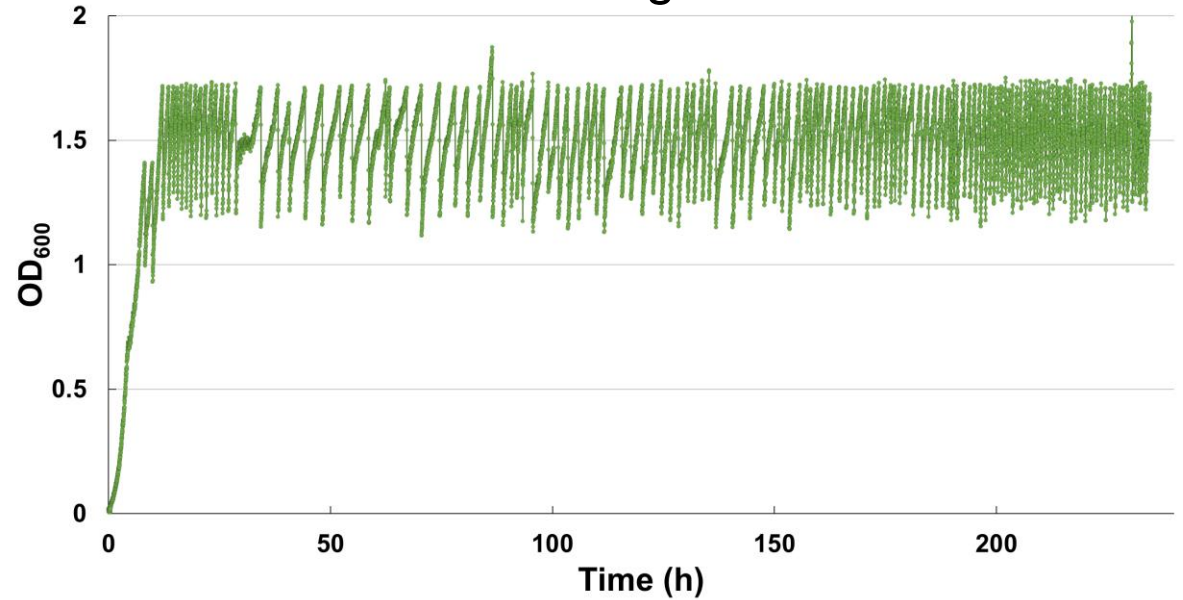


- Stable uninterrupted growth for 10 days.
- Graphical interface allows to spot deviations/errors that can be readily fixed without cancelling the cultivation.
- All data is collected, saved for posterior data analysis.

RESULTS: NO CONTAMINATION OBSERVED AFTER 10 DAYS OF THE CULTURE

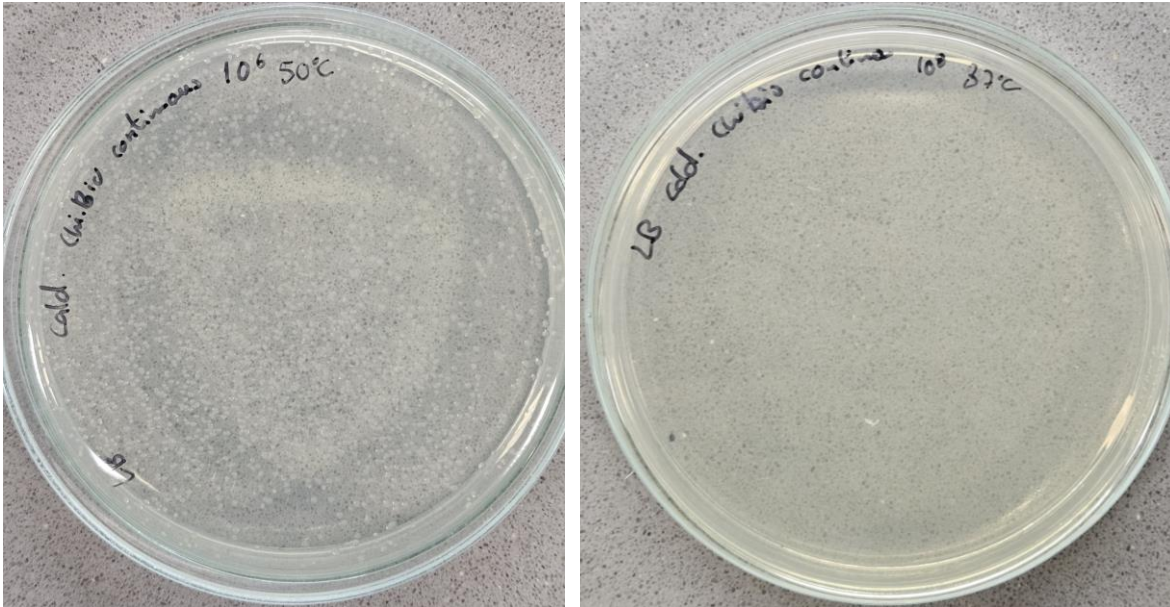

- Cells were plated on LB agar after 10 days of continuous cultivation and incubated at 50 °C or 37 °C for 24 h.
 - Numerous colonies were obtained at 50 °C, while there were no visible colonies on plate incubated 24 h at 37 °C (slower growing *Caldimonas* colonies became visible later after 48 h).
- This result indicates no contamination with mesophilic organisms.

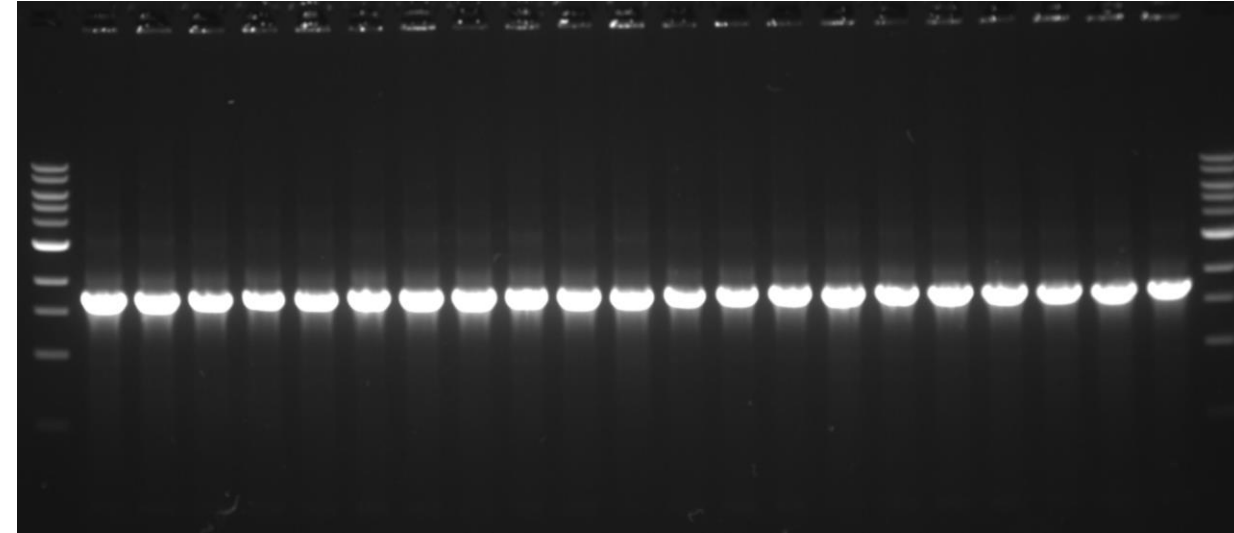

- Colonies from 50°C plate were genotyped using *phaC* gene *Caldimonas thermodepolymerans* specific primers
 - Primer forward: ATGACACAACGCTCTGCACCCC.
 - Primer reverse: TCAGGCCCGTTTCCTTGACGTAG
 - Annealing: 60 °C
 - Extension: 1 min/kb
 - Expected amplicon size: 1.7 kb
- 21 randomly picked colonies were positive, which indicates that the turbidostat culture contained only *C. thermodepolymerans* at the end of the experiment.



CONCLUSION

No contamination with mesophilic or thermophilic microflora was observed at the end of the 10-day proof-of-concept open continuous culture with *C. thermodepolymerans* grown on D-xylose in non-sterile minimal medium at 50°C.