



Waters and Lange (2015) Hygrometer:
Quoted SEE \pm 0.35 wt%, R²=0.98 on calibration data

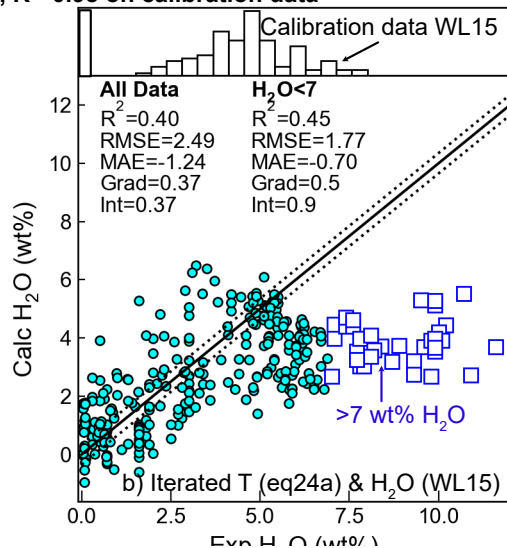

Putirka (2008) eq 24a Thermometer :
Quoted SEE \pm 36°C, R²=0.93 on global data

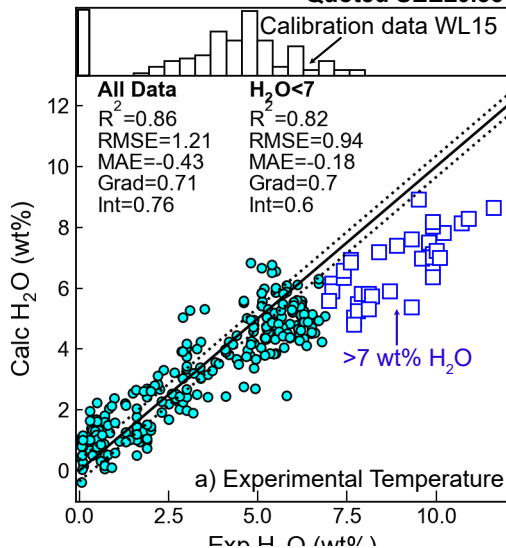