

LABORATORY OPERATIONS & PERFORMANCE DASHBOARD

Total Samples 1K	Completed Rate 84%	Failed Rate 16%	Approval Rate 100%	Average Duration 7.0 Days
---------------------	-----------------------	--------------------	-----------------------	------------------------------

Lab_Status

Approved

Department

Human Resources

Research & Development

Sales

Test_Category

Healthcare Representative

Human Resources

Laboratory Technician

Manager





Manufacturing Director

Research Director

Research Scientist

Sales Executive

Sales Representative

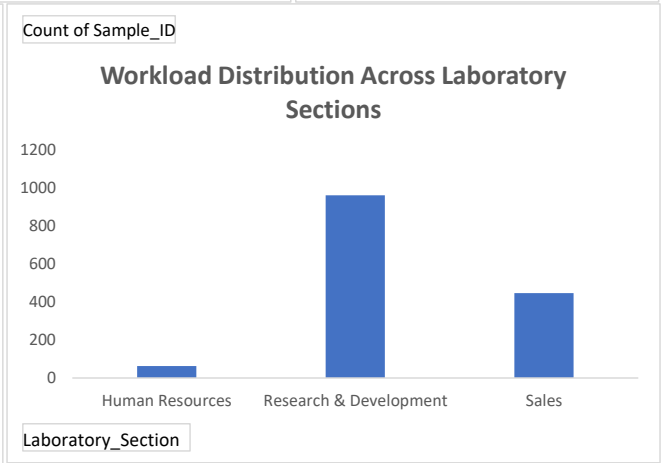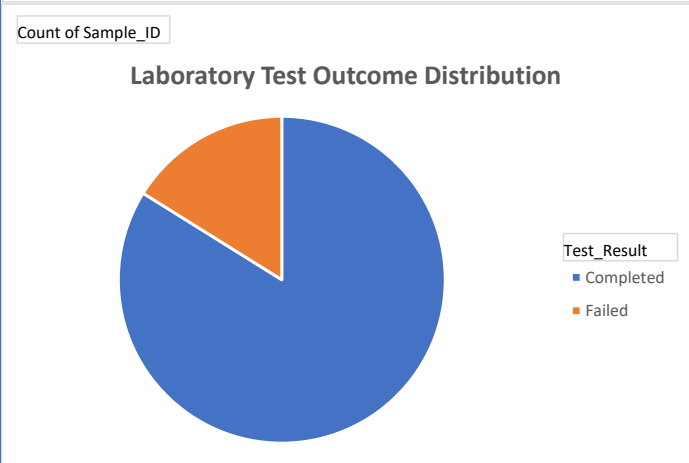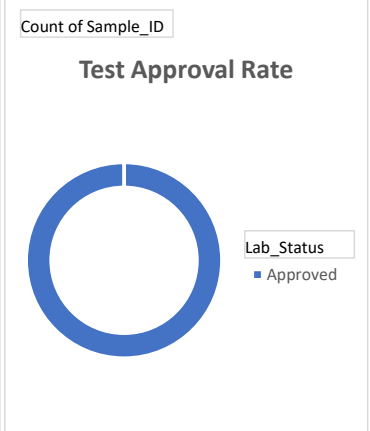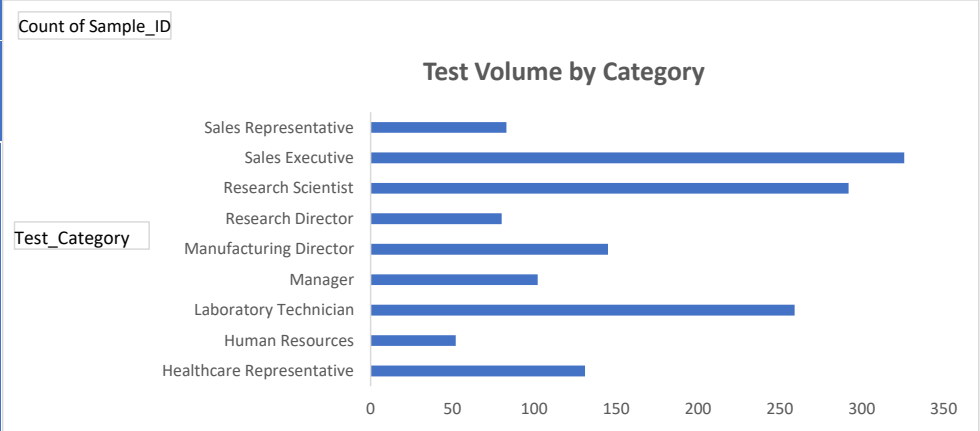

Key Insights

- The laboratory processed a total of **1,470 samples**, achieving a strong **84% completion rate**
- Only **16% of tests failed**, indicating effective laboratory processes
- The laboratory maintains an average processing time of **7 days**, showing efficient turnaround
- Research & Development handled the highest workload
- Overall laboratory performance reflects strong operational efficiency

Prepared by: Precious Amiekumo