


distribution of differences in mean accuracies (affine – original), sw_p=0.121, t_p=0.000

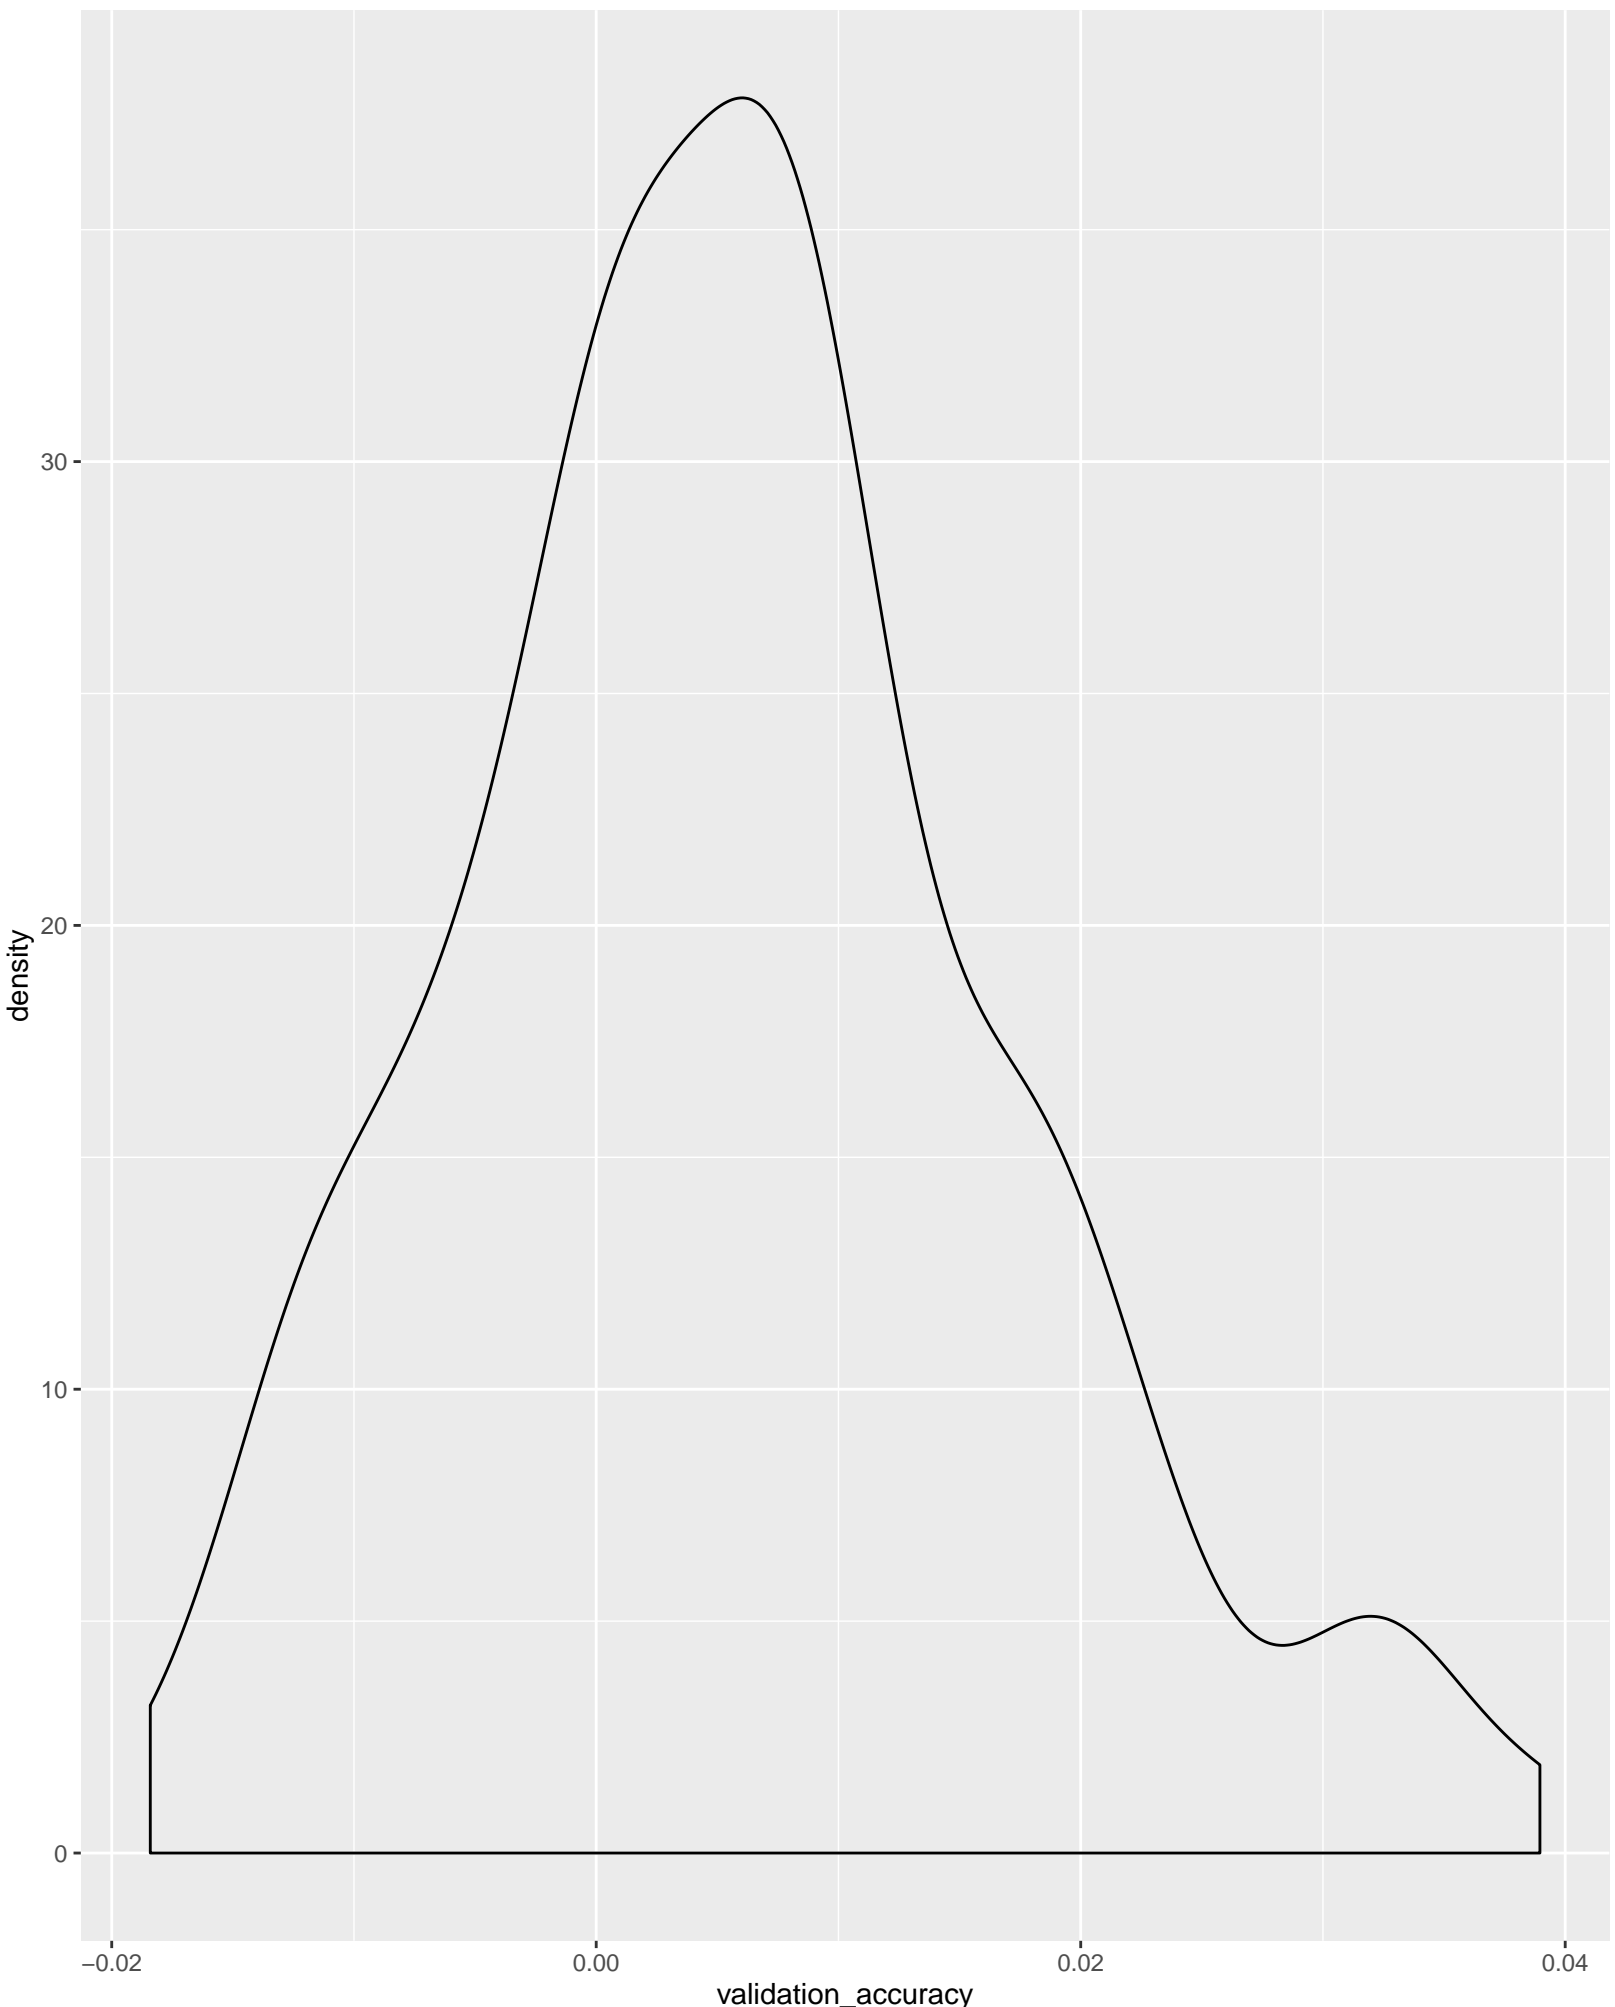

sw_p is p value for shapiro wilk test against normality; t_p is p value for right tailed one sample t test against zero mean