


distribution of differences in mean accuracies (affine – original), sw\_p=0.121, t\_p=0.000

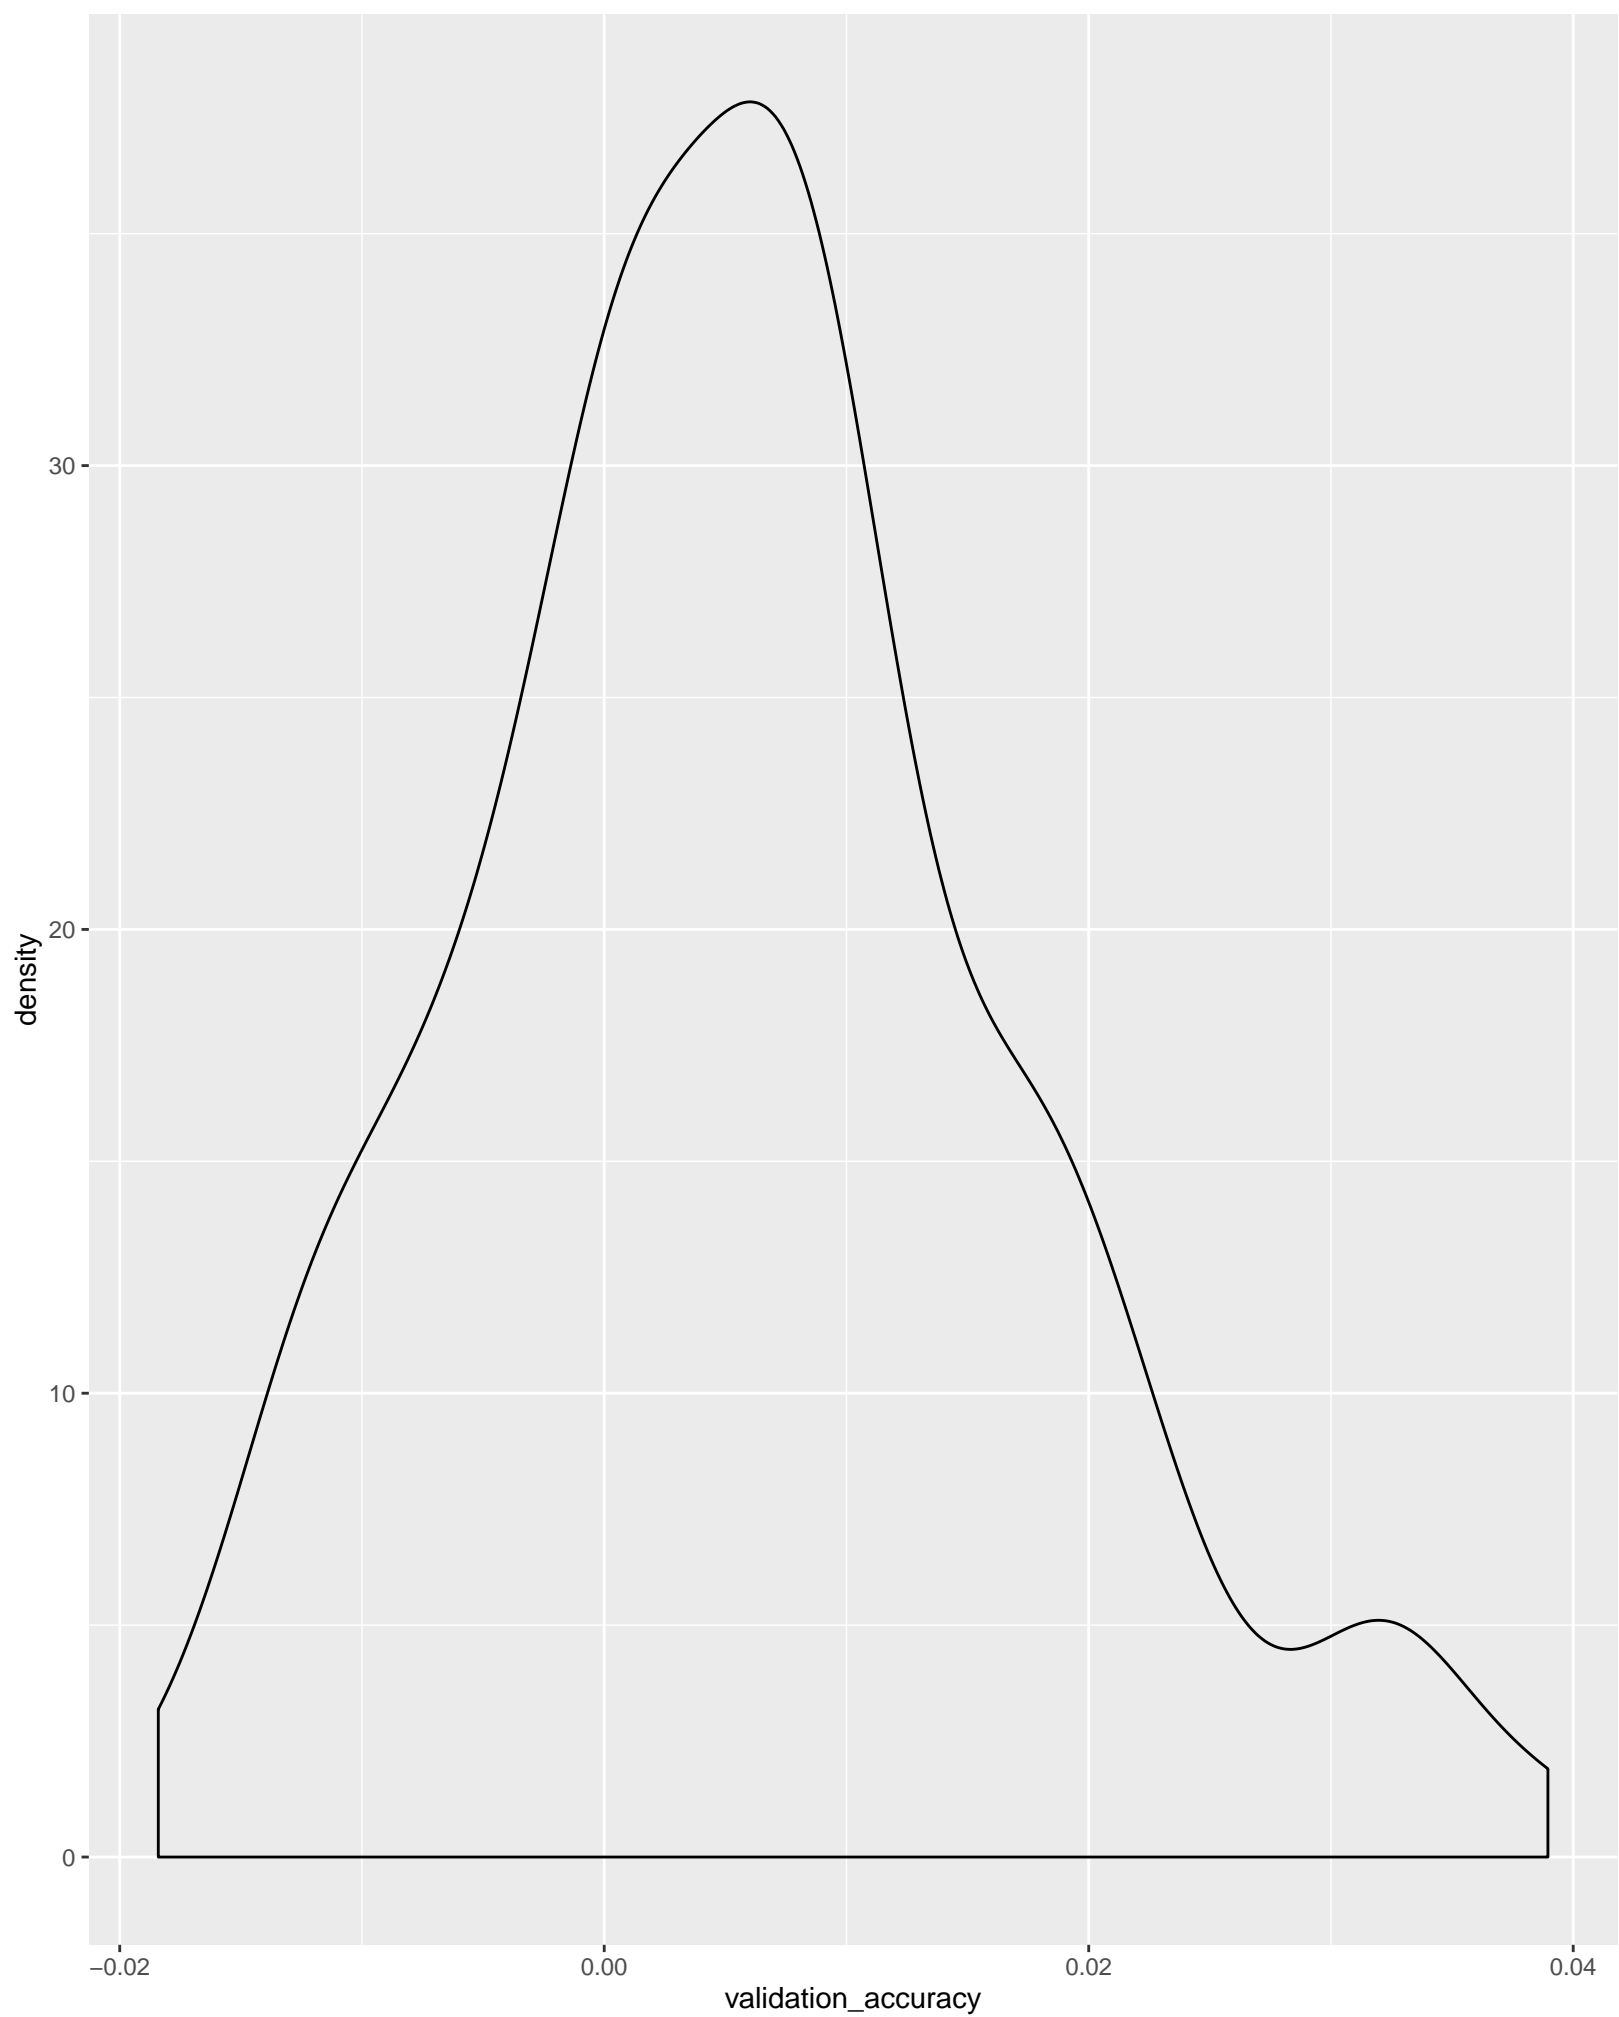

sw\_p is p value for shapiro wilk test against normality; t\_p is p value for right tailed one sample t test against 0.2% mean