Clinic block · header

CLINIC C LOGO

Clinic C

[Clinic address placeholder]
[Phone and e-mail placeholder]

Quantitative EEG and ERP report

Patient **Mock Patient 042**	Date of birth **1 Jan 2016**	Age **10 years**
Sex **female**	Recorded **15 Sep 2026**	Case code **MOCK-042**

Device block, locked · versions@1

Software	V4 mockup 0.1
Norms	Mock norms 2026.1 (synthetic)
Report	R-MOCK-042-01 · Version 1 · Draft, not issued

Device block, locked · summary@1

Summary

The largest marked deviations from the age norm in this measurement are: relative theta power, eyes open: Pz (z = -4.6), O1 (z = -4.0), O2 (z = -4.0); relative theta power, eyes closed: Pz (z = -4.4), O2 (z = -4.2), O1 (z = -4.0), P4 (z = -3.5), P3 (z = -3.2); SMR asymmetry index, eyes open: C3-C4 (z = 4.2); SMR asymmetry index, eyes closed: C3-C4 (z = 4.2); beta1 coherence, eyes closed: T5-O1 (z = 4.0), C3-T5 (z = 4.0), T5-P3 (z = 4.0), P3-O1 (z = 3.9), T3-T5 (z = 3.8), T3-C3 (z = 3.8), C3-P3 (z = 3.7); beta1 coherence, eyes open: T3-C3 (z = 3.9), C3-T5 (z = 3.9), T5-P3 (z = 3.8), P3-O1 (z = 3.8), C3-P3 (z = 3.7), T3-T5 (z = 3.7), T5-O1 (z = 3.6); P1 latency, Go: O1 (z = 3.7), O2 (z = 3.2); delta coherence, eyes closed: Cz-T6 (z = -3.5). SUM-2

This list ranks the marked values of these analyses by |z|: absolute and relative band power, maps per 1 Hz band, alpha peak frequency, theta/beta ratio, frontal alpha asymmetry index, asymmetry map, coherence per electrode pair, ERP peak amplitude and latency, and VCPT task results. It shows the 5 largest and every marked value of 3 z or more. Not ranked: the spectra per 0.5 Hz bin, which are shown as curves against the norm, and global coherence, which is still to be confirmed. SUM-RULE-2

Marked values in this measurement: band power 8 of 456, maps per 1 Hz band 0 of 1102, alpha peak and ratios 0 of 6, asymmetry map 2 of 96, coherence 15 of 2052, ERP peaks 2 of 21 and VCPT task 0 of 4. SUM-COUNT-1

Device block, locked · quality@1

Signal quality and processing

Eyes open: 164 of 180 seconds were analysed after artefact removal. Q-DUR-1

Eyes closed: 171 of 180 seconds were analysed after artefact removal. Q-DUR-1

VCPT: 1168 of 1220 seconds were analysed after artefact removal. Q-DUR-1

Accepted VCPT trials: Go 95, NoGo 92, Ignore 93, Novelty 95 (of 100 each). Q-TRIALS-1

Artefact removal changed by the clinician: component 6 (muscle, left temporal) was kept although the automatic cleaning proposed removing it; 2 of 19 components were removed. Q-ICA-MAN-1

Clinician block, editable · anamnesis

Anamnesis


Placeholder for the clinician's text. Written in the V4 report editor; the system does not write here.

Device block, locked · spectra.maps@1


Spectra and maps

Eyes open

Absolute power, z against the age norm



Relative power, z against the age norm




Relative theta power, eyes open, is below the age norm at Pz (z = -4.6), O1 (z = -4.0) and O2 (z = -4.0). SP-REL-1


The alpha peak frequency, eyes open, is 9.2 Hz and is not marked (z = 0.2). APF-IN-2

Eyes closed

Absolute power, z against the age norm

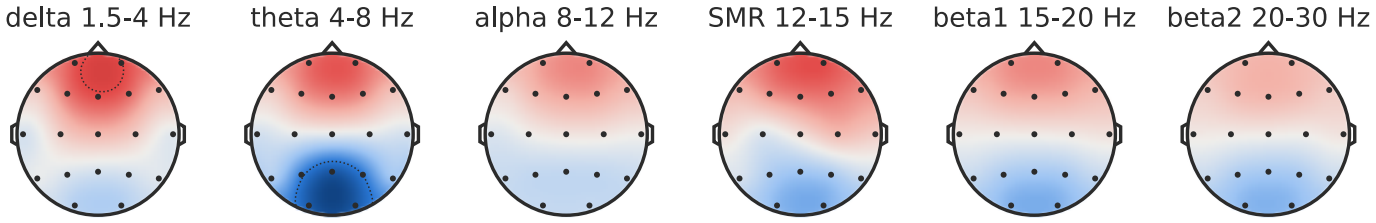


Relative power, z against the age norm

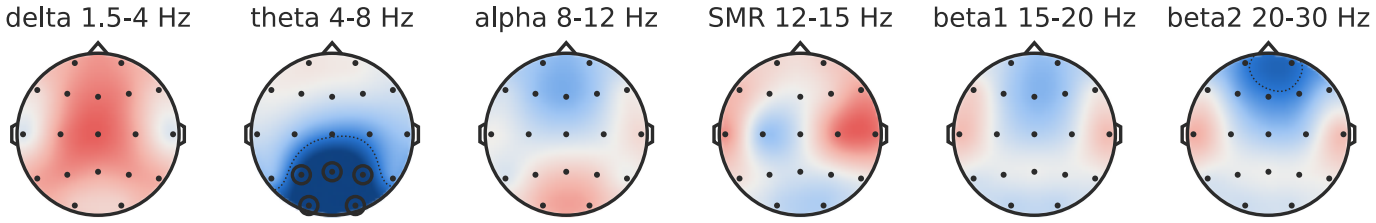

Relative theta power, eyes closed, is below the age norm at P3 (z = -3.2), Pz (z = -4.4), P4 (z = -3.5), O1 (z = -4.0) and O2 (z = -4.2). SP-REL-1

The alpha peak frequency, eyes closed, is 9.3 Hz and is not marked (z = 0.2). APF-IN-2

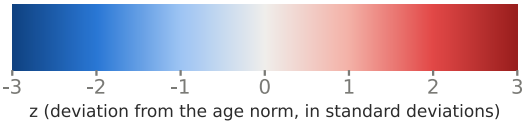

Clinician block, editable · comment.spectra

Clinician's comment

Placeholder for the clinician's text. Written in the V4 report editor; the system does not write here.

Device block, locked · limits@1

Notes on the results

The results are one input to the clinician's assessment. The software does not diagnose and does not recommend treatment. L-AID-1

z is the distance of a value from the normative mean, in standard deviations of the normative sample; about 95% of the normative sample lies between z = -2 and z = 2. L-Z-1

Marked values differ from the age norm after correction for multiple comparisons, which keeps chance results among the many comparisons rare; a value beyond 2 z that is not marked may deviate by chance alone. The method of correction is still to be chosen. L-MC-1

The earlier measurement of 12 Mar 2026 was processed again with the current software and norms (V4 mockup 0.1; Mock norms 2026.1 (synthetic)). L-REPROC-1

Measurements are shown side by side, each against its own age norm; differences between them are not tested for statistical significance. L-SIDE-1