Clinic block · header

CLINIC C LOGO

Clinic C

[Clinic address placeholder]

[Phone and e-mail placeholder]

Quantitative EEG and ERP report

Patient **Mock Patient 042**	Date of birth **1 Jan 2016**	Age **10 years**
Sex **female**	Recorded **15 Sep 2026**	Case code **MOCK-042**

Device block, locked · versions@1

Software	V4 mockup 0.1
Norms	Mock norms 2026.1 (synthetic)
Report	R-MOCK-042-01 · Version 1 · Draft, not issued

Device block, locked · summary@1

Summary

The largest deviations from the age norm in this measurement are: theta coherence Fp2-F8, eyes closed (z = 3.0); theta coherence Fp2-F3, eyes closed (z = 2.9); relative SMR power at Fz, eyes closed (z = -2.6); absolute theta power at Fz, eyes closed (z = 2.6); theta coherence F3-F4, eyes open (z = 2.5). SUM-1

This list ranks every measure compared with a norm by |z| and shows the 5 largest deviations and every deviation of 3 z or more. SUM-RULE-1

Device block, locked · quality@1

Signal quality and processing

Eyes open: 164 of 180 seconds were analysed after artefact removal. Q-DUR-1

Eyes closed: 171 of 180 seconds were analysed after artefact removal. Q-DUR-1

VCPT: 1168 of 1220 seconds were analysed after artefact removal. Q-DUR-1

Accepted VCPT trials: Go 92, NoGo 93, Ignore 93, Novelty 95 (of 100 each). Q-TRIALS-1

Artefact removal changed by the clinician: component 6 (muscle, left temporal) was kept although the automatic cleaning proposed removing it; 2 of 19 components were removed. Q-ICA-MAN-1

Clinician block, editable · anamnesis

Anamnesis


Placeholder for the clinician's text. Written in the V4 report editor; the system does not write here.

Device block, locked · spectra.maps@1


Spectra and maps

Eyes open

Absolute power, z against the age norm

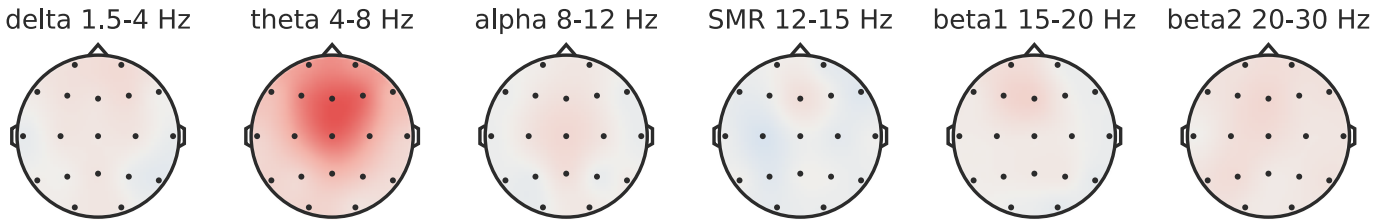

Relative power, z against the age norm

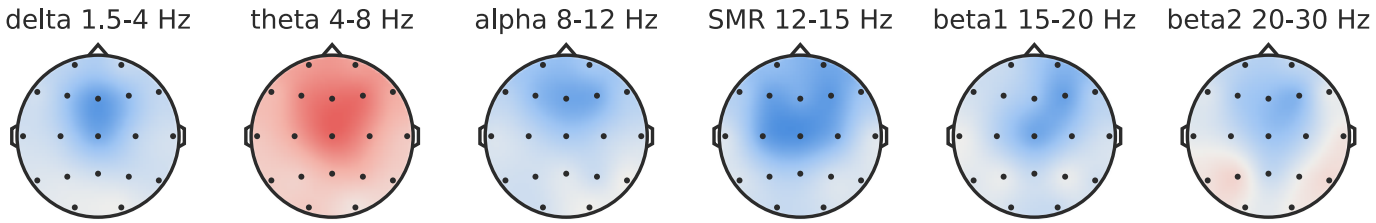


All absolute and relative band power values, eyes open, are within 2 z of the normative mean. SP-NONE-1


The alpha peak frequency, eyes open, is 8.9 Hz, within 2 z of the normative mean (z = -0.4). APF-IN-1

Eyes closed

Absolute power, z against the age norm

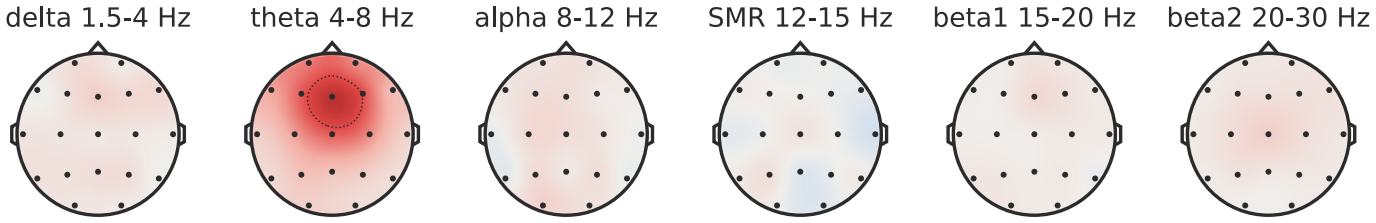

Relative power, z against the age norm

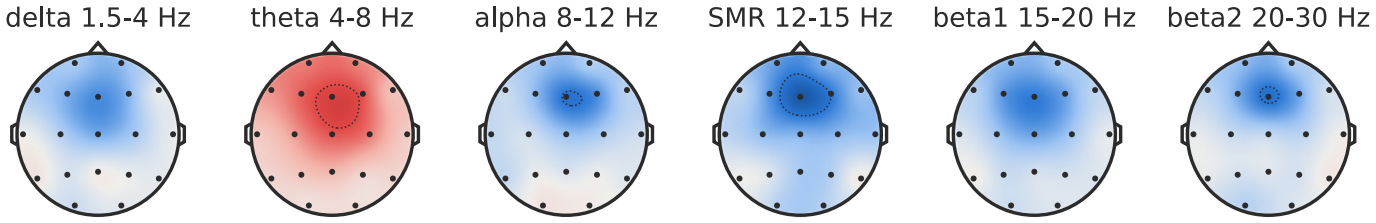

Absolute theta power, eyes closed, is above the age norm at Fz (z = 2.6) and F4 (z = 2.0). SP-ABS-1

Relative theta power, eyes closed, is above the age norm at Fz (z = 2.2). SP-REL-1


Relative alpha power, eyes closed, is below the age norm at Fz (z = -2.1). SP-REL-1

Relative SMR power, eyes closed, is below the age norm at Fz (z = -2.6) and F4 (z = -2.0). SP-REL-1

Relative beta1 power, eyes closed, is below the age norm at Fz (z = -2.0). SP-REL-1

Relative beta2 power, eyes closed, is below the age norm at Fz (z = -2.2). SP-REL-1

The alpha peak frequency, eyes closed, is 9.0 Hz, within 2 z of the normative mean (z = -0.4). APF-IN-1

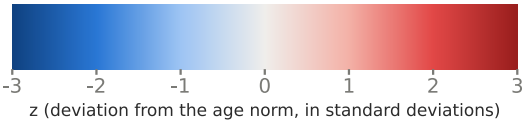

Clinician block, editable · comment.spectra

Clinician's comment

Placeholder for the clinician's text. Written in the V4 report editor; the system does not write here.

Device block, locked · limits@1

Notes on the results

The results are one input to the clinician's assessment. The software does not diagnose and does not recommend treatment. L-AID-1

z is the distance of a value from the normative mean, in standard deviations of the normative sample; about 95% of the normative sample lies between z = -2 and z = 2. L-Z-1

A deviation from the norm is statistical: among many measures, some deviate by chance alone. L-CHANCE-1

The earlier measurement of 12 Mar 2026 was processed again with the current software and norms (V4 mockup 0.1; Mock norms 2026.1 (synthetic)). L-REPROC-1

Measurements are shown side by side, each against its own age norm; differences between them are not tested for statistical significance. L-SIDE-1