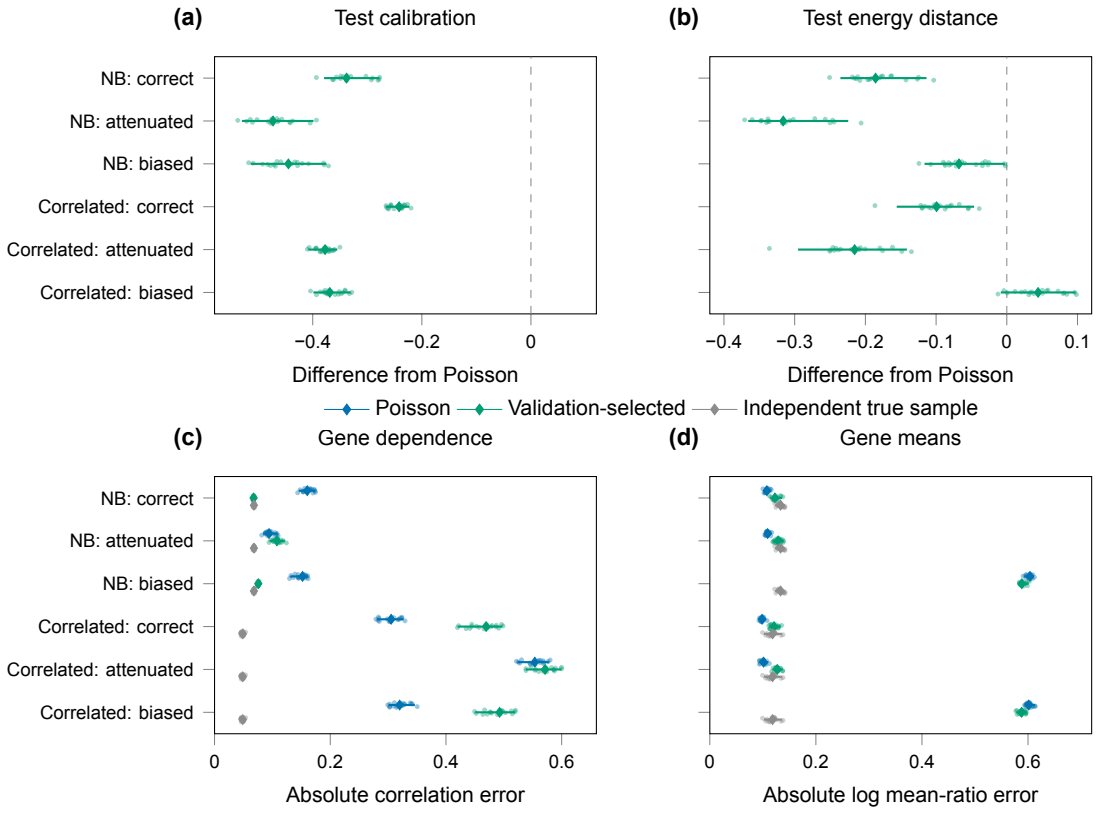

(a)
Test calibration
NB: correct
NB: attenuated
NB: biased
Correlated: correct
Correlated: attenuated
Correlated: biased
−0.4
−0.2
0
Difference from Poisson
(b)
Test energy distance
−0.4
−0.3
−0.2
−0.1
0
0.1
Difference from Poisson
Poisson
Validation-selected
Independent true sample
(c)
Gene dependence
NB: correct
NB: attenuated
NB: biased
Correlated: correct
Correlated: attenuated
Correlated: biased
0
0.2
0.4
0.6
Absolute correlation error
(d)
Gene means
0
0.2
0.4
0.6
Absolute log mean-ratio error